


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE080416\
 Data File : BE092183.D
 Acq On : 4 Aug 2016 15:25
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-PAH-BE080216.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 02 16:59:37 2016

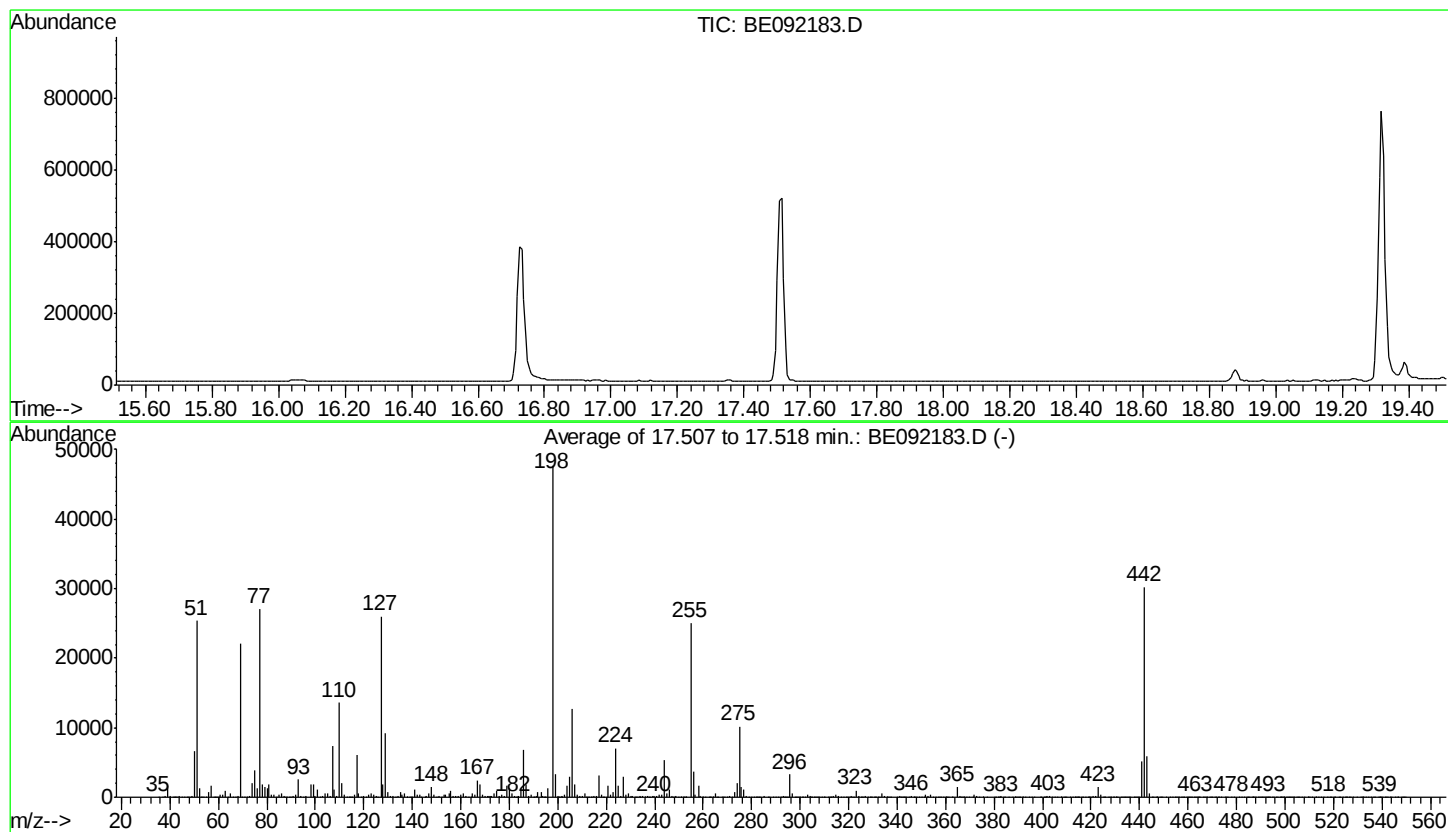

AutoFind: Scans 2539, 2540, 2541; Background Corrected with Scan 2530

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.2	25373	PASS
68	69	0.00	2	1.1	240	PASS
69	198	0.00	100	46.4	22142	PASS
70	69	0.00	2	0.3	72	PASS
127	198	10	80	54.6	26043	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	47692	PASS
199	198	5	9	7.0	3357	PASS
275	198	10	60	21.4	10217	PASS
365	198	1	100	3.1	1486	PASS
441	442	0.01	24	17.0	5127	PASS
442	198	50	100	63.3	30197	PASS
443	442	15	24	19.3	5828	PASS