

Data Path : Z:\HPCHEM1\BNA E\DATA\BE080515\
 Data File : BE090372.D
 Acq On : 5 Aug 2015 22:55
 Operator : TP/UM
 Sample : G3180-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 080315-D506-F-D-B

Quant Time: Aug 06 13:07:15 2015
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE080515.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 06 02:22:05 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	20539	5.00	ng	0.00
6) Naphthalene-d8	10.34	136	90117	5.00	ng	0.00
12) Acenaphthene-d10	14.20	164	54556	5.00	ng	0.00
18) Phenanthrene-d10	16.94	188	119535	5.00	ng	0.00
25) Chrysene-d12	21.10	240	147368	5.00	ng	0.00
32) Perylene-d12	23.40	264	137563	5.00	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.21	112	9819	2.72	ng	0.00
5) Phenol-d6	6.77	99	8623	1.50	ng	0.00
7) Nitrobenzene-d5	8.73	82	25374	3.52	ng	0.00
13) 2,4,6-Tribromophenol	15.71	330	12162	7.51	ng	0.00
14) 2-Fluorobiphenyl	12.82	172	67990	4.53	ng	0.00
27) Terphenyl-d14	19.56	244	132451	6.10	ng	0.00
Target Compounds						
30) Bis(2-ethylhexyl)phthalate	21.03	149	1808	0.34	ng	Qvalue # 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE080515\
Data File : BE090372.D
Acq On : 5 Aug 2015 22:55
Operator : TP/UM
Sample : G3180-03
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
080315-D506-F-D-B

Quant Time: Aug 06 13:07:15 2015
Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE080515.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 06 02:22:05 2015
Response via : Initial Calibration

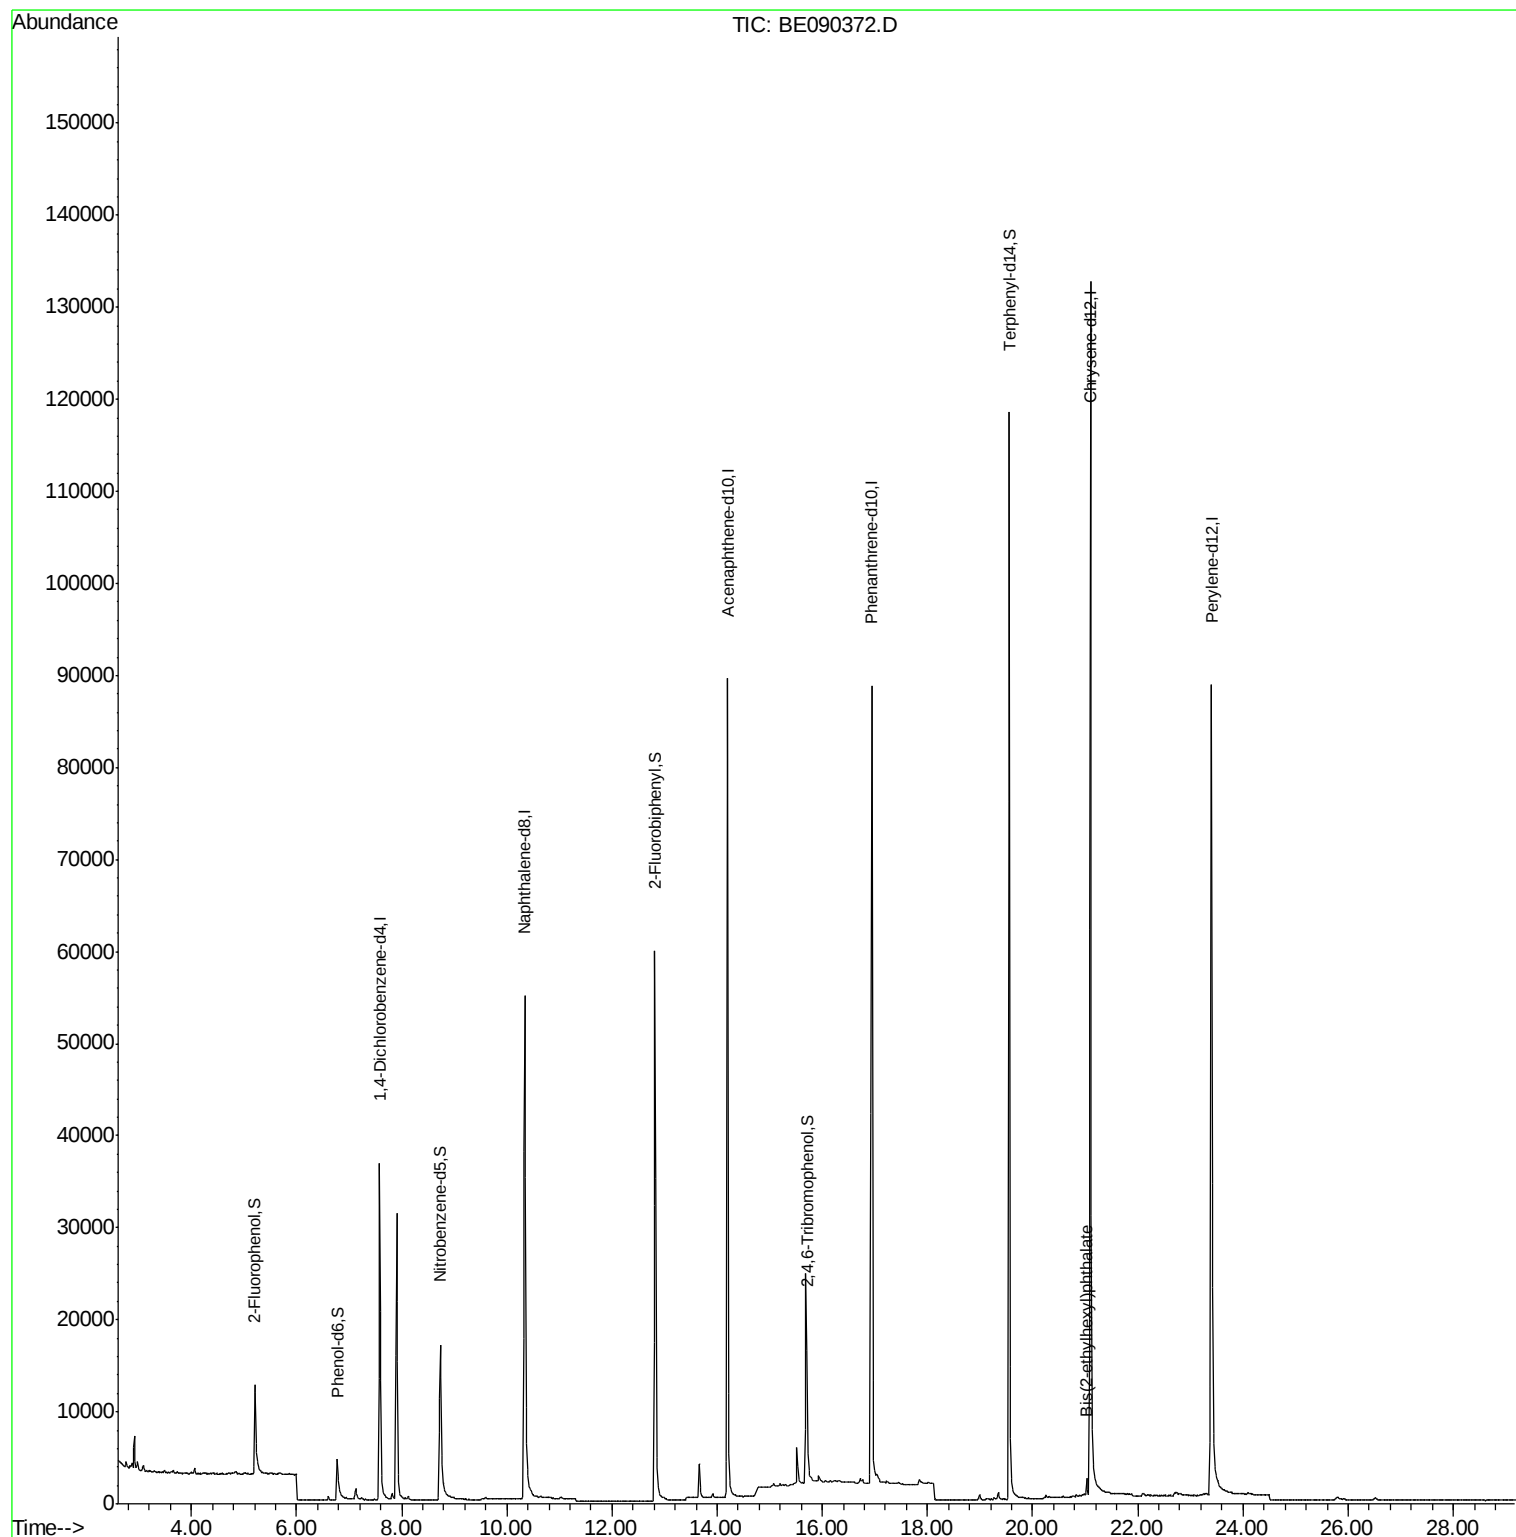



#1

1,4-Dichlorobenzene-d4

Concen: 5.00 ng

RT: 7.59 min Scan# 846

Delta R.T. -0.00 min

Lab File: BE090372.D

Acq: 5 Aug 2015 22:55

Instrument :

BNA_E

ClientSampleId :

080315-D506-F-D-B


Tot Ion:152 Resp: 20539

Ion Ratio Lower Upper

152 100

150 152.9 123.0 184.4




115 61.2 48.9 73.3

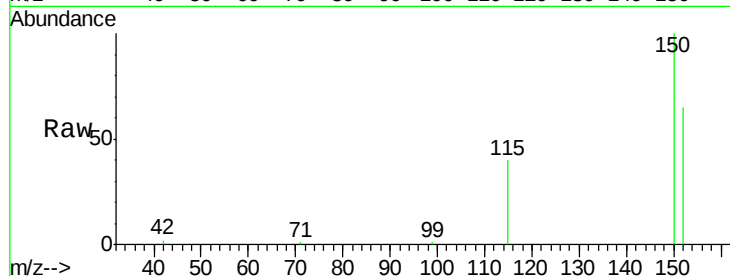

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

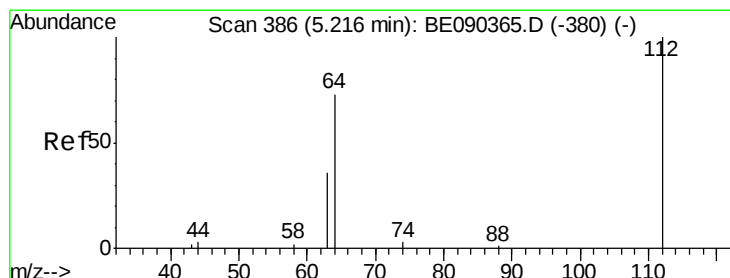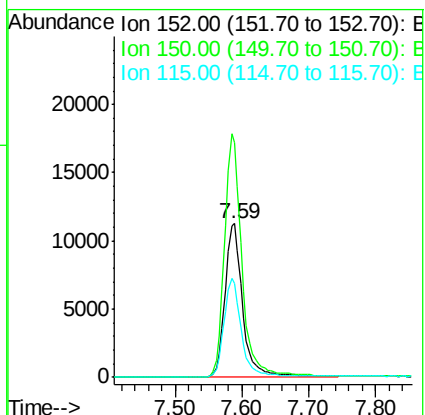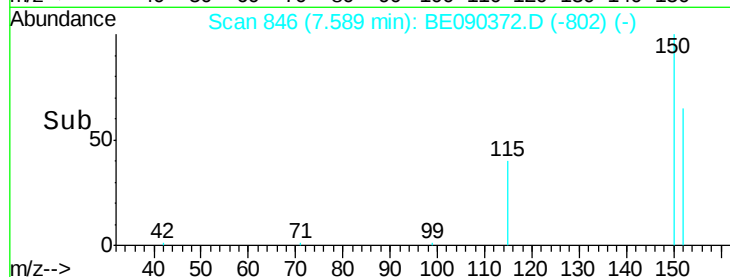

#4

2-Fluorophenol

Concen: 2.72 ng

RT: 5.21 min Scan# 385

Delta R.T. -0.00 min

Lab File: BE090372.D

Acq: 5 Aug 2015 22:55


Tgt Ion:112 Resp: 9819

Ion Ratio Lower Upper

112 100

64 71.1 37.1 55.7#



63 36.4 19.5 29.3#

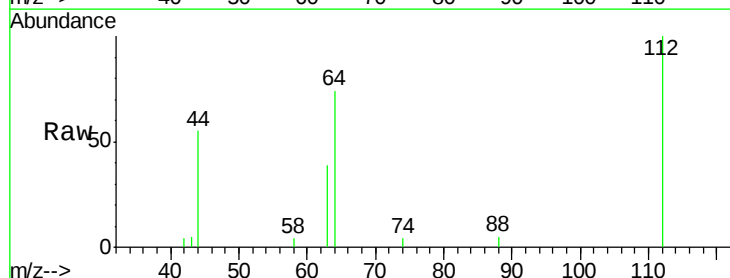

Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

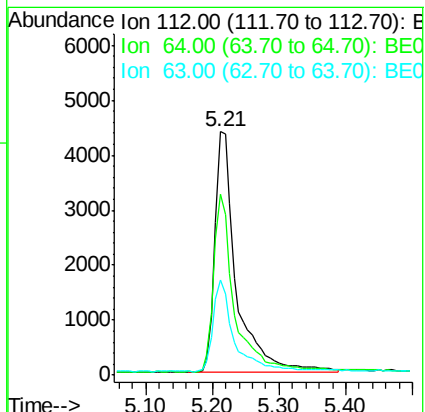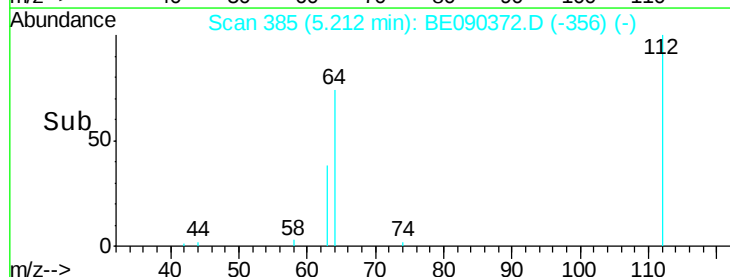



#5

Phenol-d6

Concen: 1.50 ng

RT: 6.77 min Scan# 667

Delta R.T. -0.00 min

Lab File: BE090372.D

Acq: 5 Aug 2015 22:55

Instrument :

BNA_E

ClientSampleId :

080315-D506-F-D-B


Tot Ion: 99 Resp: 8623

Ion Ratio Lower Upper




99 100

42 21.5 18.2 27.4

71 35.7 27.4 41.0

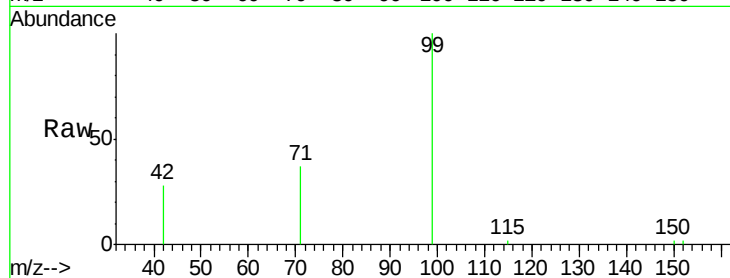

Abundance Ion 99.00 (98.70 to 99.70): BE0
Ion 42.00 (41.70 to 42.70): BE0
Ion 71.00 (70.70 to 71.70): BE0

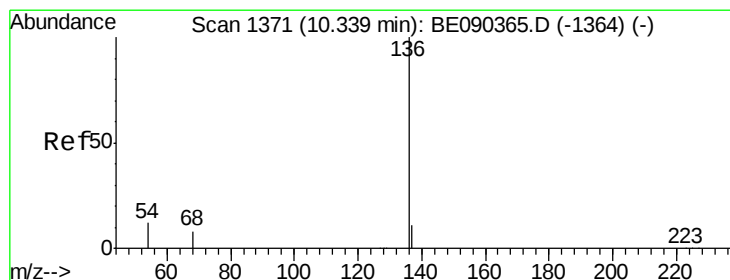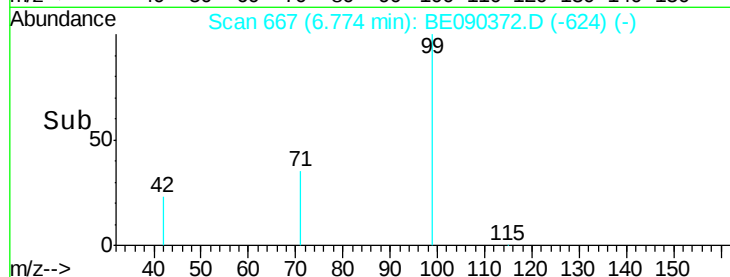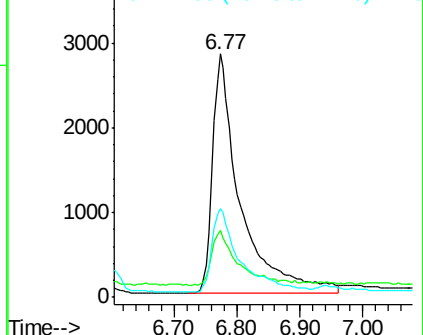

#6

Naphthalene-d8

Concen: 5.00 ng

RT: 10.34 min Scan# 1371

Delta R.T. 0.00 min

Lab File: BE090372.D

Acq: 5 Aug 2015 22:55

Tgt Ion: 136 Resp: 90117


Ion Ratio Lower Upper

136 100



137 10.9 8.7 13.1


54 12.3 9.4 14.0

68 8.5 6.5 9.7

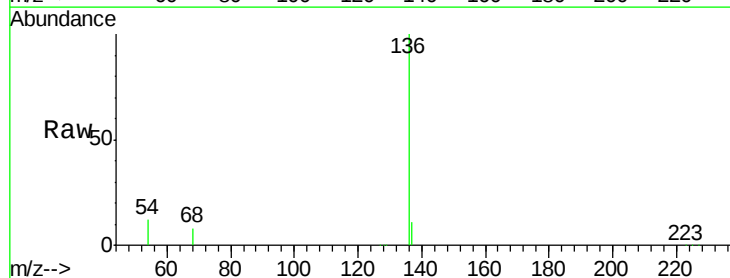

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BE0
Ion 68.00 (67.70 to 68.70): BE0

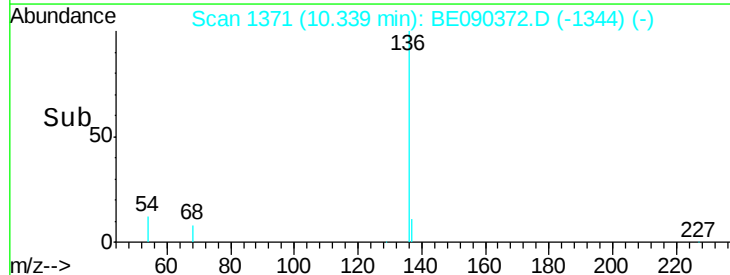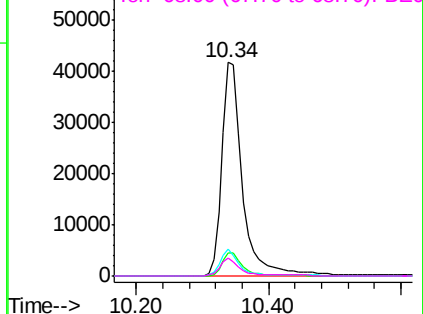

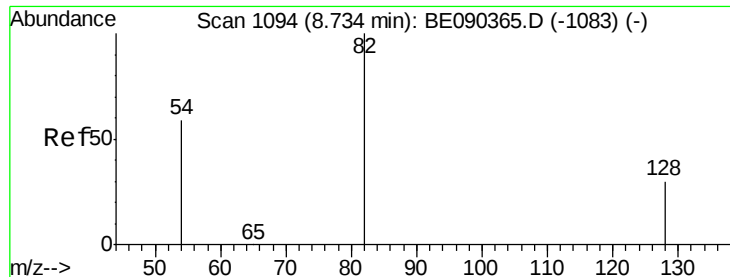

#7

Nitrobenzene-d5

Concen: 3.52 ng

RT: 8.73 min Scan# 1094

Delta R.T. 0.00 min

Lab File: BE090372.D

Acq: 5 Aug 2015 22:55

Instrument :

BNA_E

ClientSampleId :

080315-D506-F-D-B


Tot Ion: 82 Resp: 25374

Ion Ratio Lower Upper




82 100

128 31.2 25.0 37.6

54 59.0 48.8 73.2

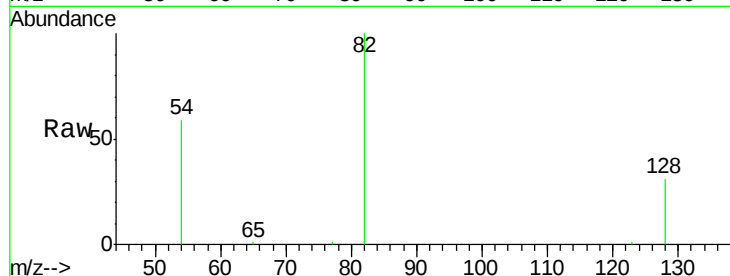

Abundance Ion 82.00 (81.70 to 82.70): BE0
Ion 128.00 (127.70 to 128.70): BE0
Ion 54.00 (53.70 to 54.70): BE0

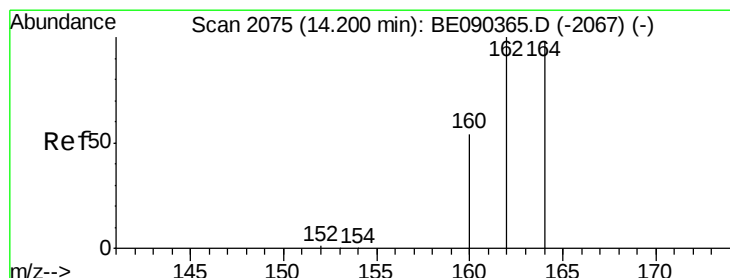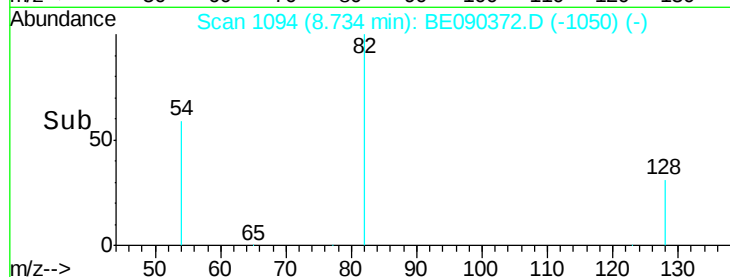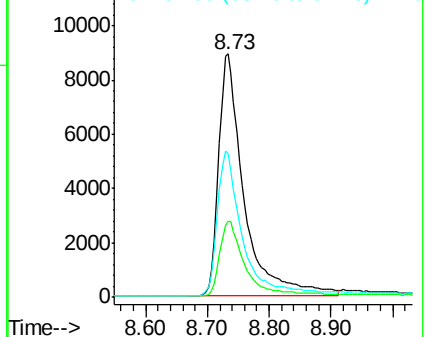

#12

Acenaphthene-d10

Concen: 5.00 ng

RT: 14.20 min Scan# 2076

Delta R.T. 0.00 min

Lab File: BE090372.D

Acq: 5 Aug 2015 22:55


Tgt Ion: 164 Resp: 54556

Ion Ratio Lower Upper



164 100

162 98.9 81.8 122.8

160 49.3 44.2 66.4

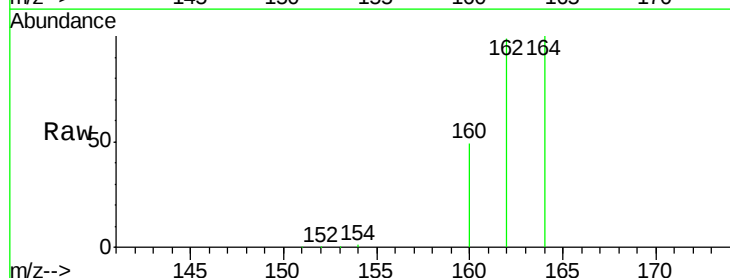

Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

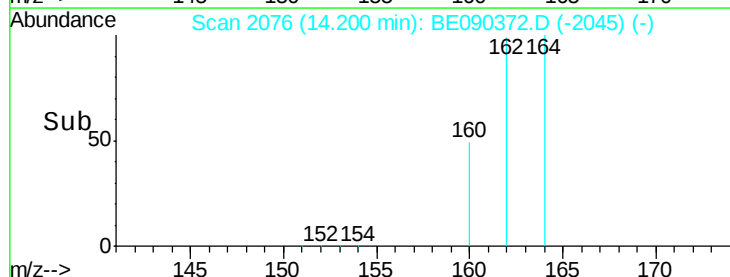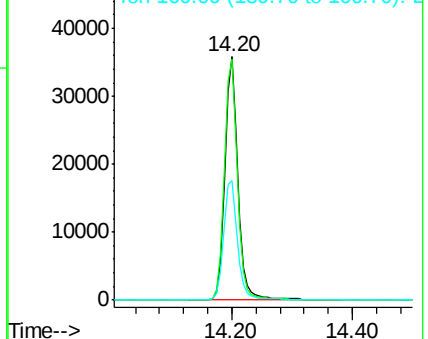







#13
 2,4,6-Tribromophenol
 Concen: 7.51 ng
 RT: 15.71 min Scan# 2207
 Delta R.T. 0.00 min
 Lab File: BE090372.D
 Acq: 5 Aug 2015 22:55

Instrument :
 BNA_E
 ClientSampleId :
 080315-D506-F-D-B

Tot Ion:330 Resp: 12162
 Ion Ratio Lower Upper
 330 100
 332 96.7 75.8 113.6
 141 155.9 114.4 171.6

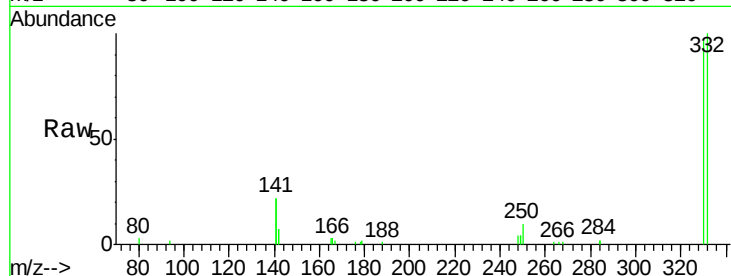


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

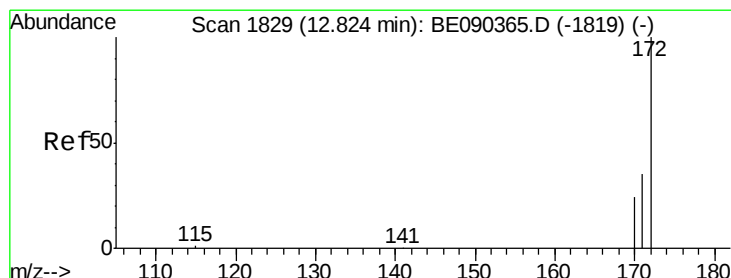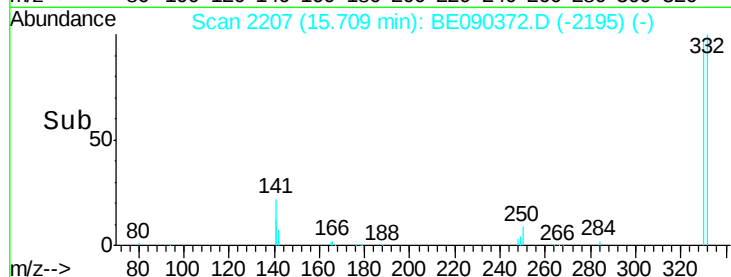
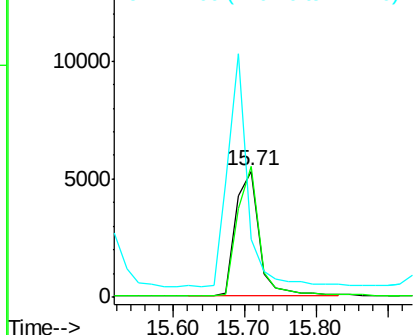


#14
 2-Fluorobiphenyl
 Concen: 4.53 ng
 RT: 12.82 min Scan# 1828
 Delta R.T. -0.01 min
 Lab File: BE090372.D
 Acq: 5 Aug 2015 22:55

Tgt Ion:172 Resp: 67990
 Ion Ratio Lower Upper
 172 100
 171 35.2 28.5 42.7
 170 24.1 19.8 29.8

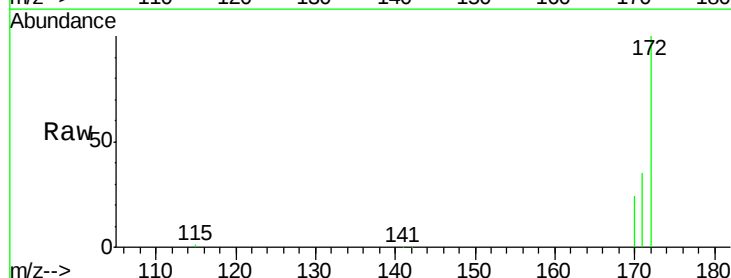

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

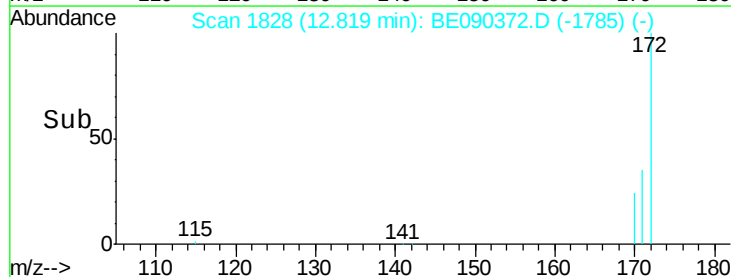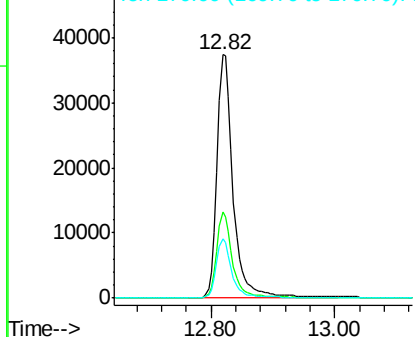



#18

Phenanthrene-d10

Concen: 5.00 ng

RT: 16.94 min Scan# 2278

Delta R.T. 0.00 min

Lab File: BE090372.D

Acq: 5 Aug 2015 22:55

Instrument :

BNA_E

ClientSampleId :

080315-D506-F-D-B





Tot Ion:188 Resp: 119535

Ion Ratio Lower Upper

188 100

94 7.0 5.7 8.5

80 7.2 5.8 8.8

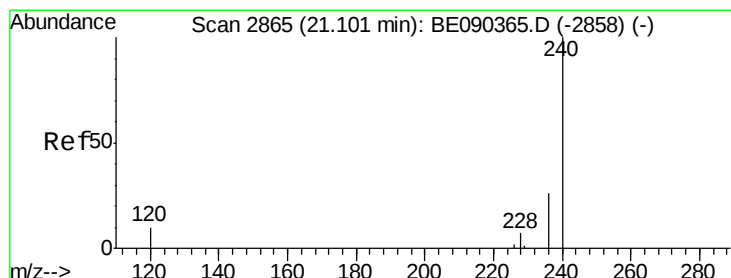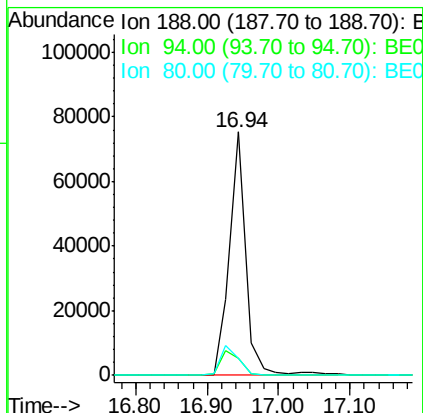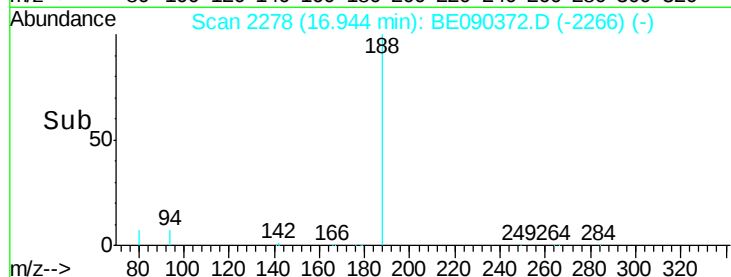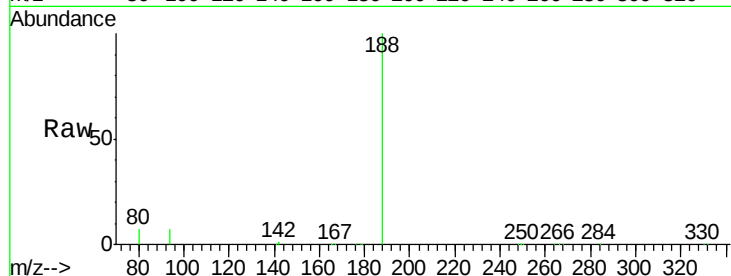

#25

Chrysene-d12

Concen: 5.00 ng

RT: 21.10 min Scan# 2866

Delta R.T. -0.00 min

Lab File: BE090372.D

Acq: 5 Aug 2015 22:55




Tgt Ion:240 Resp: 147368

Ion Ratio Lower Upper

240 100

120 9.8 8.3 12.5

236 26.3 21.0 31.4

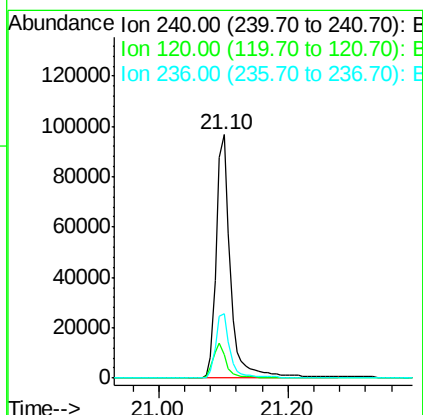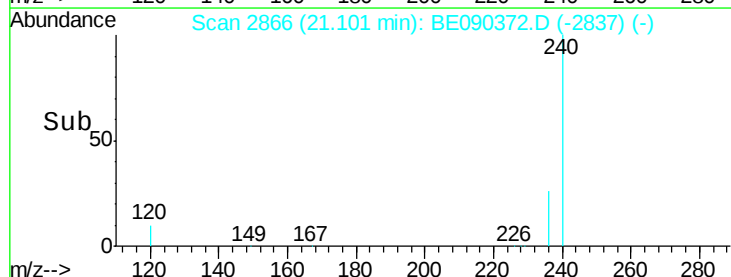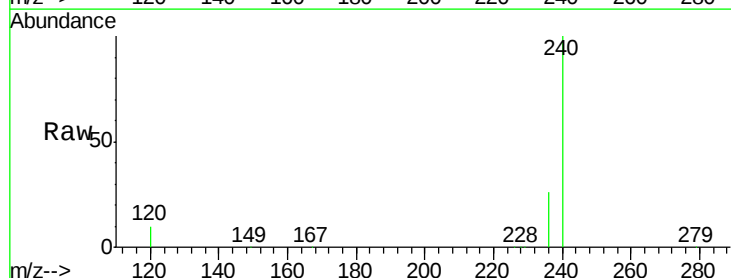



#27

Terphenyl-d14

Concen: 6.10 ng

RT: 19.56 min Scan# 2615

Delta R.T. -0.01 min

Lab File: BE090372.D

Acq: 5 Aug 2015 22:55

Instrument :

BNA_E

ClientSampleId :

080315-D506-F-D-B


Tot Ion:244 Resp: 132451

Ion Ratio Lower Upper

244 100

212 7.9 6.6 9.8




122 11.6 10.2 15.4

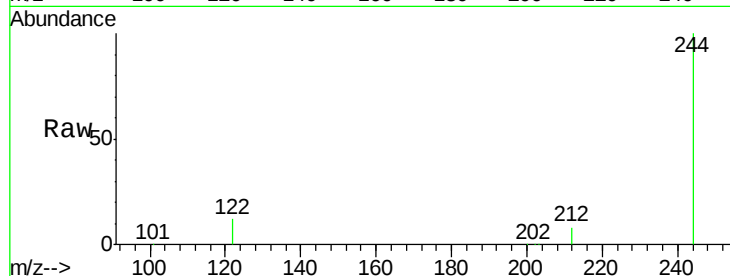

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

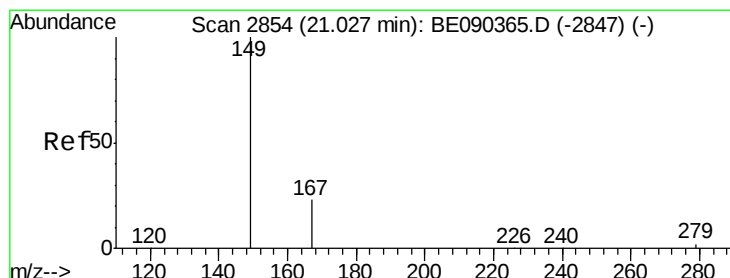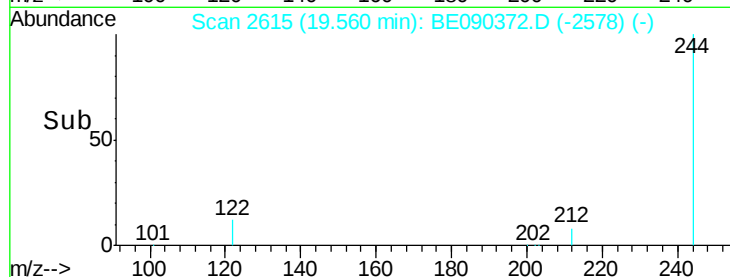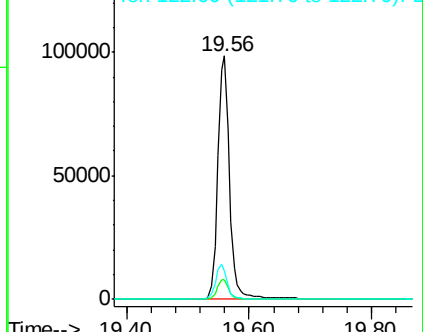

#30

Bis(2-ethylhexyl)phthalate

Concen: 0.34 ng

RT: 21.03 min Scan# 2855

Delta R.T. 0.00 min

Lab File: BE090372.D

Acq: 5 Aug 2015 22:55


Tgt Ion:149 Resp: 1808

Ion Ratio Lower Upper

149 100

167 25.1 19.8 29.8



279 3.8 2.4 3.6#

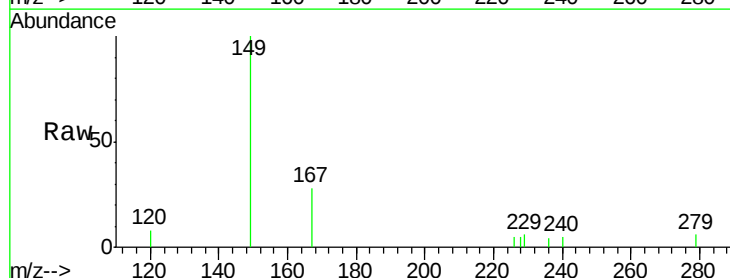


Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

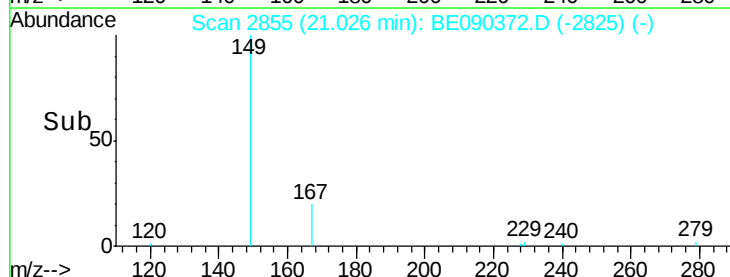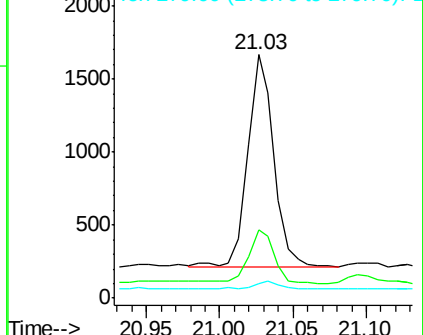

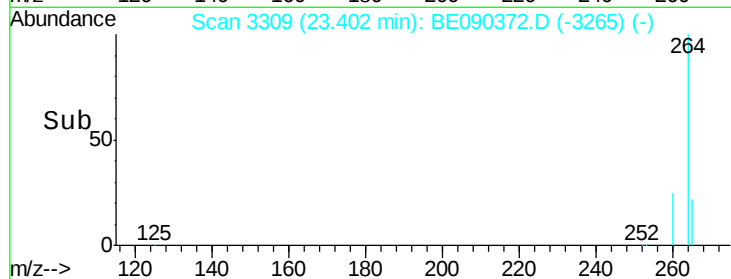

#32
 Pervlene-d12
 Concen: 5.00 ng
 RT: 23.40 min Scan# 3309
 Delta R.T. 0.00 min
 Lab File: BE090372.D
 Acq: 5 Aug 2015 22:55

Instrument :
 BNA_E
 ClientSampleId :
 080315-D506-F-D-B

Tot Ion	Ratio	Lower	Upper
264	100		
260	25.0	20.1	30.1
265	22.2	17.2	25.8

