


Data Path : Z:\HPCHEM1\BNA E\DATA\BE080515\
Data File : BE090377.D
Acq On : 6 Aug 2015 5:32
Operator : TP/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP1

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE080515.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Aug 06 12:28:08 2015

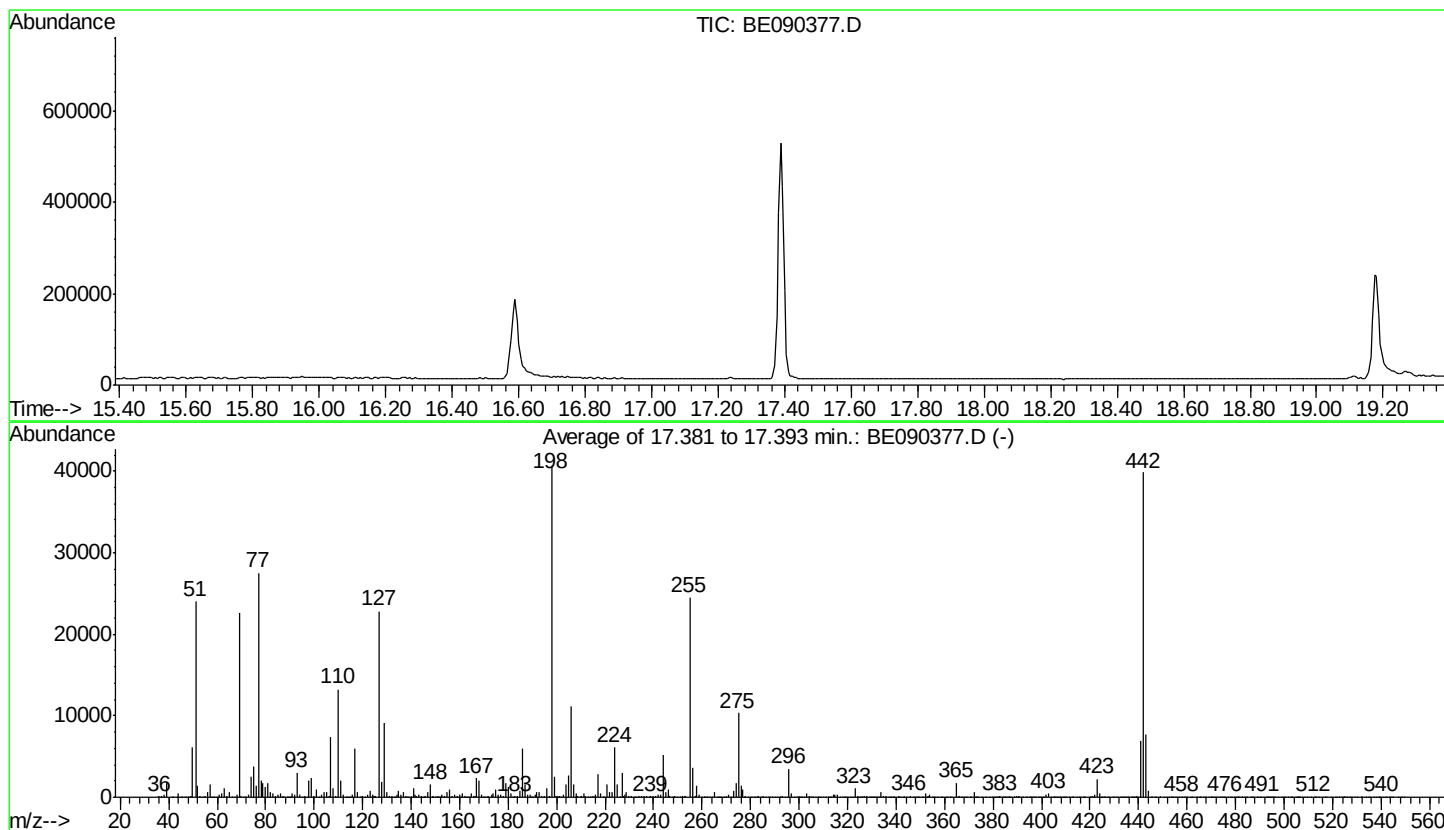

AutoFind: Scans 2518, 2519, 2520; Background Corrected with Scan 2509

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	59.0	24005	PASS
68	69	0.00	2	1.2	265	PASS
69	198	0.00	100	55.7	22649	PASS
70	69	0.00	2	0.5	107	PASS
127	198	10	80	56.2	22845	PASS
197	198	0.00	2	0.5	202	PASS
198	198	100	100	100.0	40673	PASS
199	198	5	9	6.2	2538	PASS
275	198	10	60	25.3	10297	PASS
365	198	1	100	4.3	1754	PASS
441	442	0.01	24	17.3	6912	PASS
442	198	50	100	98.1	39898	PASS
443	442	15	24	19.3	7720	PASS