


Data Path : Z:\HPCHEM1\BNA E\DATA\BE080515\
 Data File : Be090360.d
 Acq On : 5 Aug 2015 15:33
 Operator : TP/UM
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE080515.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 06 12:28:08 2015

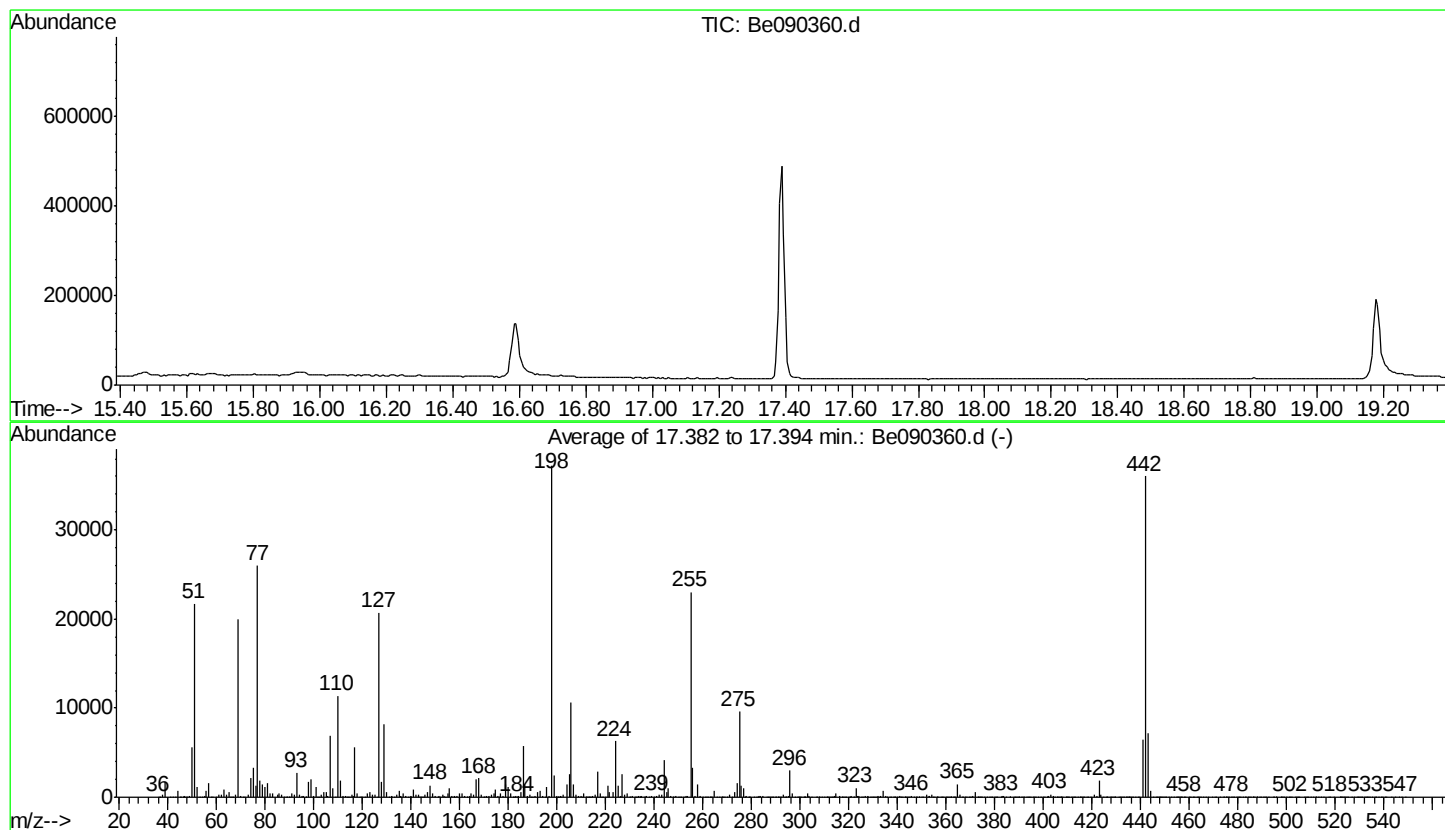

AutoFind: Scans 2518, 2519, 2520; Background Corrected with Scan 2510

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	58.3	21697	PASS
68	69	0.00	2	1.8	363	PASS
69	198	0.00	100	53.7	19999	PASS
70	69	0.00	2	0.5	94	PASS
127	198	10	80	55.7	20726	PASS
197	198	0.00	2	0.6	210	PASS
198	198	100	100	100.0	37215	PASS
199	198	5	9	6.7	2480	PASS
275	198	10	60	25.8	9585	PASS
365	198	1	100	3.9	1446	PASS
441	442	0.01	24	18.0	6478	PASS
442	198	50	100	96.8	36041	PASS
443	442	15	24	19.9	7177	PASS