
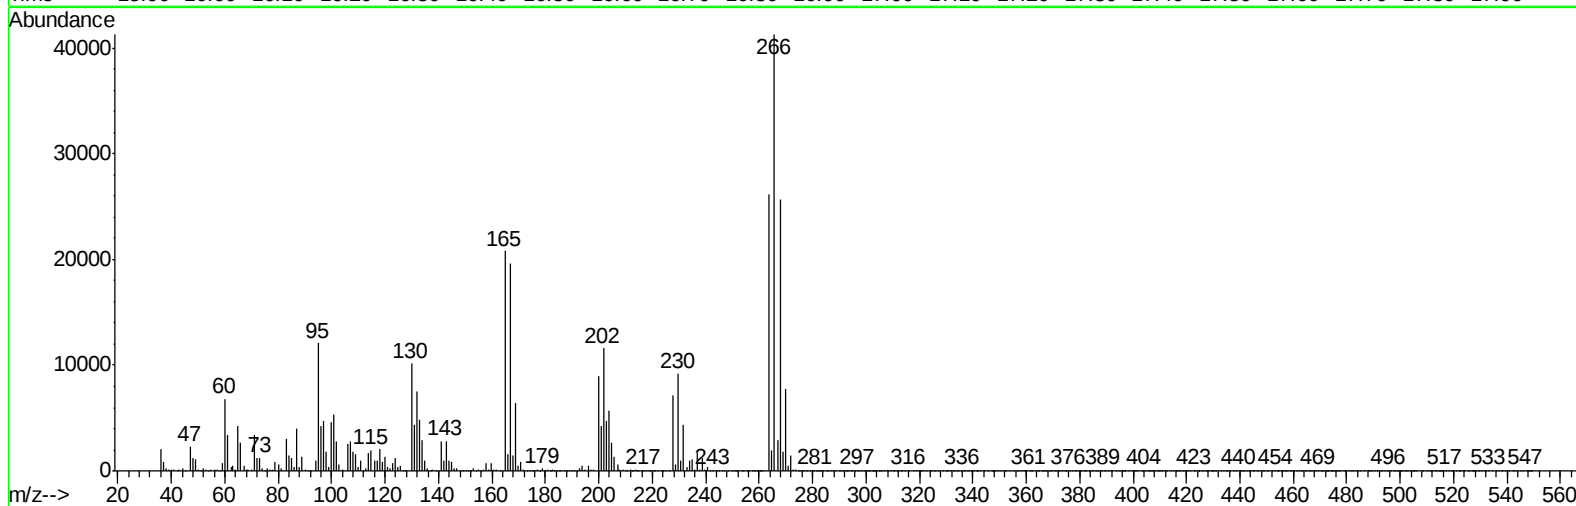


Data Path : Z:\HPCHEM1\BNA_E\Data\BE080517\
Data File : BE093671.D
Acq On : 5 Aug 2017 9:20
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 07 18:07:55 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE080117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 02 10:58:31 2017
Response via : Initial Calibration

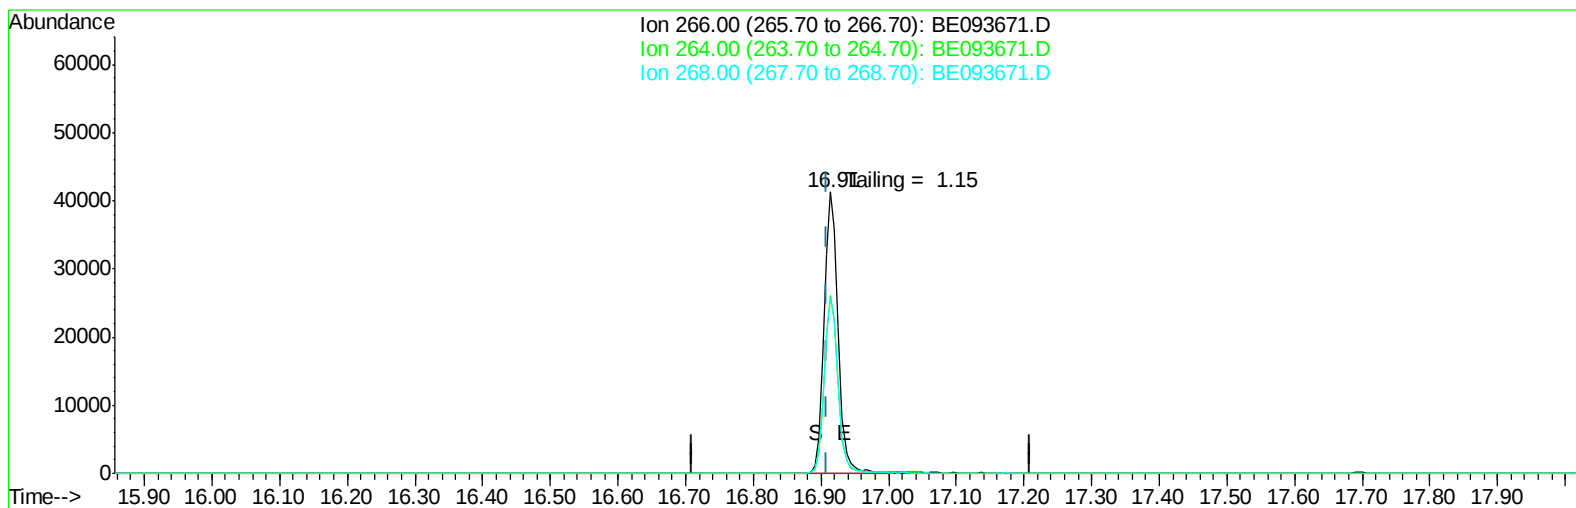

TIC: BE093671.D

(22) Pentachlorophenol

16.914min (+0.004) 1541.68ng

response 60473

Ion	Exp%	Act%
266.00	100	100
264.00	70.00	63.28
268.00	65.00	62.12
0.00	0.00	0.00