


Data Path : Z:\HPCHEM1\BNA_E\Data\BE080517\
 Data File : BE093671.D
 Acq On : 5 Aug 2017 9:20
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE080117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 02 10:58:31 2017

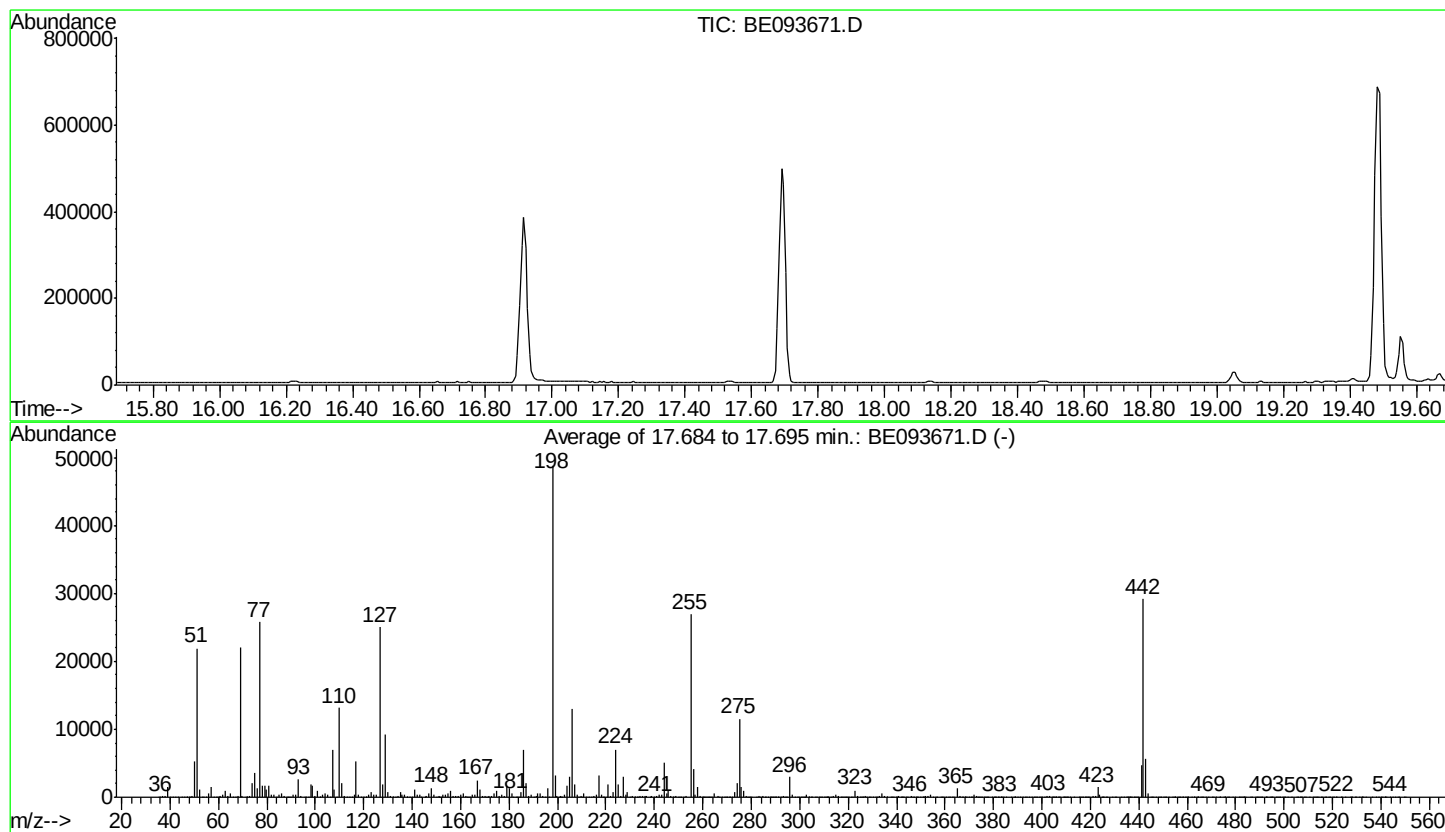

AutoFind: Scans 2569, 2570, 2571; Background Corrected with Scan 2561

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.8	21863	PASS
68	69	0.00	2	0.5	105	PASS
69	198	0.00	100	45.0	21978	PASS
70	69	0.00	2	0.6	131	PASS
127	198	10	80	51.2	24973	PASS
197	198	0.00	2	0.2	85	PASS
198	198	100	100	100.0	48808	PASS
199	198	5	9	6.6	3238	PASS
275	198	10	60	23.7	11564	PASS
365	198	1	100	2.5	1243	PASS
441	442	0.01	24	15.9	4641	PASS
442	198	50	100	59.7	29128	PASS
443	442	15	24	19.3	5635	PASS