


Data Path : Z:\HPCHEM1\BNA E\DATA\BE080715\  
Data File : BE090393.D  
Acq On : 7 Aug 2015 11:33  
Operator : TP/UM  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_E  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_E\METHODS\8270-SIM-BE080515.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Thu Aug 06 12:28:08 2015

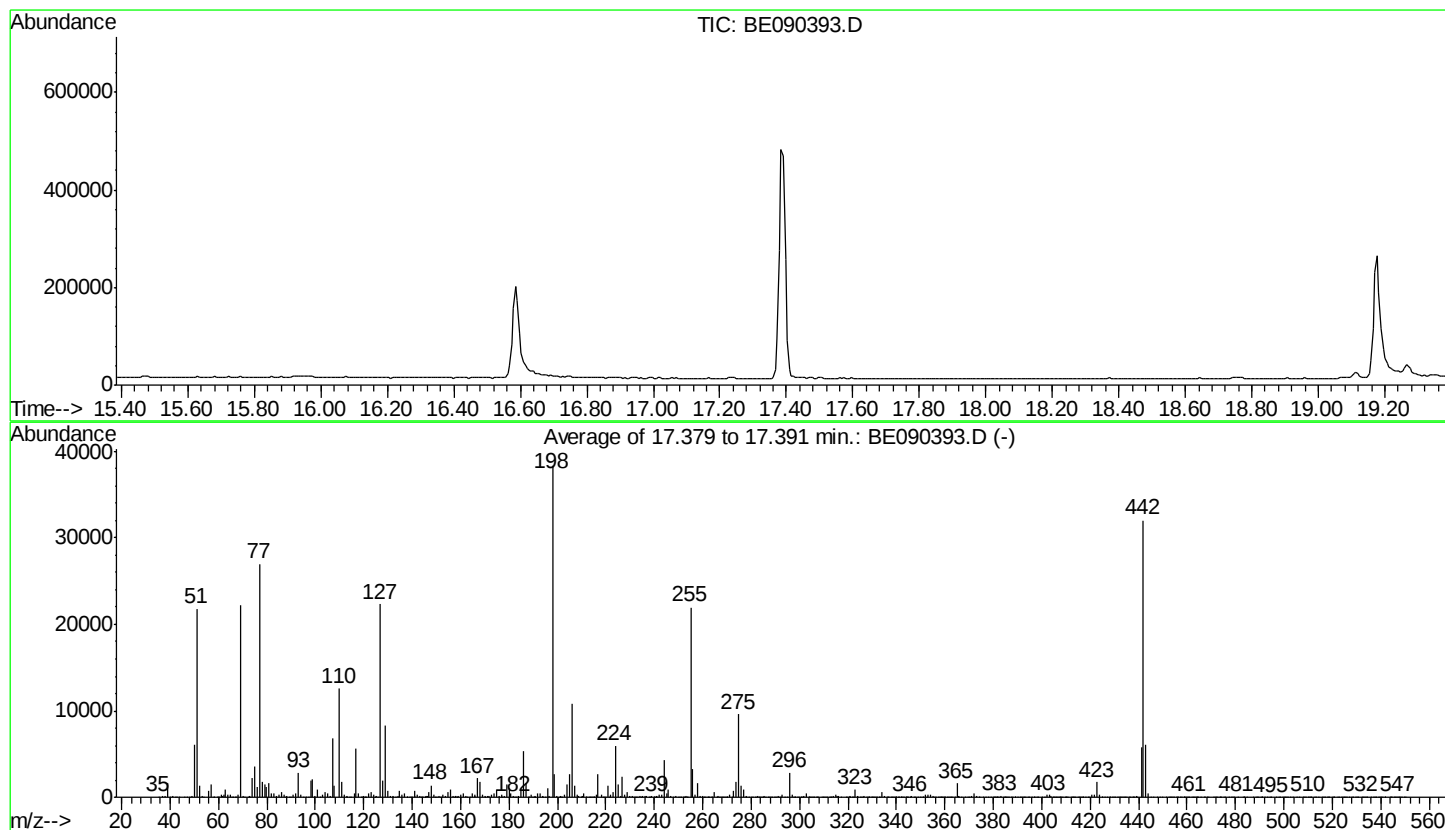

AutoFind: Scans 2517, 2518, 2519; Background Corrected with Scan 2511

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 56.8      | 21798   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.3       | 299     | PASS             |
| 69          | 198          | 0.00         | 100          | 57.8      | 22159   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.4       | 81      | PASS             |
| 127         | 198          | 10           | 80           | 58.3      | 22362   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 38367   | PASS             |
| 199         | 198          | 5            | 9            | 6.9       | 2656    | PASS             |
| 275         | 198          | 10           | 60           | 25.1      | 9623    | PASS             |
| 365         | 198          | 1            | 100          | 4.1       | 1567    | PASS             |
| 441         | 442          | 0.01         | 24           | 18.1      | 5804    | PASS             |
| 442         | 198          | 50           | 100          | 83.4      | 32011   | PASS             |
| 443         | 442          | 15           | 24           | 19.1      | 6129    | PASS             |