


Data Path : Z:\HPCHEM1\BNA E\DATA\BE080715\
 Data File : BE090393.D
 Acq On : 7 Aug 2015 11:33
 Operator : TP/UM
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE080515.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 06 12:28:08 2015

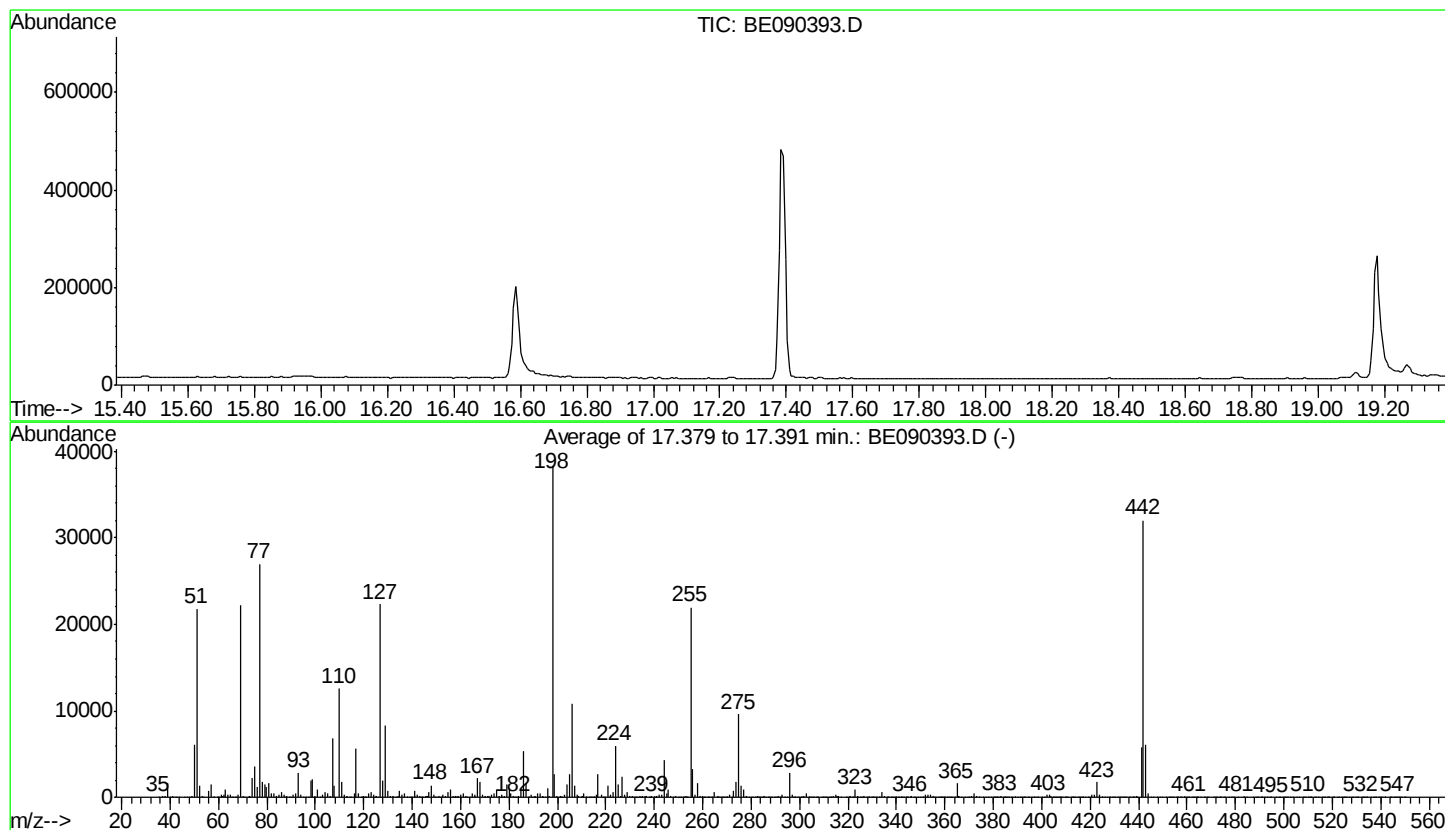

AutoFind: Scans 2517, 2518, 2519; Background Corrected with Scan 2511

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	56.8	21798	PASS
68	69	0.00	2	1.3	299	PASS
69	198	0.00	100	57.8	22159	PASS
70	69	0.00	2	0.4	81	PASS
127	198	10	80	58.3	22362	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	38367	PASS
199	198	5	9	6.9	2656	PASS
275	198	10	60	25.1	9623	PASS
365	198	1	100	4.1	1567	PASS
441	442	0.01	24	18.1	5804	PASS
442	198	50	100	83.4	32011	PASS
443	442	15	24	19.1	6129	PASS