
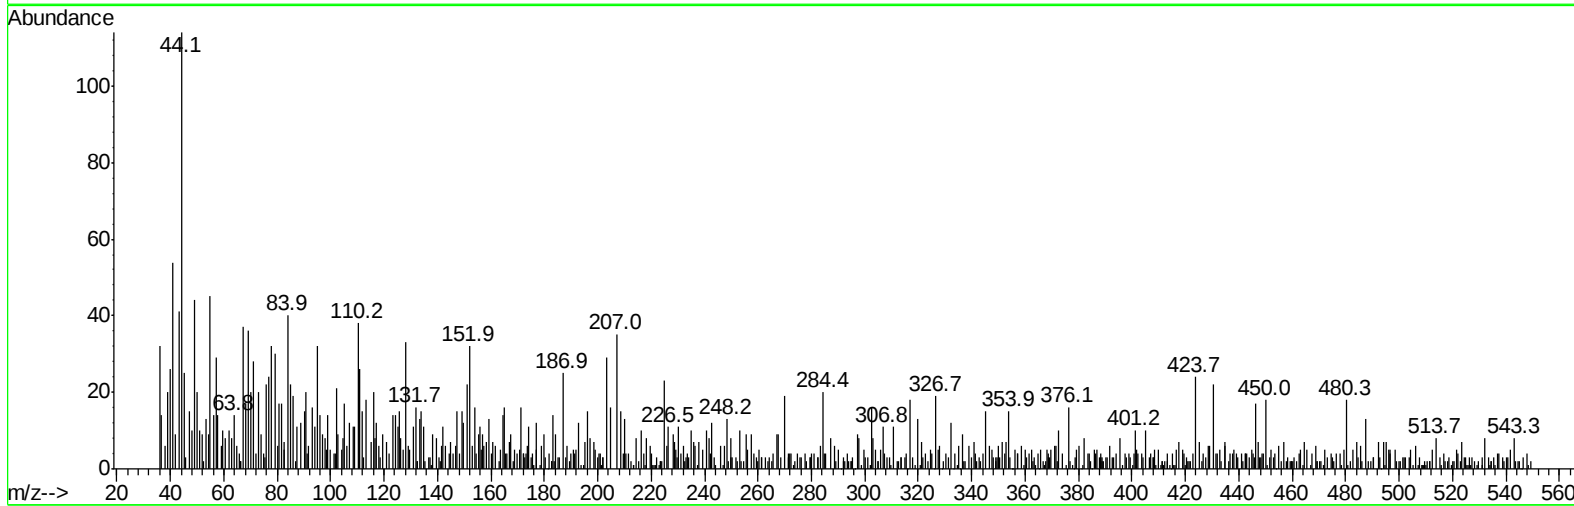


Data Path : Z:\HPCHEM1\BNA E\DATA\BE080717\
Data File : BE093692.D
Acq On : 7 Aug 2017 8:42
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 08 01:09:15 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 07 16:02:51 2017
Response via : Initial Calibration

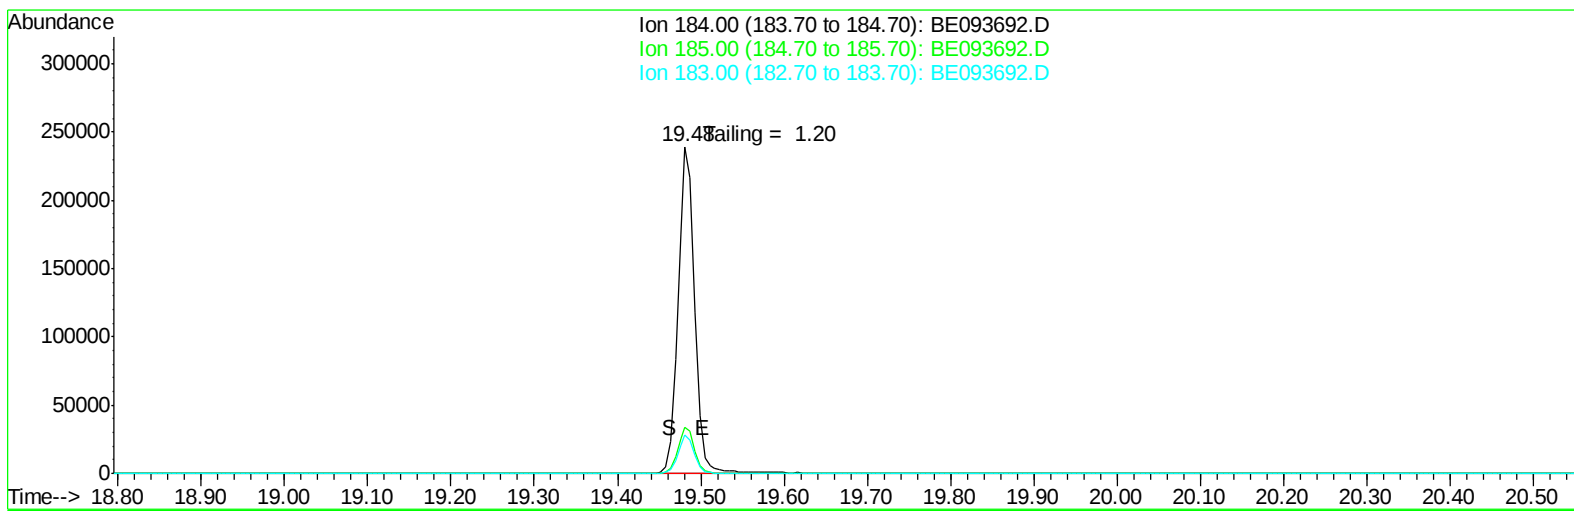

TIC: BE093692.D

(76) Benzidine



12.055min (-0.190) 8.42ng

response 5

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	54.55#
183.00	12.20	163.64#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE080717\
Data File : BE093692.D
Acq On : 7 Aug 2017 8:42
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 08 01:09:15 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 07 16:02:51 2017
Response via : Initial Calibration

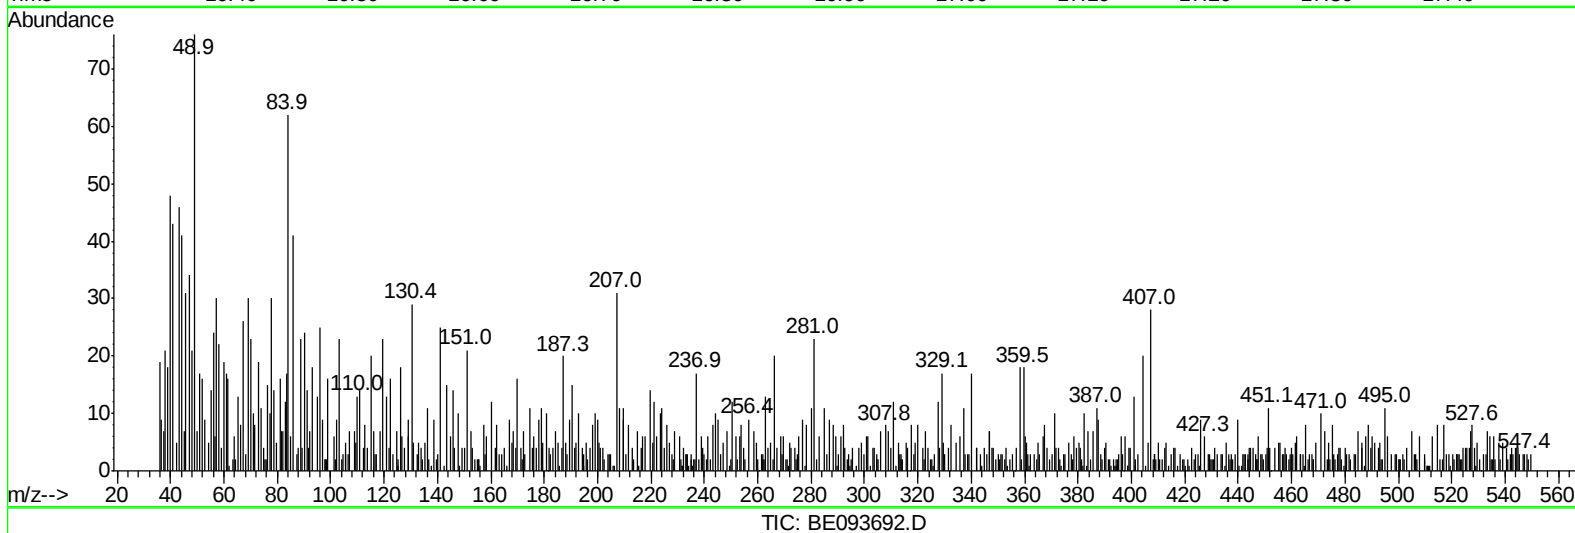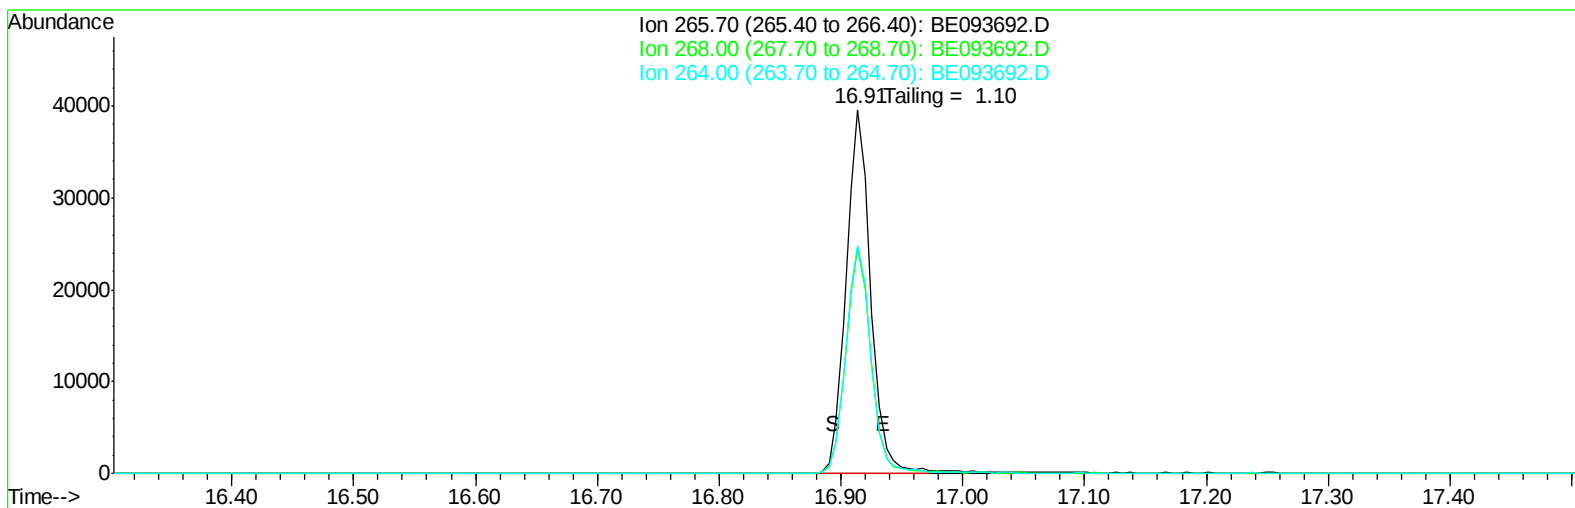

(69) Pentachlorophenol (C)

10.562min (-0.182) 2699.53ng

response 25

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	27.27#
264.00	64.60	40.91#
0.00	0.00	0.00