


Data Path : Z:\HPCHEM1\BNA E\Data\BE080717\
 Data File : BE093692.D
 Acq On : 7 Aug 2017 8:42
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE080717.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 07 14:30:21 2017

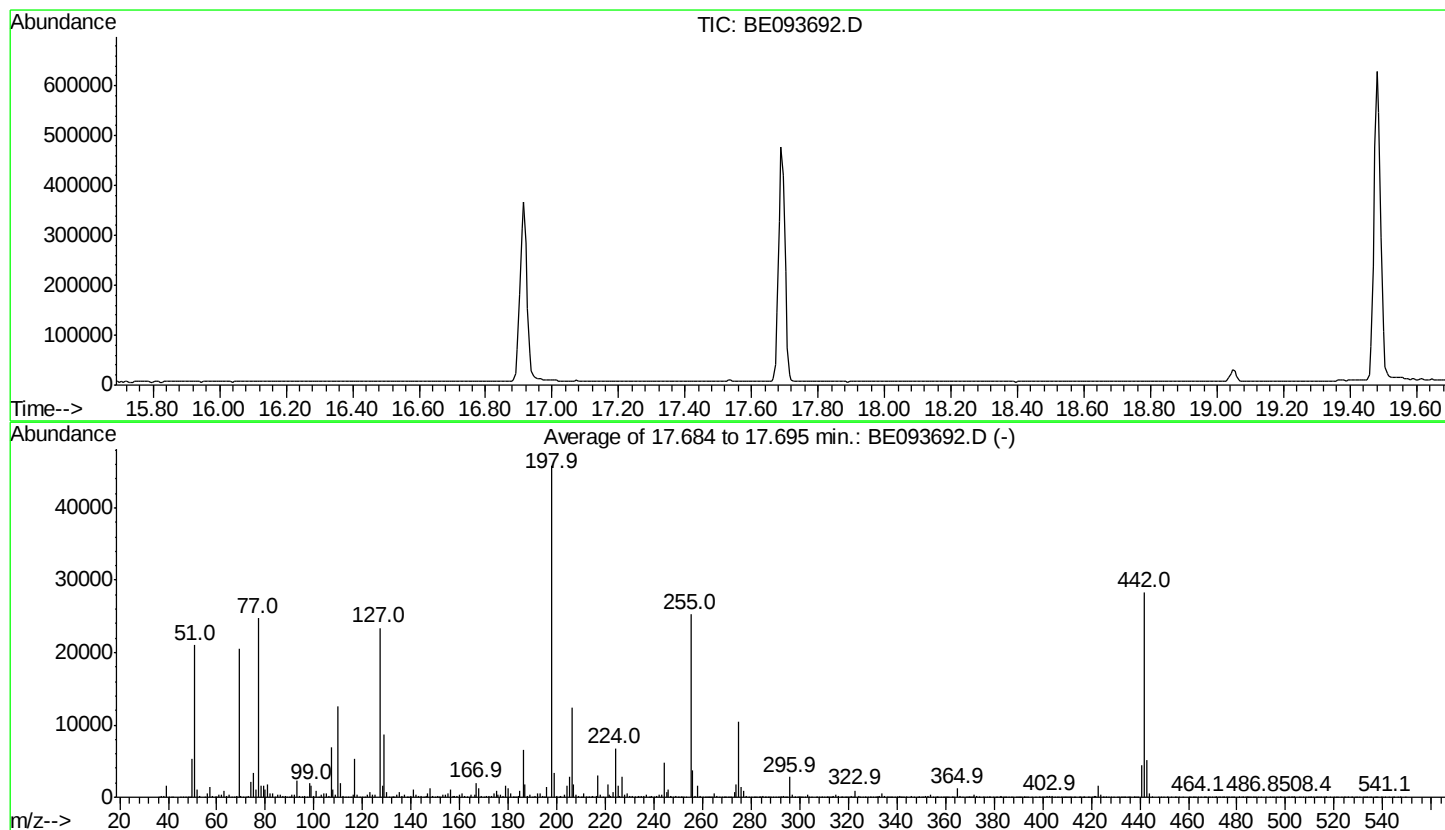

AutoFind: Scans 2569, 2570, 2571; Background Corrected with Scan 2562

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.8	20989	PASS
68	69	0.00	2	1.1	236	PASS
69	198	0.00	100	44.8	20547	PASS
70	69	0.00	2	0.7	134	PASS
127	198	10	80	51.0	23362	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	45829	PASS
199	198	5	9	7.3	3332	PASS
275	198	10	60	22.9	10481	PASS
365	198	1	100	2.5	1166	PASS
441	442	0.01	24	15.9	4478	PASS
442	198	50	100	61.6	28241	PASS
443	442	15	24	18.5	5215	PASS