


Data Path : Z:\HPCHEM1\BNA_E\Data\BE080816\
 Data File : BE092217.D
 Acq On : 8 Aug 2016 15:06
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-PAH-BE080216.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 08 18:55:30 2016

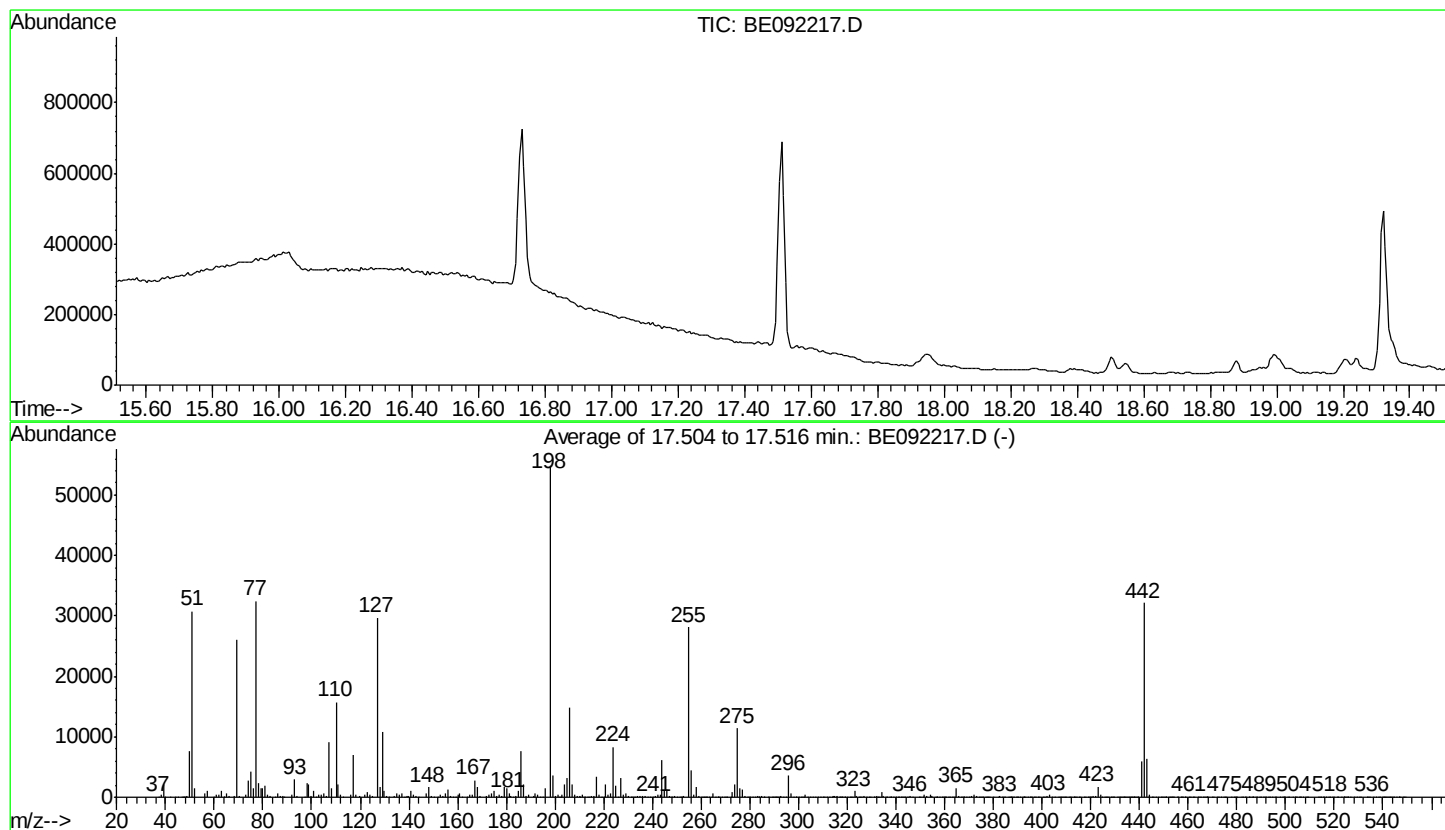

AutoFind: Scans 2539, 2540, 2541; Background Corrected with Scan 2532

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	56.2	30800	PASS
68	69	0.00	2	0.7	181	PASS
69	198	0.00	100	47.4	25987	PASS
70	69	0.00	2	0.4	116	PASS
127	198	10	80	54.1	29678	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	54844	PASS
199	198	5	9	6.5	3583	PASS
275	198	10	60	20.8	11426	PASS
365	198	1	100	2.9	1595	PASS
441	442	0.01	24	18.5	5937	PASS
442	198	50	100	58.6	32136	PASS
443	442	15	24	19.9	6401	PASS