

Data Path : Z:\HPCHEM1\BNA E\DATA\BE080817\
 Data File : BE093712.D
 Acq On : 8 Aug 2017 11:53
 Operator : SJ/JU
 Sample : PB101074BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SBLK74

Quant Time: Aug 09 04:21:32 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 09 04:20:36 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.92	152	3297	0.40	ng/ul	0.00
2) Naphthalene-d8	10.71	136	17120	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.53	164	10752	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.26
16) Chrysene-d12	21.41	240	21826	0.40	ng/ul	0.00
20) Perylene-d12	23.76	264	1522445	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.29	152	7559	0.27	ng/ul	0.00
14) Fluoranthene-d10	19.27	212	18296	0.00	ng/ul	0.00
Target Compounds						
9) Fluorene	15.51	166	2350	0.053	ng/ul#	21
17) Pyrene	19.64	202	2508	0.039	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE080817\
Data File : BE093712.D
Acq On : 8 Aug 2017 11:53
Operator : SJ/JU
Sample : PB101074BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK74

Quant Time: Aug 09 04:21:32 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 09 04:20:36 2017
Response via : Initial Calibration

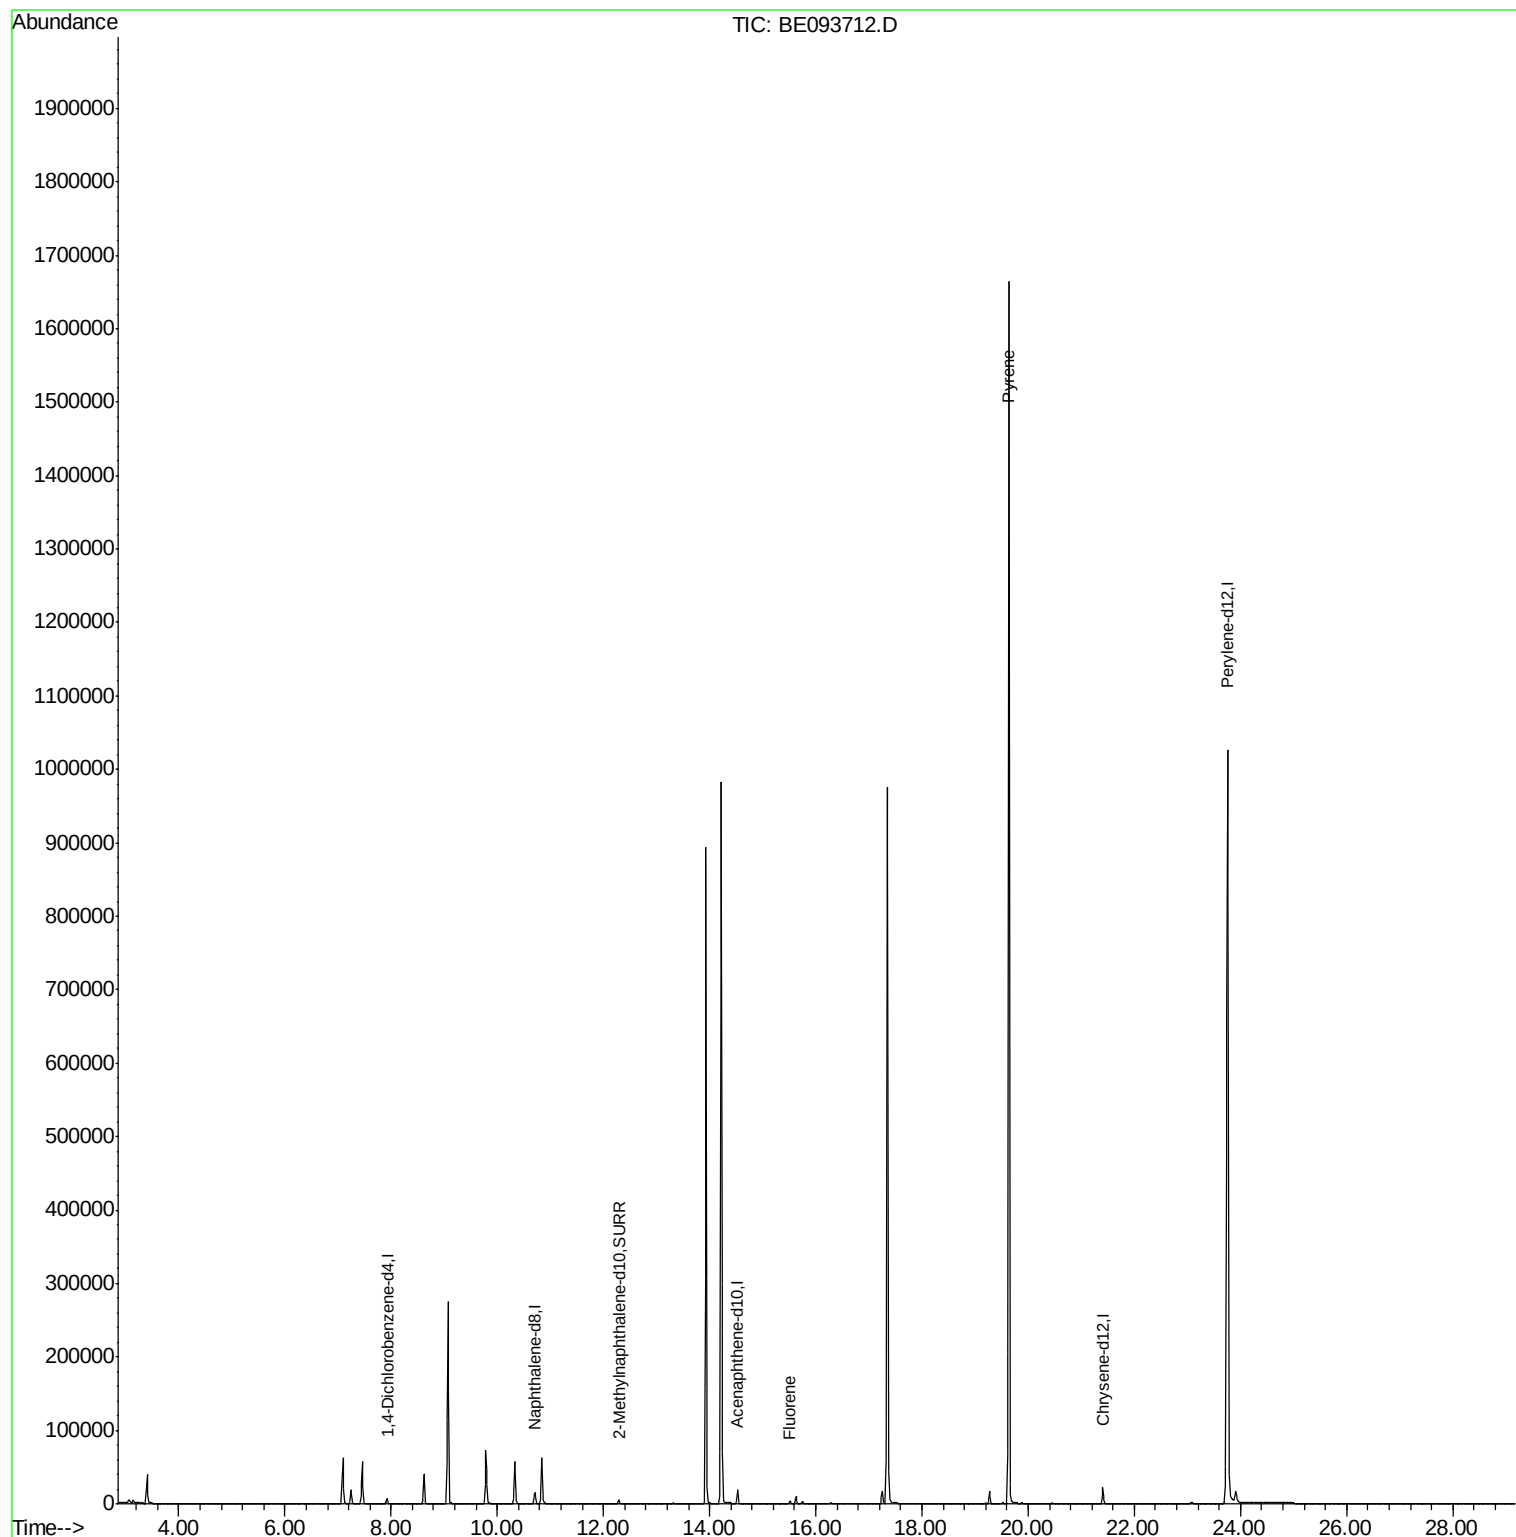

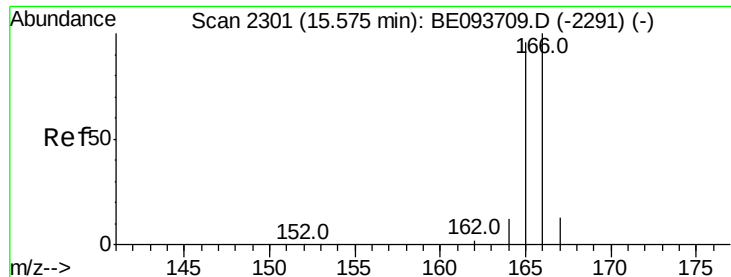

#9

Fluorene

Concen: 0.053 ng/ul

RT: 15.51 min Scan# 2293

Delta R.T. -0.06 min

Lab File: BE093712.D

Acq: 8 Aug 2017 11:53

Instrument :

BNA_E

ClientSampleId :

SBLK74





Tot Ion:166 Resp: 2350

Ion Ratio Lower Upper

166 100

165 6.5 73.4 110.2#

167 30.9 14.6 22.0#

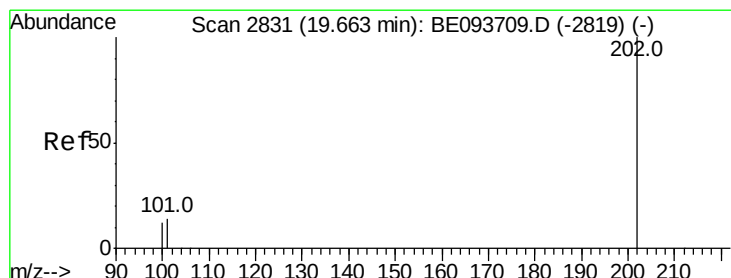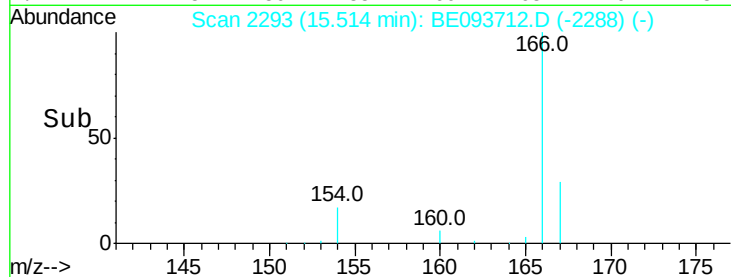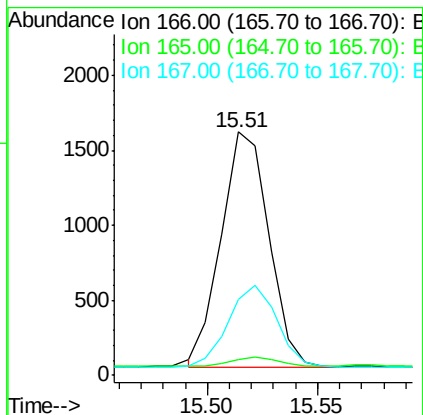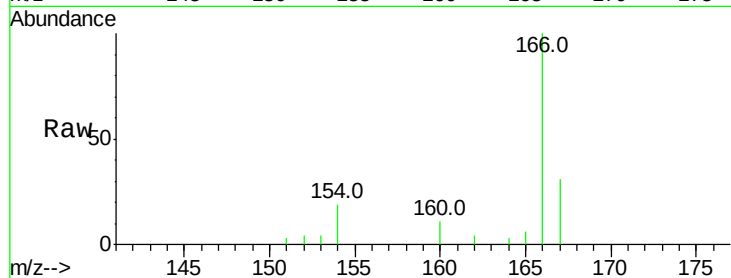

#17

Pyrene

Concen: 0.039 ng/ul

RT: 19.64 min Scan# 2825

Delta R.T. -0.03 min

Lab File: BE093712.D

Acq: 8 Aug 2017 11:53

Tgt Ion:202 Resp: 2508

Ion Ratio Lower Upper

202 100

101 179.1 18.2 27.4#

100 1070.2 15.6 23.4#

