

Data Path : Z:\HPCHEM1\BNA E\DATA\BE080817\
 Data File : BE093713.D
 Acq On : 8 Aug 2017 12:28
 Operator : SJ/JU
 Sample : PB101075BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SBLK75

Quant Time: Aug 09 04:21:38 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 09 04:20:36 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.92	152	3464	0.40	ng/ul	0.00
2) Naphthalene-d8	10.71	136	17682	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.52	164	10824	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.26
16) Chrysene-d12	21.41	240	23093	0.40	ng/ul	0.00
20) Perylene-d12	23.75	264	1560325	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.29	152	7618	0.27	ng/ul	0.00
14) Fluoranthene-d10	19.27	212	18300	0.00	ng/ul	0.00
Target Compounds						
9) Fluorene	15.52	166	2321	0.052	ng/ul#	20
17) Pyrene	19.64	202	2467	0.037	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE080817\
Data File : BE093713.D
Acq On : 8 Aug 2017 12:28
Operator : SJ/JU
Sample : PB101075BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK75

Quant Time: Aug 09 04:21:38 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 09 04:20:36 2017
Response via : Initial Calibration

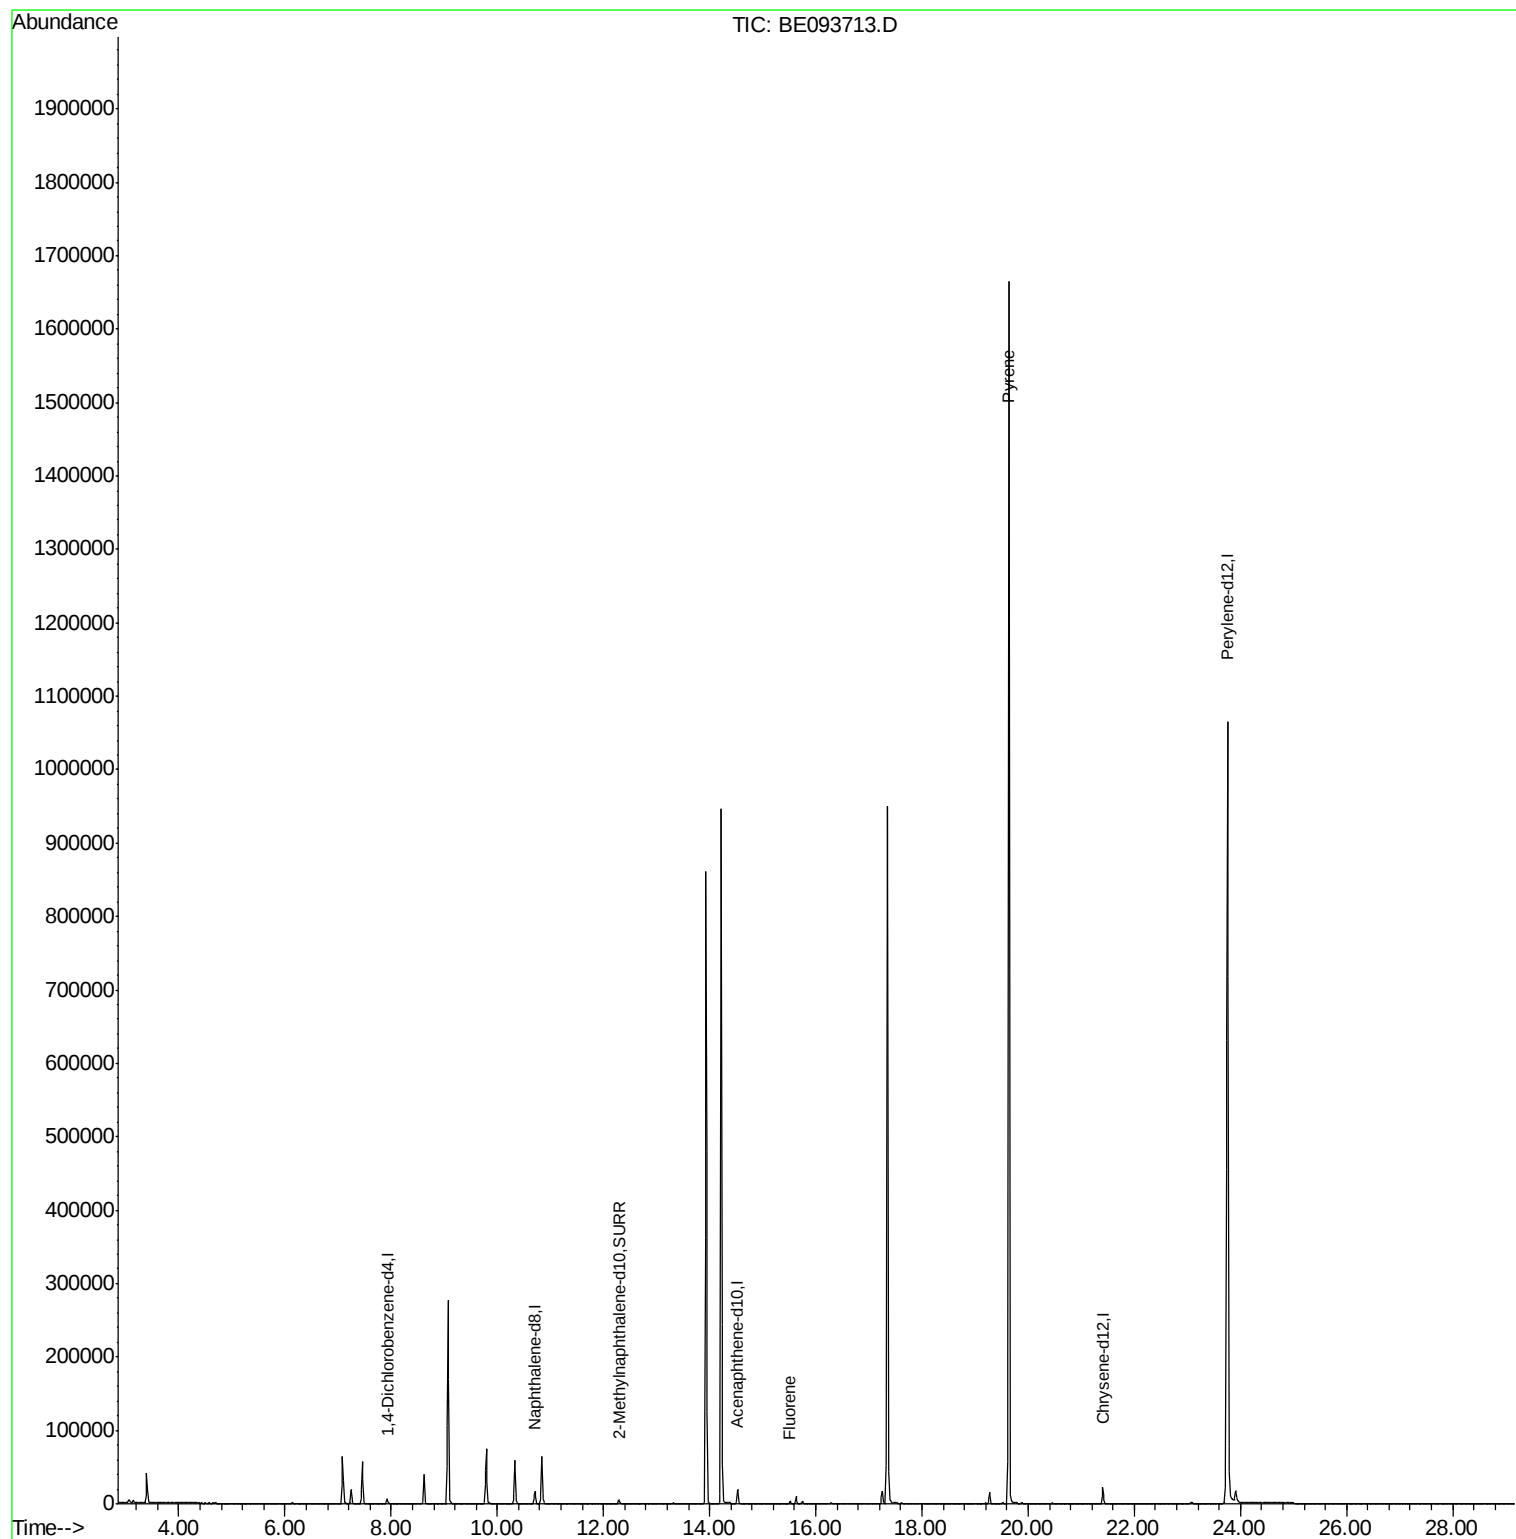

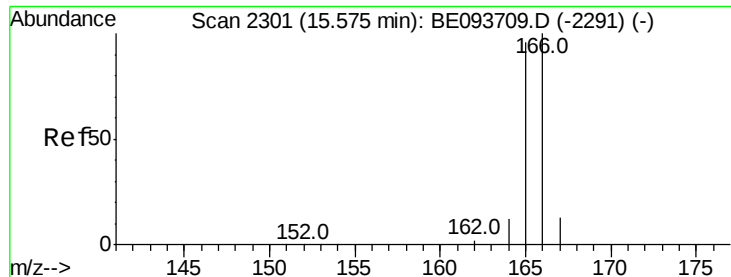

#9

Fluorene

Concen: 0.052 ng/ul

RT: 15.52 min Scan# 2293

Delta R.T. -0.06 min

Lab File: BE093713.D

Acq: 8 Aug 2017 12:28

Instrument :

BNA_E

ClientSampleId :

SBLK75





Tot Ion:166 Resp: 2321

Ion Ratio Lower Upper

166 100

165 6.1 73.4 110.2#

167 32.5 14.6 22.0#

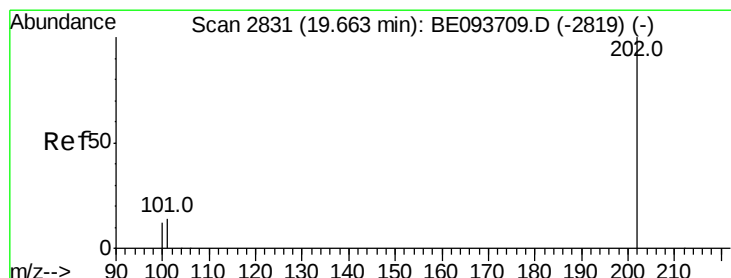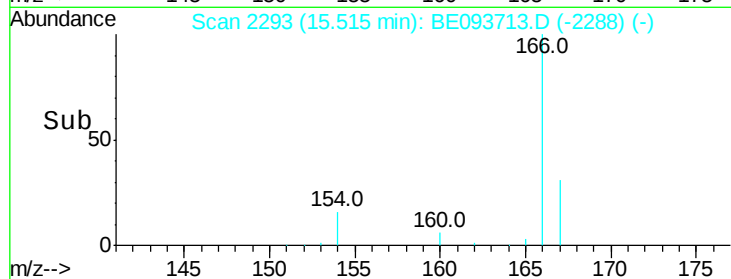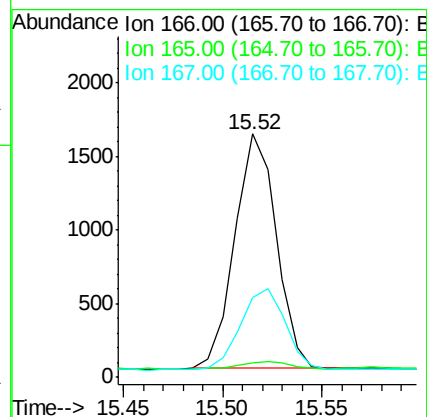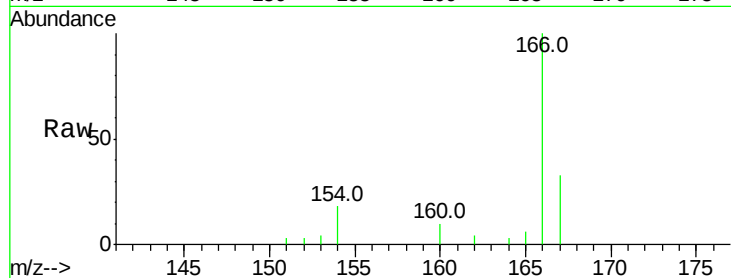

#17

Pyrene

Concen: 0.037 ng/ul

RT: 19.64 min Scan# 2826

Delta R.T. -0.02 min

Lab File: BE093713.D

Acq: 8 Aug 2017 12:28

Tgt Ion:202 Resp: 2467

Ion Ratio Lower Upper

202 100

101 169.7 18.2 27.4#

100 905.8 15.6 23.4#

