

Data Path : Z:\HPCHEM1\BNA E\DATA\BE080817\
 Data File : BE093714.D
 Acq On : 8 Aug 2017 13:07
 Operator : SJ/JU
 Sample : I4504-11
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AG5

Quant Time: Aug 09 04:21:44 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 09 04:20:36 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.92	152	3478	0.40	ng/ul	0.00
2) Naphthalene-d8	10.71	136	17669	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.53	164	10619	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.26	188	22607	0.40	ng/ul	0.00
16) Chrysene-d12	21.41	240	22257	0.40	ng/ul	0.00
20) Perylene-d12	23.75	264	1403573	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.29	152	6775	0.24	ng/ul	0.00
14) Fluoranthene-d10	19.27	212	16825	0.24	ng/ul	0.00
Target Compounds						
9) Fluorene	15.51	166	2137	0.048	ng/ul#	20
17) Pyrene	19.64	202	2319	0.036	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE080817\
Data File : BE093714.D
Acq On : 8 Aug 2017 13:07
Operator : SJ/JU
Sample : I4504-11
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AG5

Quant Time: Aug 09 04:21:44 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 09 04:20:36 2017
Response via : Initial Calibration

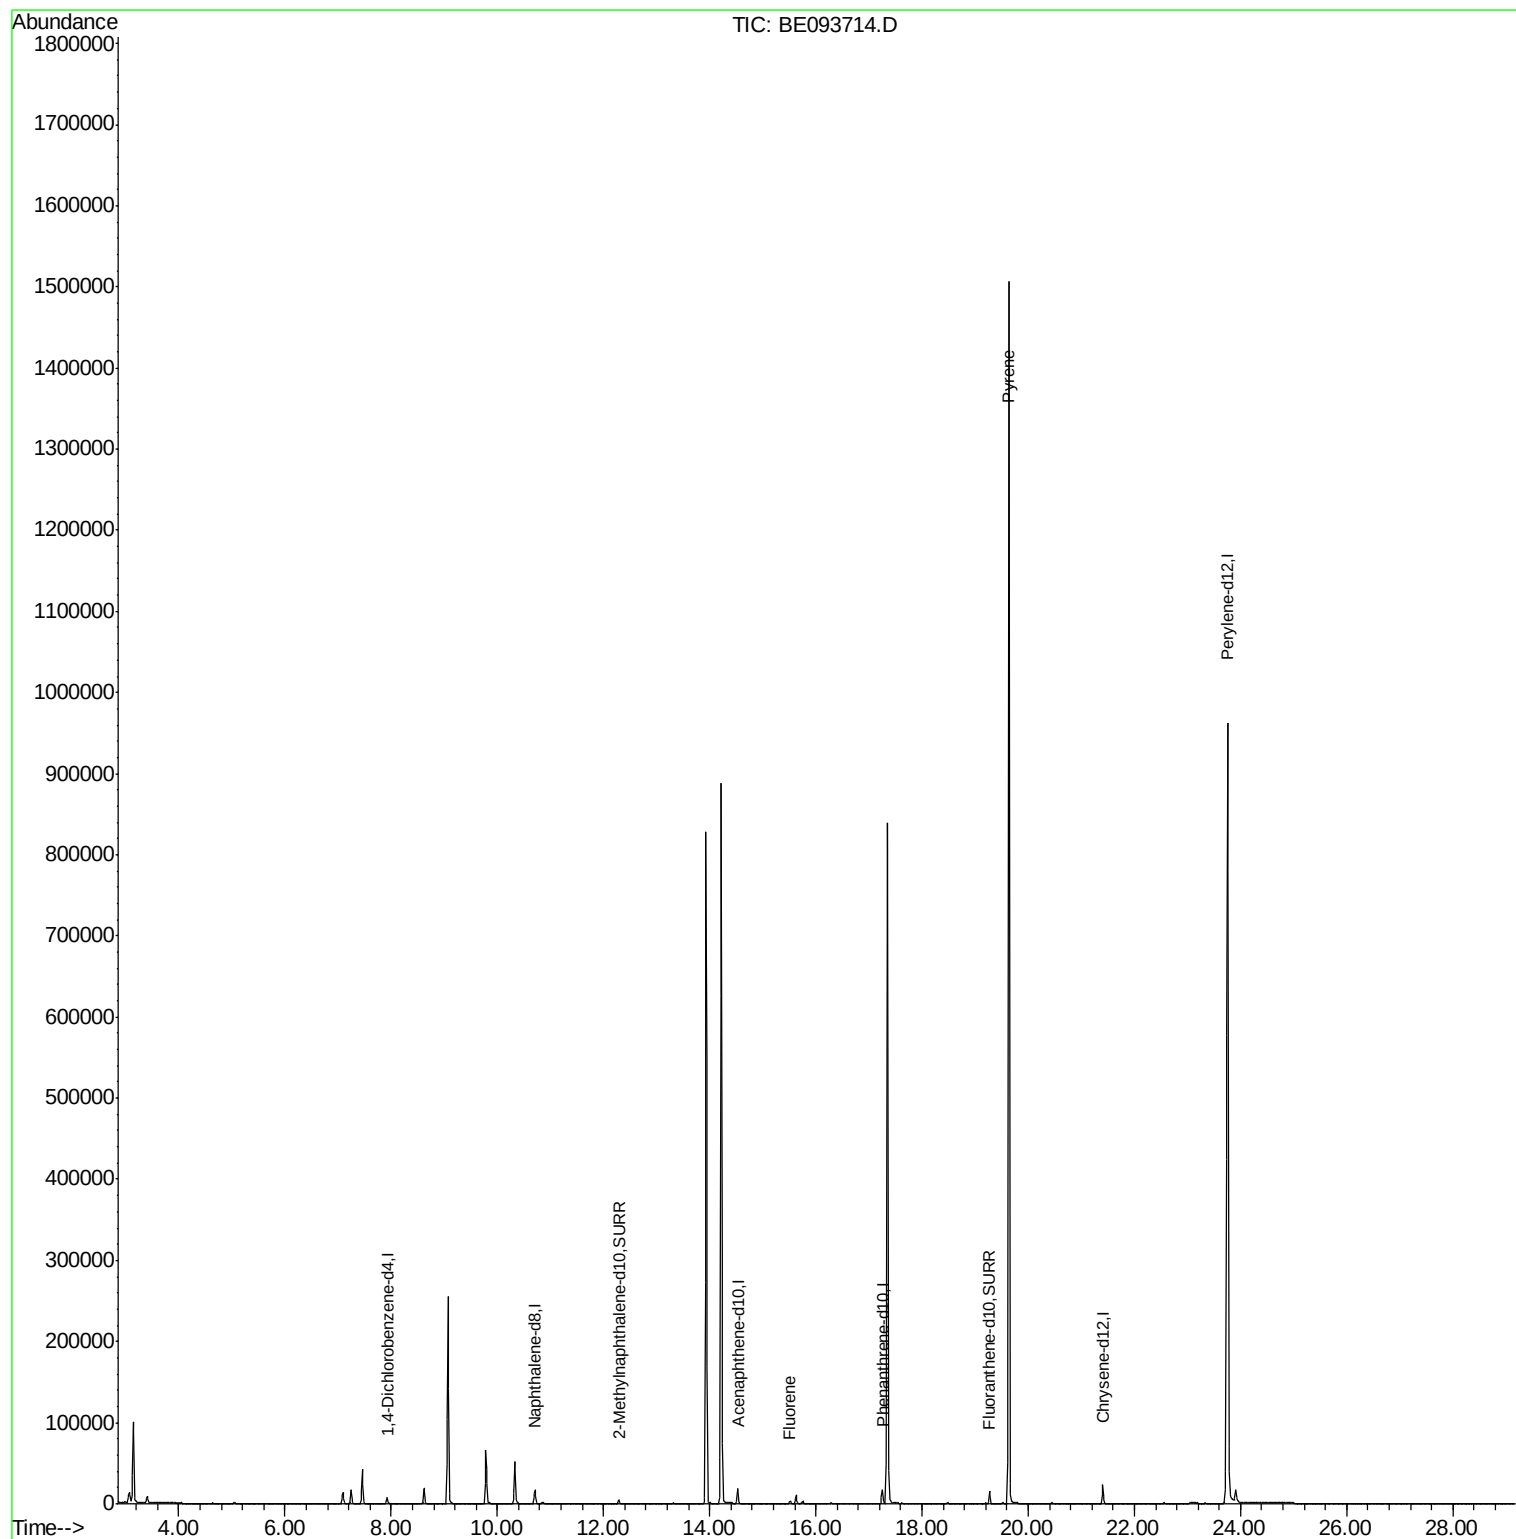

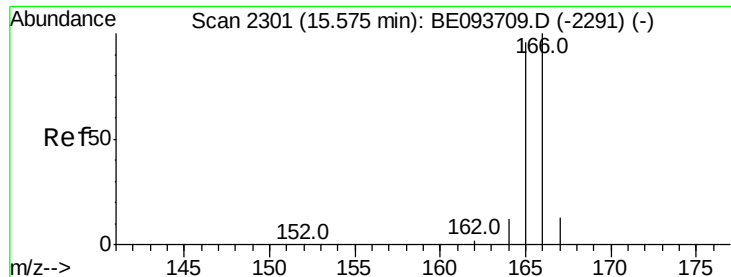

#9

Fluorene

Concen: 0.048 ng/ul

RT: 15.51 min Scan# 2292

Delta R.T. -0.06 min

Lab File: BE093714.D

Acq: 8 Aug 2017 13:07

Instrument :

BNA_E

ClientSampleId :

C0AG5





Tot Ion:166 Resp: 2137

Ion Ratio Lower Upper

166 100

165 6.8 73.4 110.2#

167 32.6 14.6 22.0#

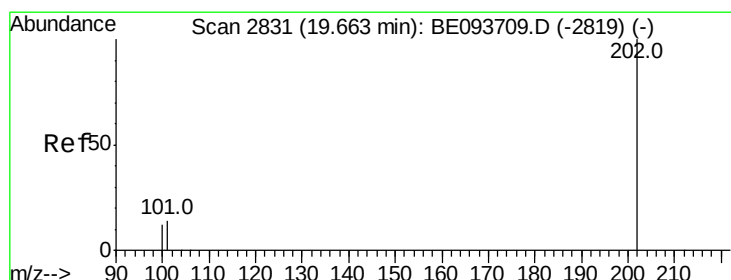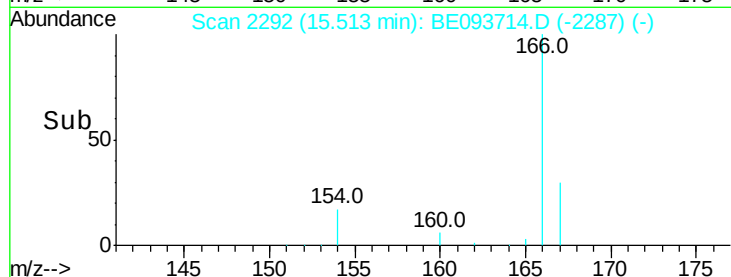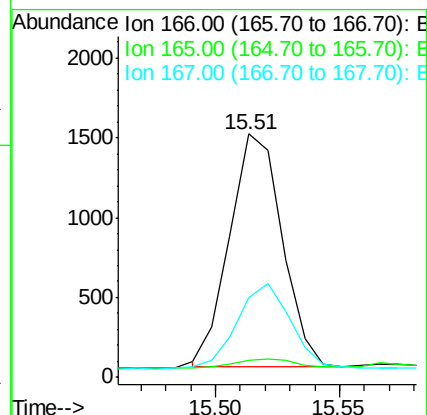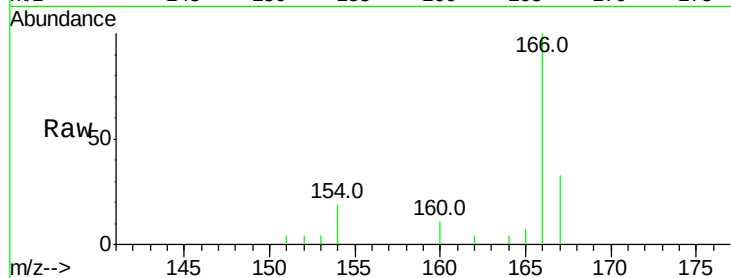

#17

Pyrene

Concen: 0.036 ng/ul

RT: 19.64 min Scan# 2824

Delta R.T. -0.03 min

Lab File: BE093714.D

Acq: 8 Aug 2017 13:07

Tgt Ion:202 Resp: 2319

Ion Ratio Lower Upper

202 100

101 181.4 18.2 27.4#

100 1068.0 15.6 23.4#

