

Data Path : Z:\HPCHEM1\BNA E\DATA\BE080817\
 Data File : BE093717.D
 Acq On : 8 Aug 2017 14:57
 Operator : SJ/JU
 Sample : I4504-03
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AF9

Quant Time: Aug 09 04:22:03 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 09 04:20:36 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.92	152	3262	0.40	ng/ul	0.00
2) Naphthalene-d8	10.71	136	16874	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.53	164	10611	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.26
16) Chrysene-d12	21.41	240	23724	0.40	ng/ul	0.00
20) Perylene-d12	23.75	264	1473321	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.29	152	6885	0.25	ng/ul	0.00
14) Fluoranthene-d10	19.27	212	19319	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	19.64	202	3528	0.051	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE080817\
Data File : BE093717.D
Acq On : 8 Aug 2017 14:57
Operator : SJ/JU
Sample : I4504-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AF9

Quant Time: Aug 09 04:22:03 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 09 04:20:36 2017
Response via : Initial Calibration

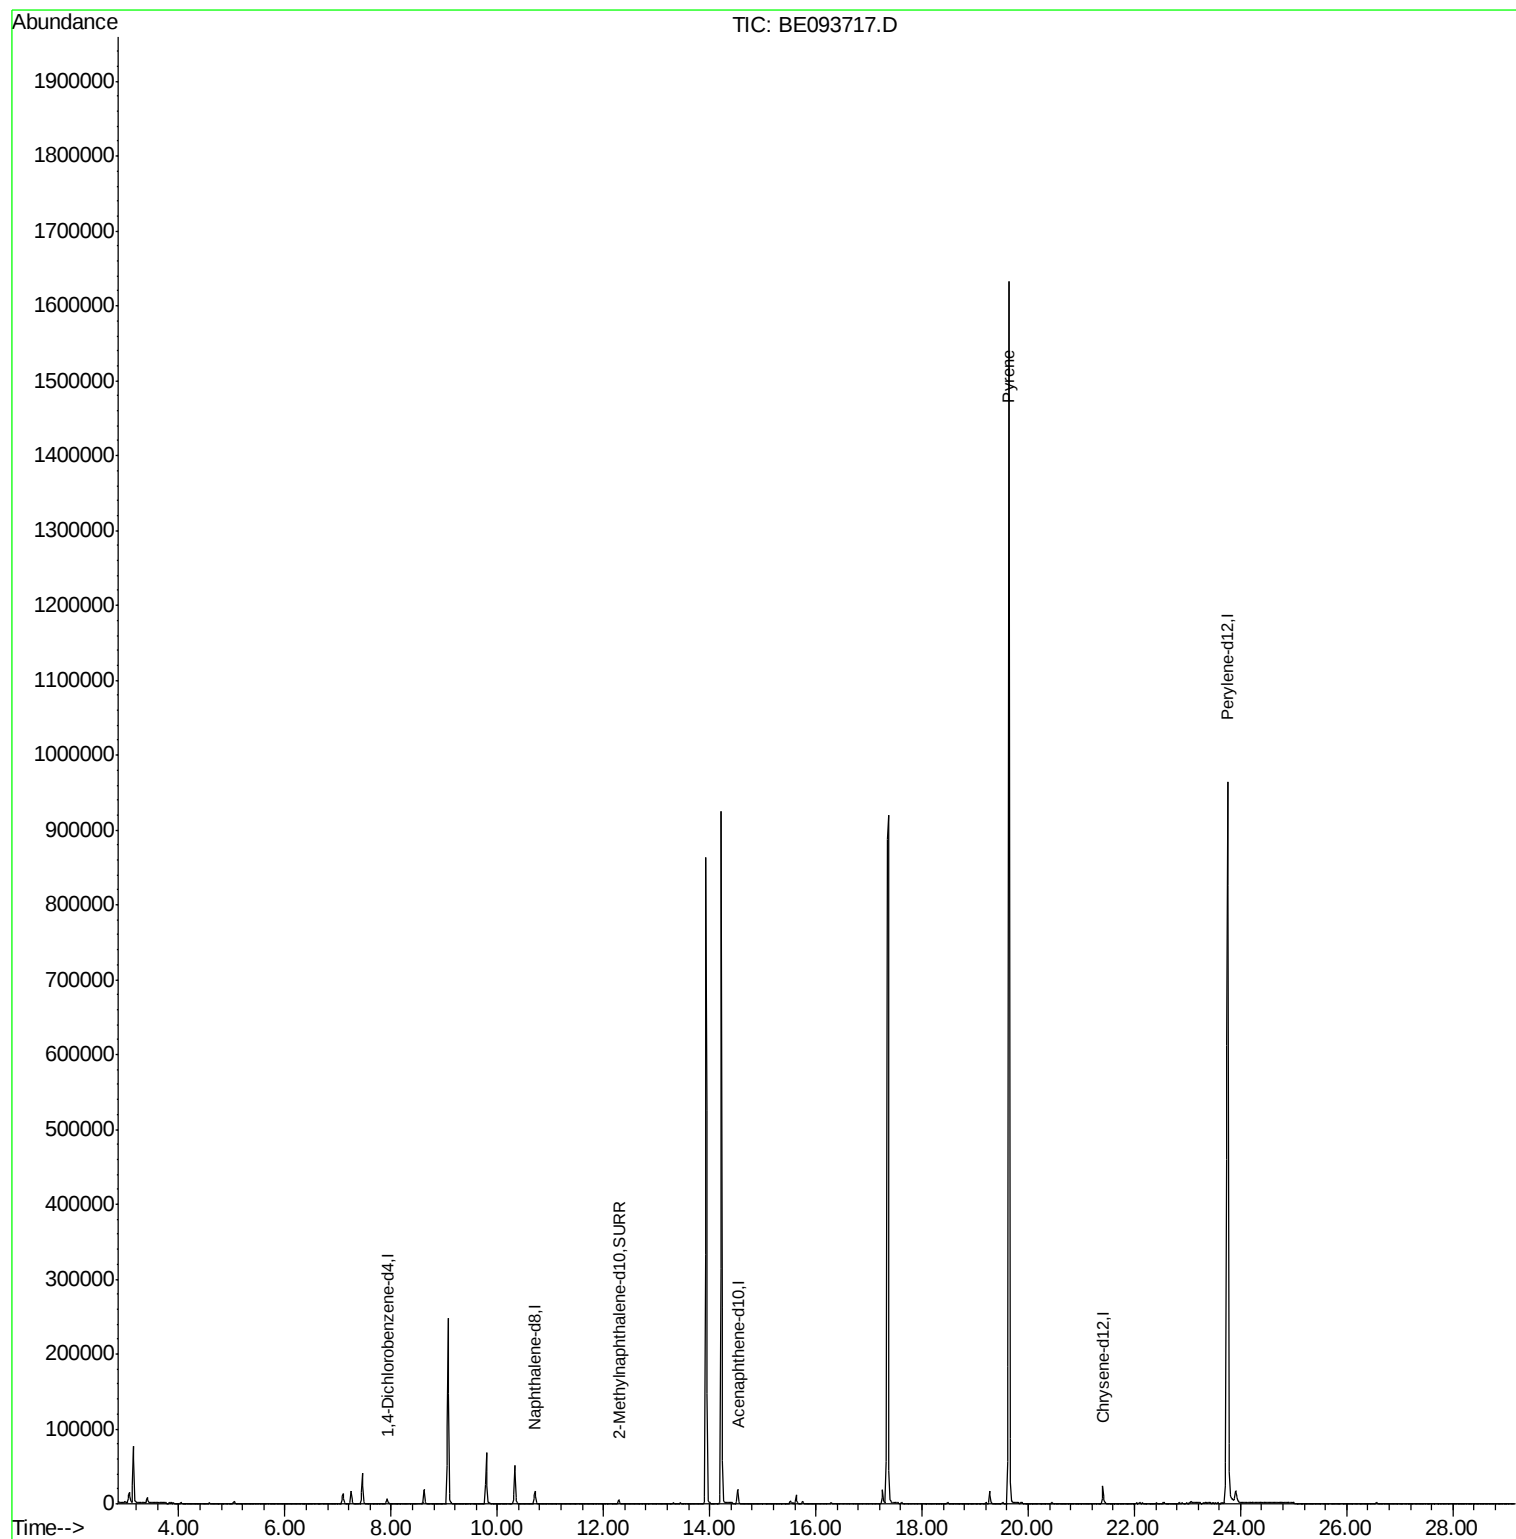

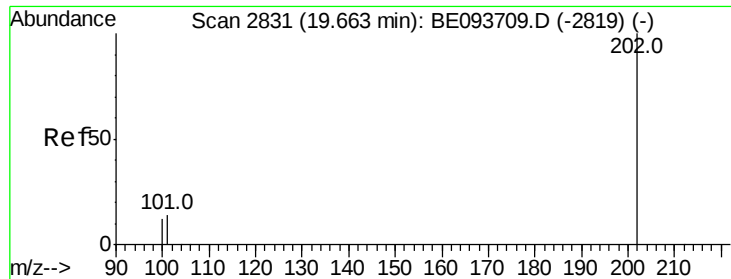

#17
 Pvrene
 Concen: 0.051 ng/ul
 RT: 19.64 min Scan# 2826
 Delta R.T. -0.02 min
 Lab File: BE093717.D
 Acq: 8 Aug 2017 14:57

Instrument :
 BNA_E
 ClientSampleId :
 C0AF9

Tot Ion: 202 Resp: 3528
 Ion Ratio Lower Upper
 202 100
 101 165.6 18.2 27.4#
 100 884.9 15.6 23.4#

