

Data Path : Z:\HPCHEM1\BNA E\DATA\BE080817\
 Data File : BE093727.D
 Acq On : 8 Aug 2017 21:10
 Operator : SJ/JU
 Sample : I4529-08
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AA2

Quant Time: Aug 09 05:32:38 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 09 05:31:57 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.92	152	3308	0.40	ng/ul	0.00
2) Naphthalene-d8	10.71	136	17132	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.53	164	10487	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.26	188	22625	0.40	ng/ul	0.00
16) Chrysene-d12	21.41	240	22662	0.40	ng/ul	0.00
20) Perylene-d12	23.75	264	1512365	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.29	152	7351	0.26	ng/ul	0.00
14) Fluoranthene-d10	19.27	212	19569	0.27	ng/ul	0.00
Target Compounds						
17) Pyrene	19.64	202	2602	0.039	ng/ul#	Ovalue 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE080817\
Data File : BE093727.D
Acq On : 8 Aug 2017 21:10
Operator : SJ/JU
Sample : I4529-08
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AA2

Quant Time: Aug 09 05:32:38 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 09 05:31:57 2017
Response via : Initial Calibration

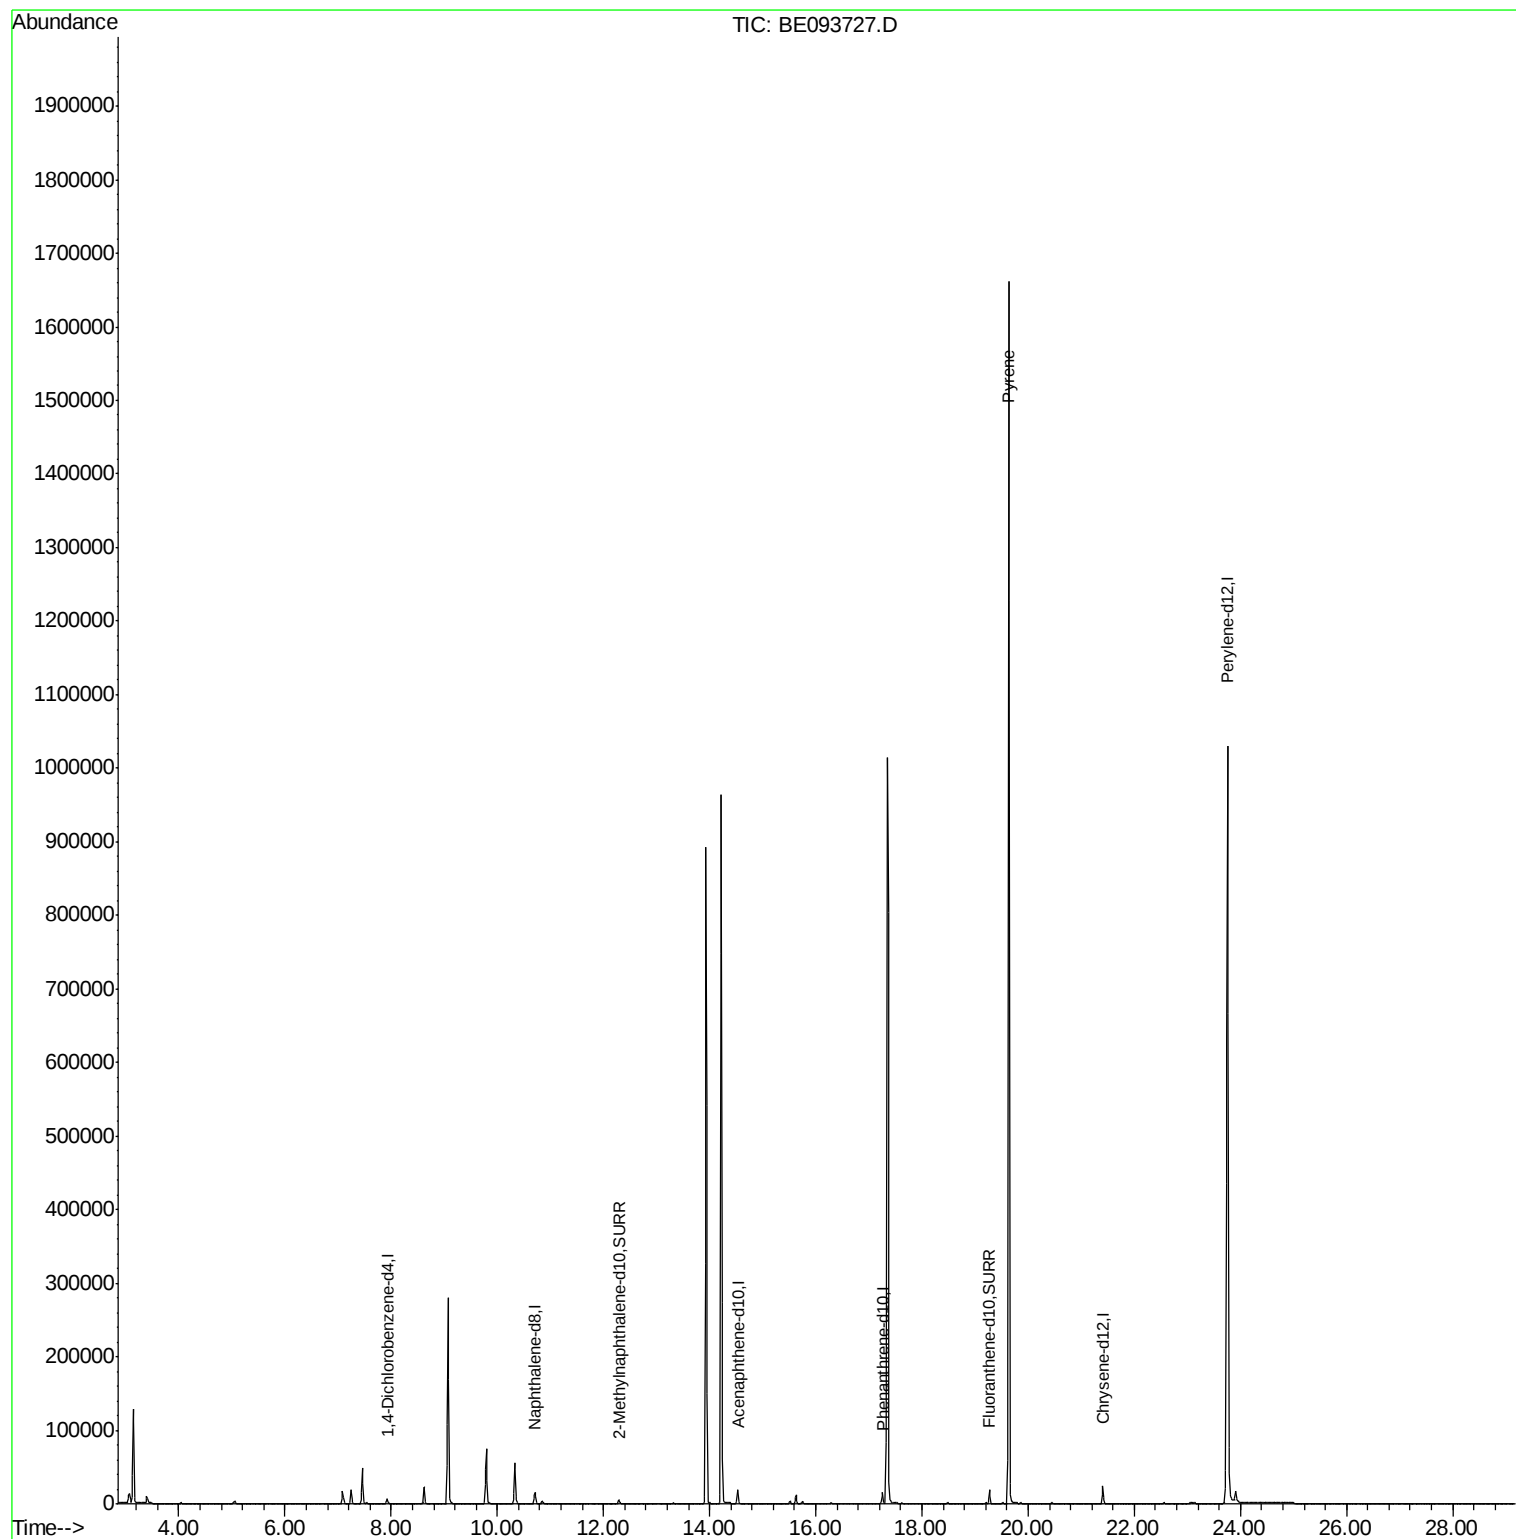

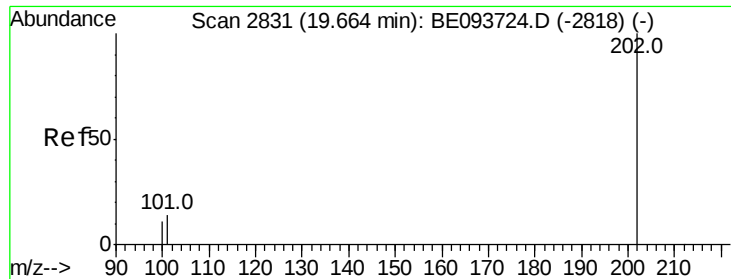

#17

Pvrene

Concen: 0.039 ng/ul

RT: 19.64 min Scan# 2825

Delta R.T. -0.02 min

Lab File: BE093727.D

Acq: 8 Aug 2017 21:10

Instrument :

BNA_E

ClientSampleId :

C0AA2


Tot Ion:202 Resp: 2602

Ion Ratio Lower Upper

202 100

101 168.7 18.2 27.4#

100 893.1 15.6 23.4#

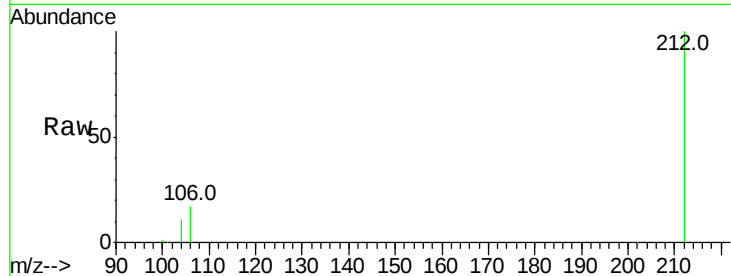

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): E

