

Data Path : Z:\HPCHEM1\BNA E\DATA\BE080817\
 Data File : BE093728.D
 Acq On : 8 Aug 2017 21:46
 Operator : SJ/JU
 Sample : I4529-13
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AB0

Quant Time: Aug 09 05:32:45 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 09 05:31:57 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.92	152	3397	0.40	ng/ul	0.00
2) Naphthalene-d8	10.71	136	17586	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.53	164	10798	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.26	188	23187	0.40	ng/ul	0.00
16) Chrysene-d12	21.41	240	22942	0.40	ng/ul	0.00
20) Perylene-d12	23.75	264	1256612	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.29	152	6300	0.22	ng/ul	0.00
14) Fluoranthene-d10	19.27	212	17491	0.24	ng/ul	0.00
Target Compounds						
17) Pyrene	19.64	202	2291	0.034	ng/ul#	Ovalue 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE080817\
Data File : BE093728.D
Acq On : 8 Aug 2017 21:46
Operator : SJ/JU
Sample : I4529-13
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AB0

Quant Time: Aug 09 05:32:45 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 09 05:31:57 2017
Response via : Initial Calibration

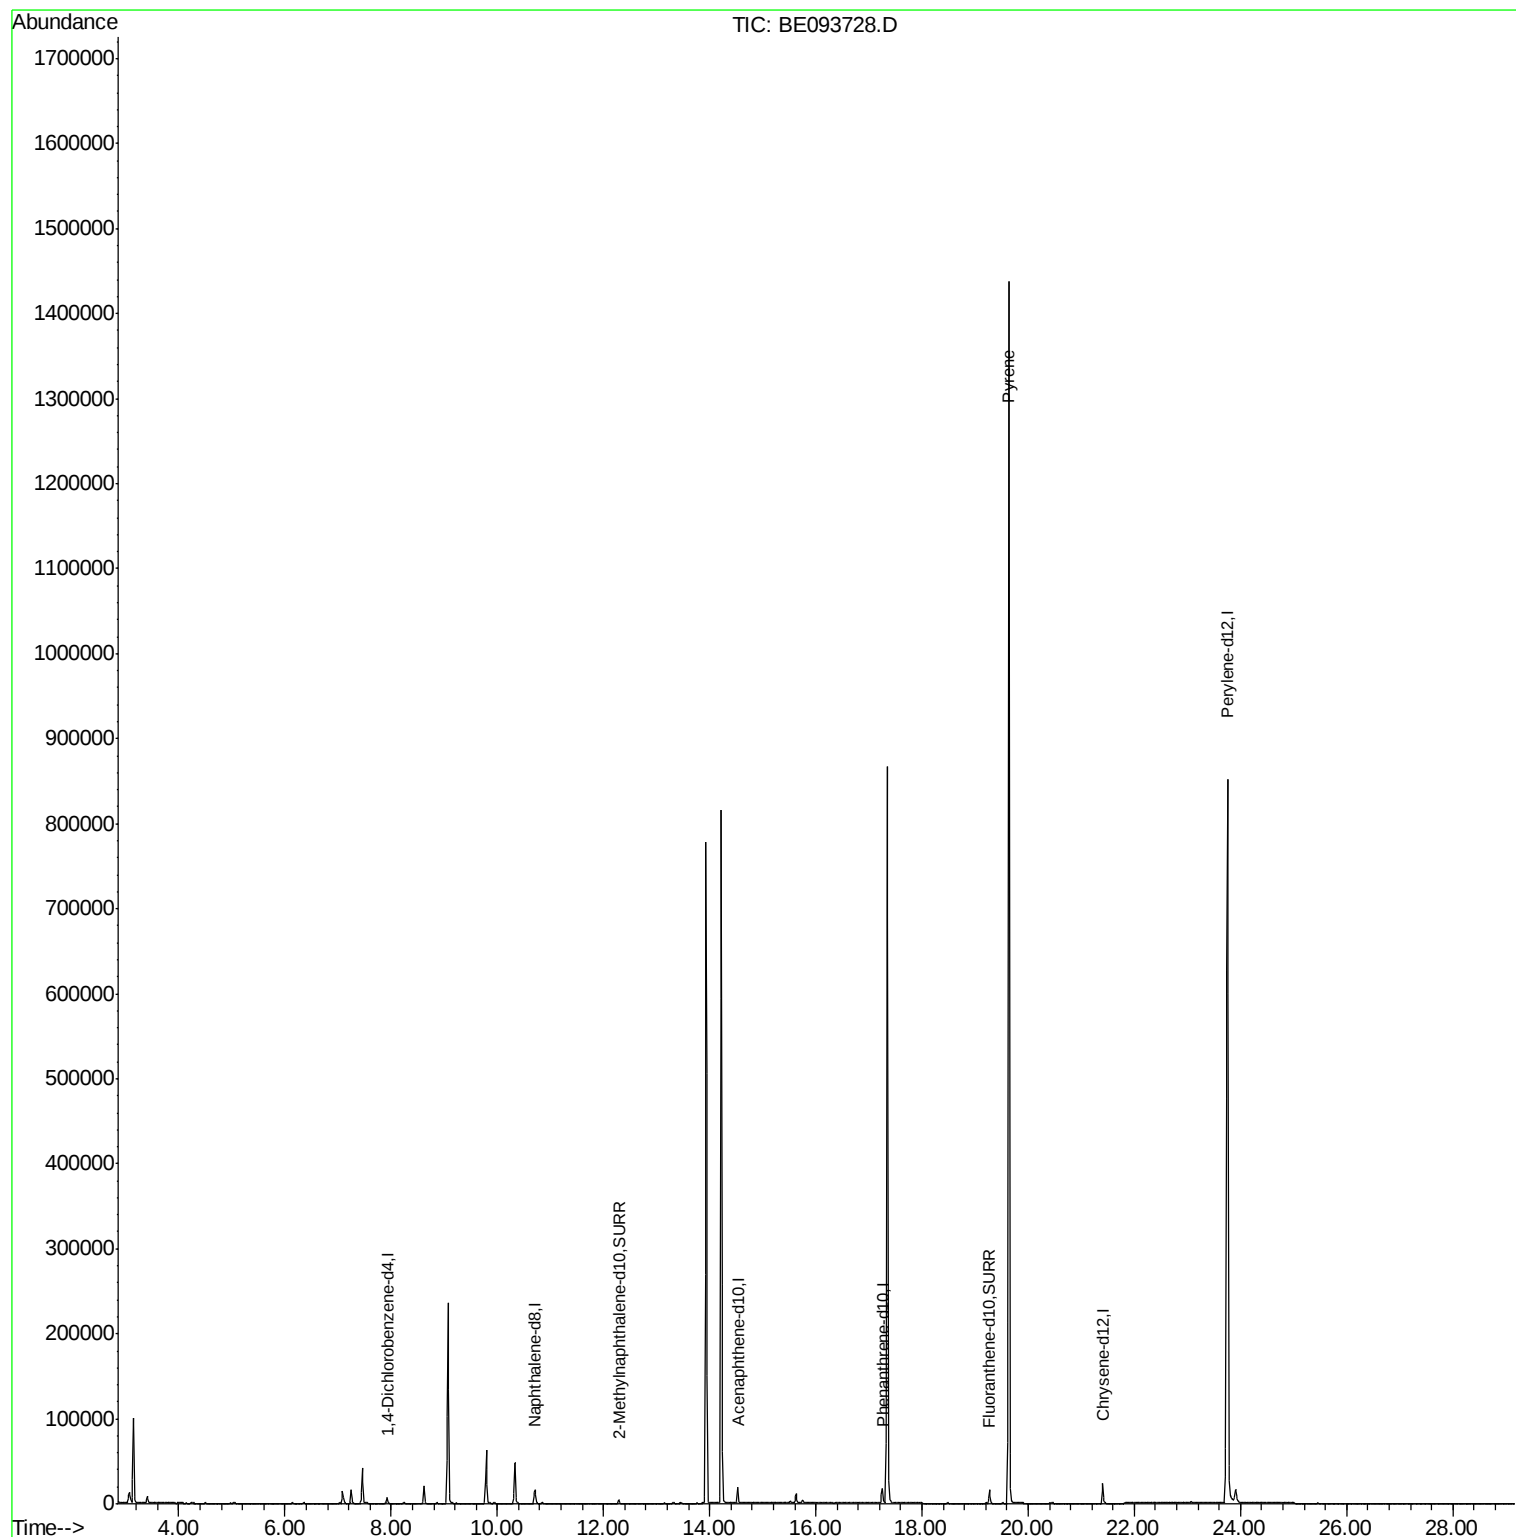


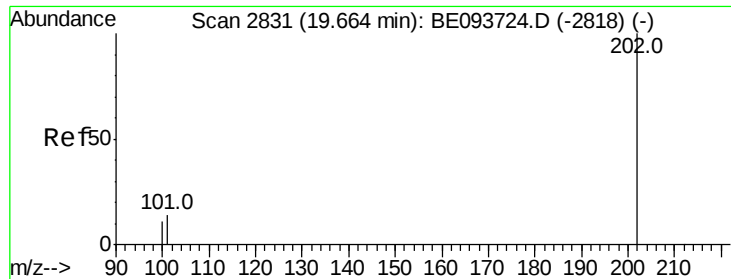

#17
 Pvrene
 Concen: 0.034 ng/ul
 RT: 19.64 min Scan# 2824
 Delta R.T. -0.03 min
 Lab File: BE093728.D
 Acq: 8 Aug 2017 21:46

Instrument :
 BNA_E
 ClientSampleId :
 C0AB0

Tot Ion	Ratio	Lower	Upper
202	100		
101	166.3	18.2	27.4#
100	952.1	15.6	23.4#

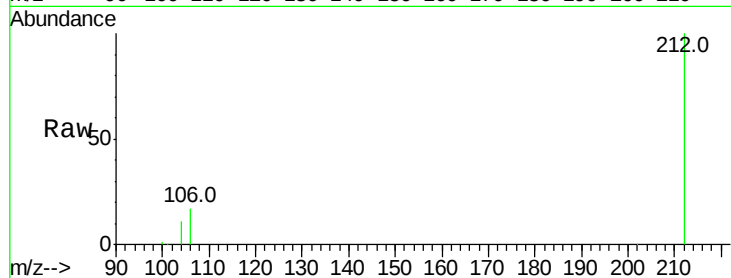

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): BE

