

Data Path : Z:\HPCHEM1\BNA E\DATA\BE080817\
 Data File : BE093731.D
 Acq On : 8 Aug 2017 23:37
 Operator : SJ/JU
 Sample : I4529-16
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AH8

Quant Time: Aug 09 05:33:23 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 09 05:31:57 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.92	152	3253	0.40	ng/ul	0.00
2) Naphthalene-d8	10.71	136	17158	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.52	164	10956	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.26	188	23239	0.40	ng/ul	0.00
16) Chrysene-d12	21.41	240	22766	0.40	ng/ul	0.00
20) Perylene-d12	23.75	264	1373206	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.29	152	7006	0.25	ng/ul	0.00
14) Fluoranthene-d10	19.27	212	17943	0.24	ng/ul	0.00
Target Compounds				Ovalue		
3) Naphthalene	10.75	128	6378	0.153	ng/ul#	94
5) 2-Methylnaphthalene	12.36	142	1719	0.056	ng/ul	99
8) Acenaphthene	14.60	153	2940	0.082	ng/ul#	24
17) Pyrene	19.64	202	2386	0.036	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE080817\
Data File : BE093731.D
Acq On : 8 Aug 2017 23:37
Operator : SJ/JU
Sample : I4529-16
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AH8

Quant Time: Aug 09 05:33:23 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 09 05:31:57 2017
Response via : Initial Calibration

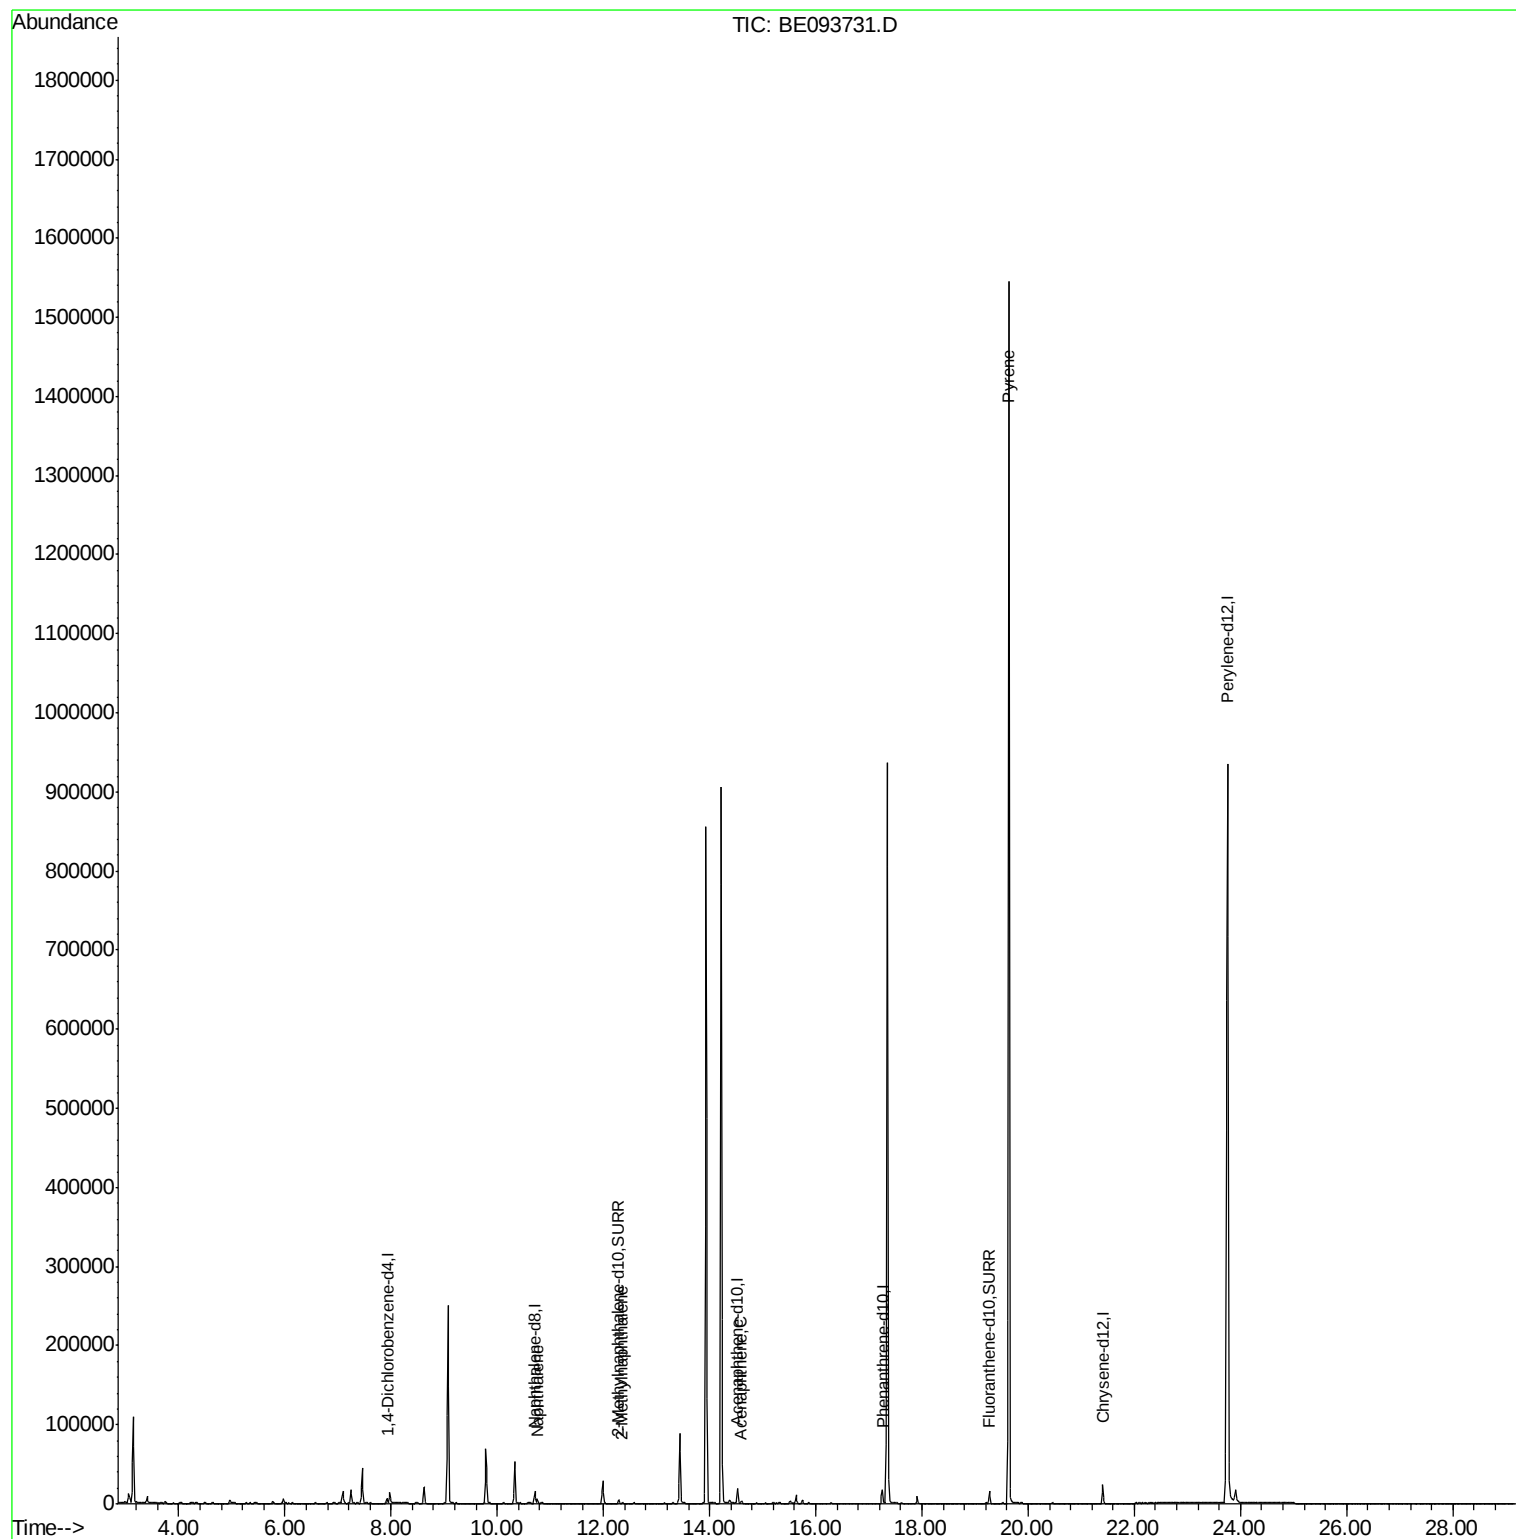

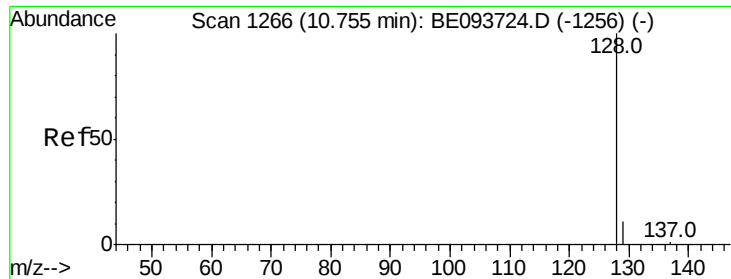

#3

Naphthalene

Concen: 0.153 ng/ul

RT: 10.75 min Scan# 1266

Delta R.T. -0.00 min

Lab File: BE093731.D

Acq: 8 Aug 2017 23:37

Instrument :

BNA_E

ClientSampleId :

C0AH8


Tot Ion:128 Resp: 6378

Ion Ratio Lower Upper

128 100

129 12.9 11.3 16.9




127 0.0 4.0 6.0#

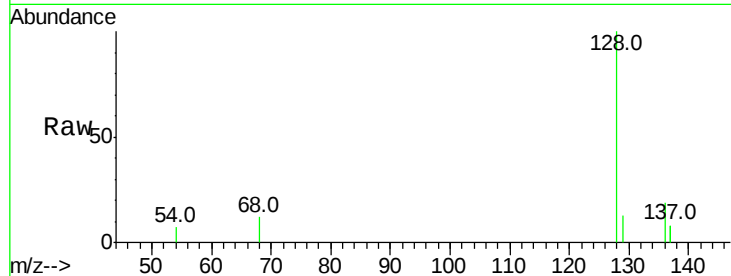

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

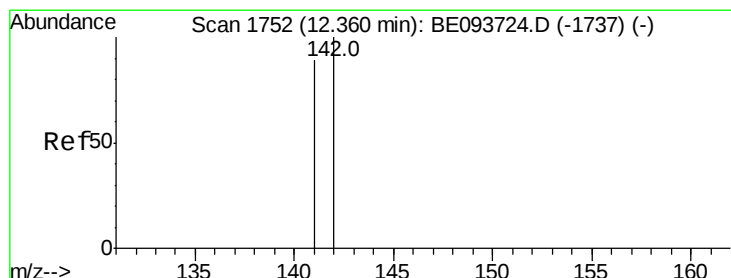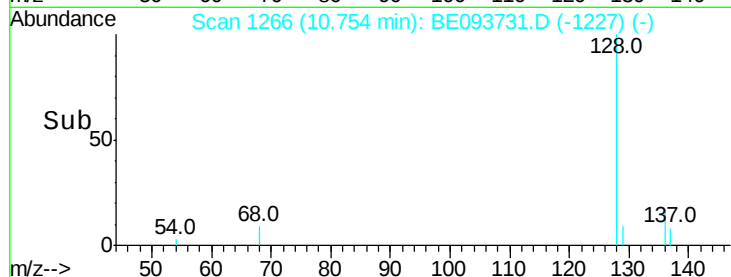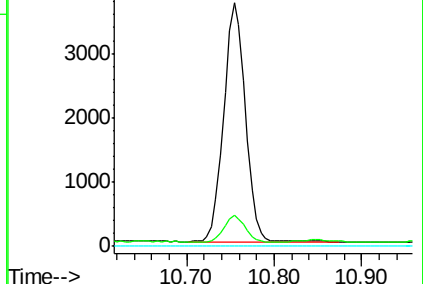

#5

2-Methylnaphthalene

Concen: 0.056 ng/ul

RT: 12.36 min Scan# 1752

Delta R.T. -0.00 min

Lab File: BE093731.D


Acq: 8 Aug 2017 23:37

Tgt Ion:142 Resp: 1719

Ion Ratio Lower Upper



142 100


141 91.3 72.6 108.8

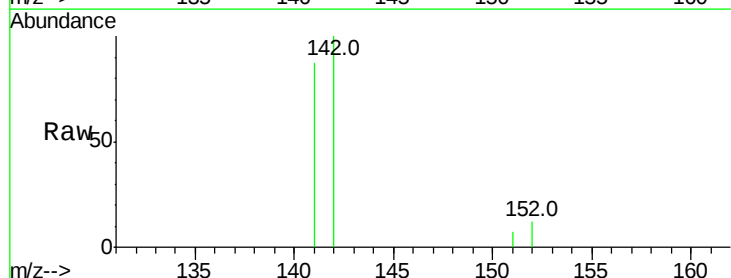

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

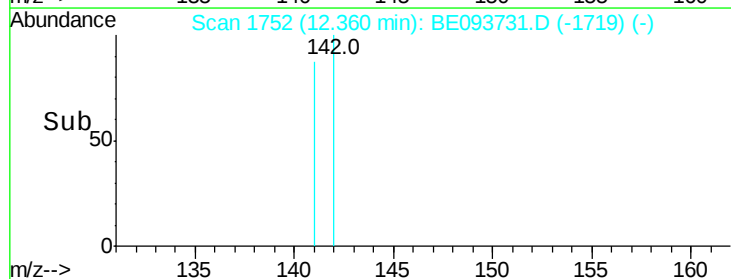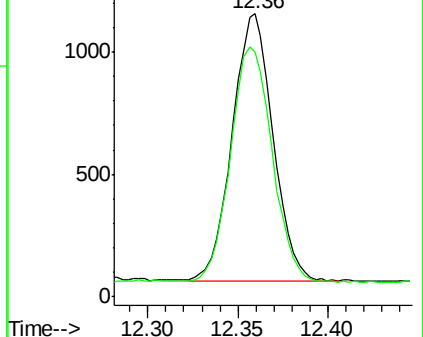

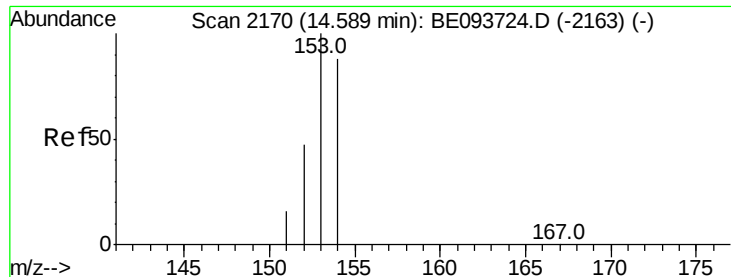

#8

Acenaphthene

Concen: 0.082 ng/ul

RT: 14.60 min Scan# 2171

Delta R.T. 0.01 min

Lab File: BE093731.D

Acq: 8 Aug 2017 23:37

Instrument :

BNA_E

ClientSampleId :

C0AH8


Tot Ion:153 Resp: 2940

Ion Ratio Lower Upper

153 100

152 5.7 40.3 60.5#




154 12.7 71.4 107.2#

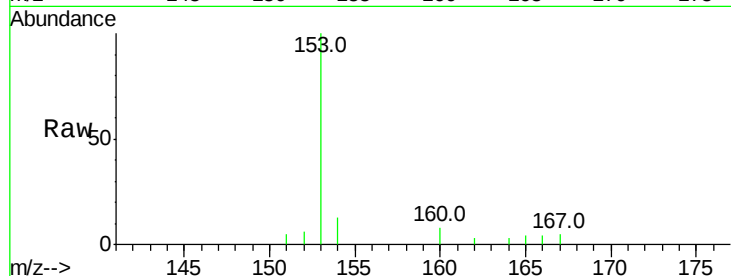

Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

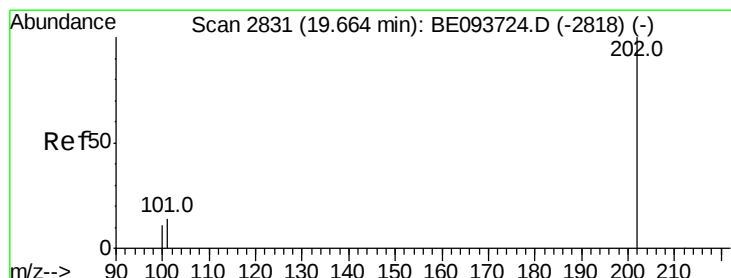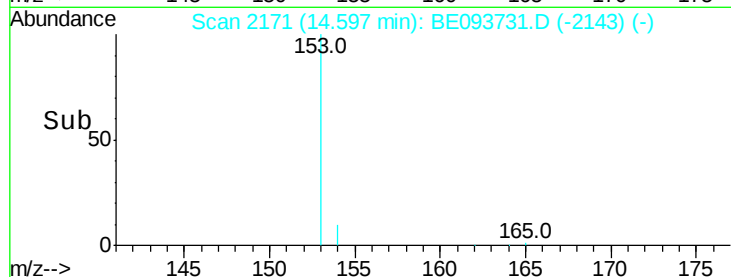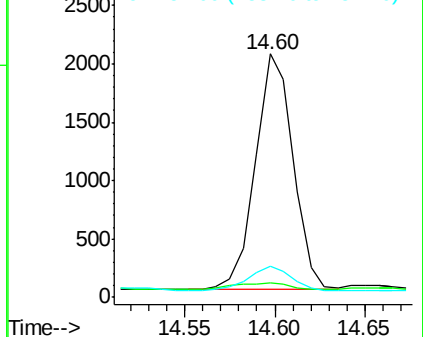

#17

Pyrene

Concen: 0.036 ng/ul

RT: 19.64 min Scan# 2825

Delta R.T. -0.03 min

Lab File: BE093731.D

Acq: 8 Aug 2017 23:37


Tgt Ion:202 Resp: 2386

Ion Ratio Lower Upper

202 100

101 178.9 18.2 27.4#

100 1026.4 15.6 23.4#

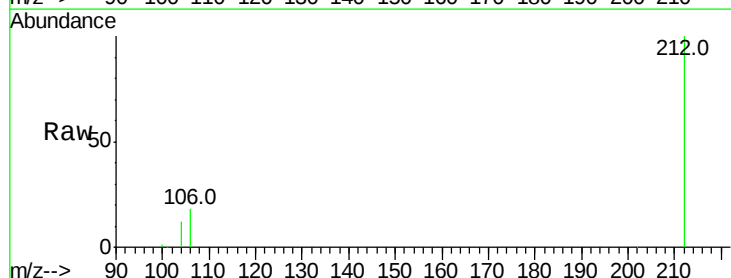

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): E

