

Data Path : Z:\HPCHEM1\BNA E\DATA\BE080817\
 Data File : BE093733.D
 Acq On : 9 Aug 2017 00:51
 Operator : SJ/JU
 Sample : PB101303BL
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SBLK03

Quant Time: Aug 09 05:33:46 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 09 05:31:57 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.92	152	3443	0.40	ng/ul	0.00
2) Naphthalene-d8	10.71	136	18264	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.53	164	11483	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.26
16) Chrysene-d12	21.41	240	23393	0.40	ng/ul	0.00
20) Perylene-d12	23.76	264	1625731	0.40	ng/ul	-0.15
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.29	152	8701	0.29	ng/ul	0.00
14) Fluoranthene-d10	19.27	212	20750	0.00	ng/ul	0.00
Target Compounds						
					Ovalue	
9) Fluorene	15.51	166	2706	0.057	ng/ul#	20
17) Pyrene	19.64	202	2705	0.040	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE080817\
Data File : BE093733.D
Acq On : 9 Aug 2017 00:51
Operator : SJ/JU
Sample : PB101303BL
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK03

Quant Time: Aug 09 05:33:46 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 09 05:31:57 2017
Response via : Initial Calibration

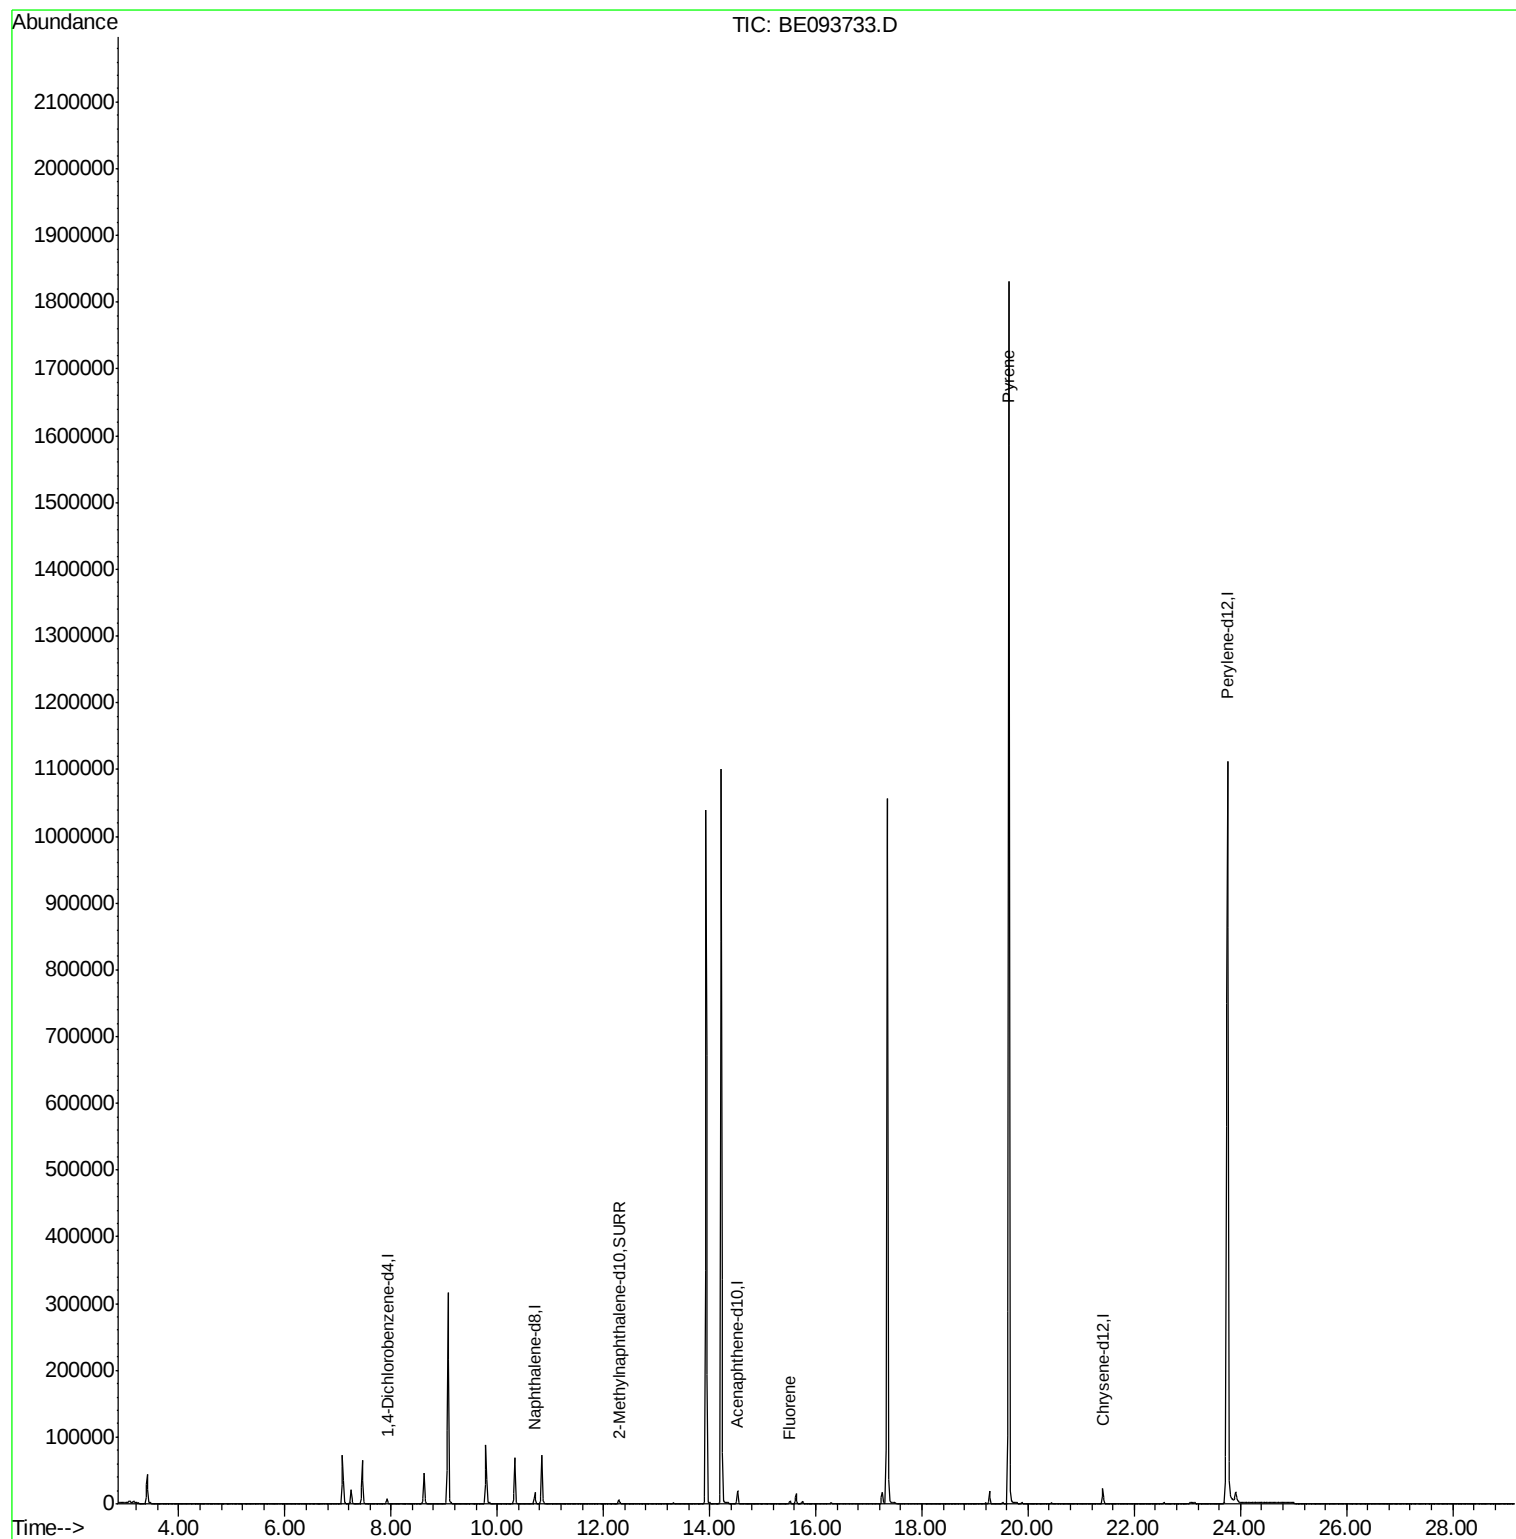

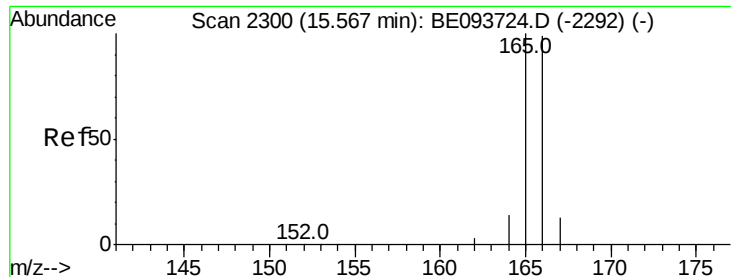

#9

Fluorene

Concen: 0.057 ng/ul

RT: 15.51 min Scan# 2293

Delta R.T. -0.05 min

Lab File: BE093733.D

Acq: 9 Aug 2017 00:51

Instrument :

BNA_E

ClientSampleId :

SBLK03


Tot Ion:166 Resp: 2706

Ion Ratio Lower Upper

166 100

165 5.8 73.4 110.2#




167 30.0 14.6 22.0#

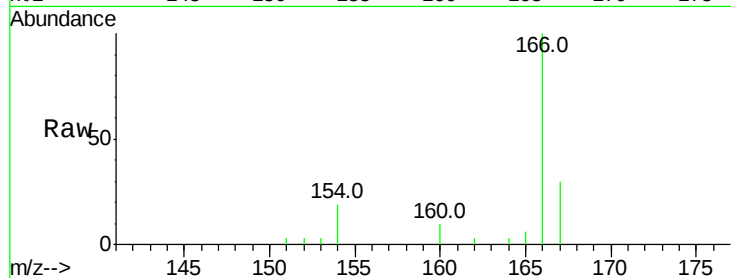

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

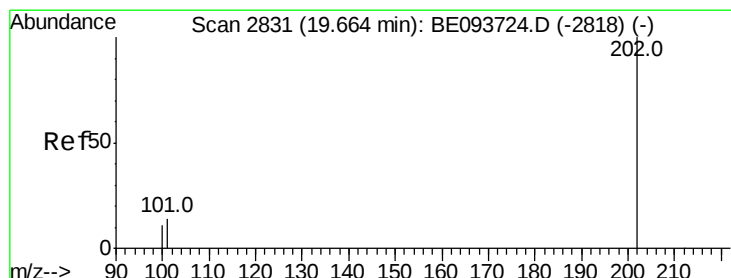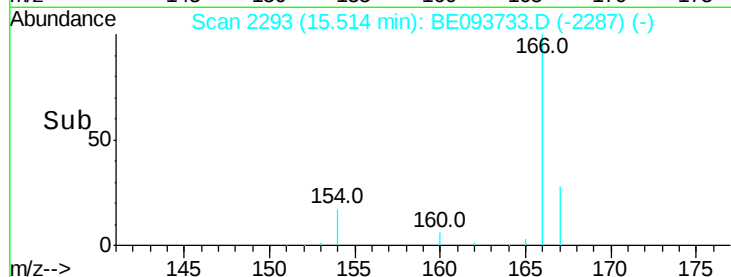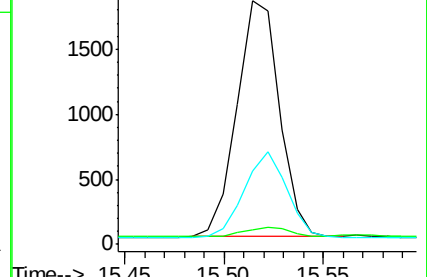

#17

Pyrene

Concen: 0.040 ng/ul

RT: 19.64 min Scan# 2825

Delta R.T. -0.03 min

Lab File: BE093733.D

Acq: 9 Aug 2017 00:51


Tgt Ion:202 Resp: 2705

Ion Ratio Lower Upper

202 100

101 175.0 18.2 27.4#

100 989.1 15.6 23.4#

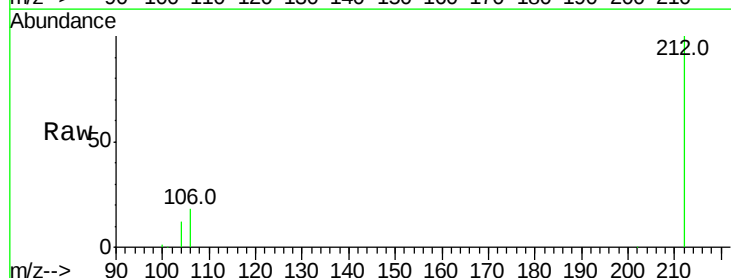

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): E

