

Data Path : Z:\HPCHEM1\BNA E\DATA\BE080817\
 Data File : BE093737.D
 Acq On : 9 Aug 2017 3:20
 Operator : SJ/JU
 Sample : I4557-05
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AC8

Quant Time: Aug 09 05:34:26 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 09 05:31:57 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.92	152	3378	0.40	ng/ul	0.00
2) Naphthalene-d8	10.70	136	17283	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.53	164	10811	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.26
16) Chrysene-d12	21.41	240	23134	0.40	ng/ul	0.00
20) Perylene-d12	23.76	264	1513166	0.40	ng/ul	-0.15
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.29	152	7177	0.26	ng/ul	0.00
14) Fluoranthene-d10	19.27	212	20845	0.00	ng/ul	0.00
Target Compounds						
9) Fluorene	15.51	166	2491	0.055	ng/ul#	22
17) Pyrene	19.64	202	2760	0.041	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE080817\
Data File : BE093737.D
Acq On : 9 Aug 2017 3:20
Operator : SJ/JU
Sample : I4557-05
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AC8

Quant Time: Aug 09 05:34:26 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 09 05:31:57 2017
Response via : Initial Calibration

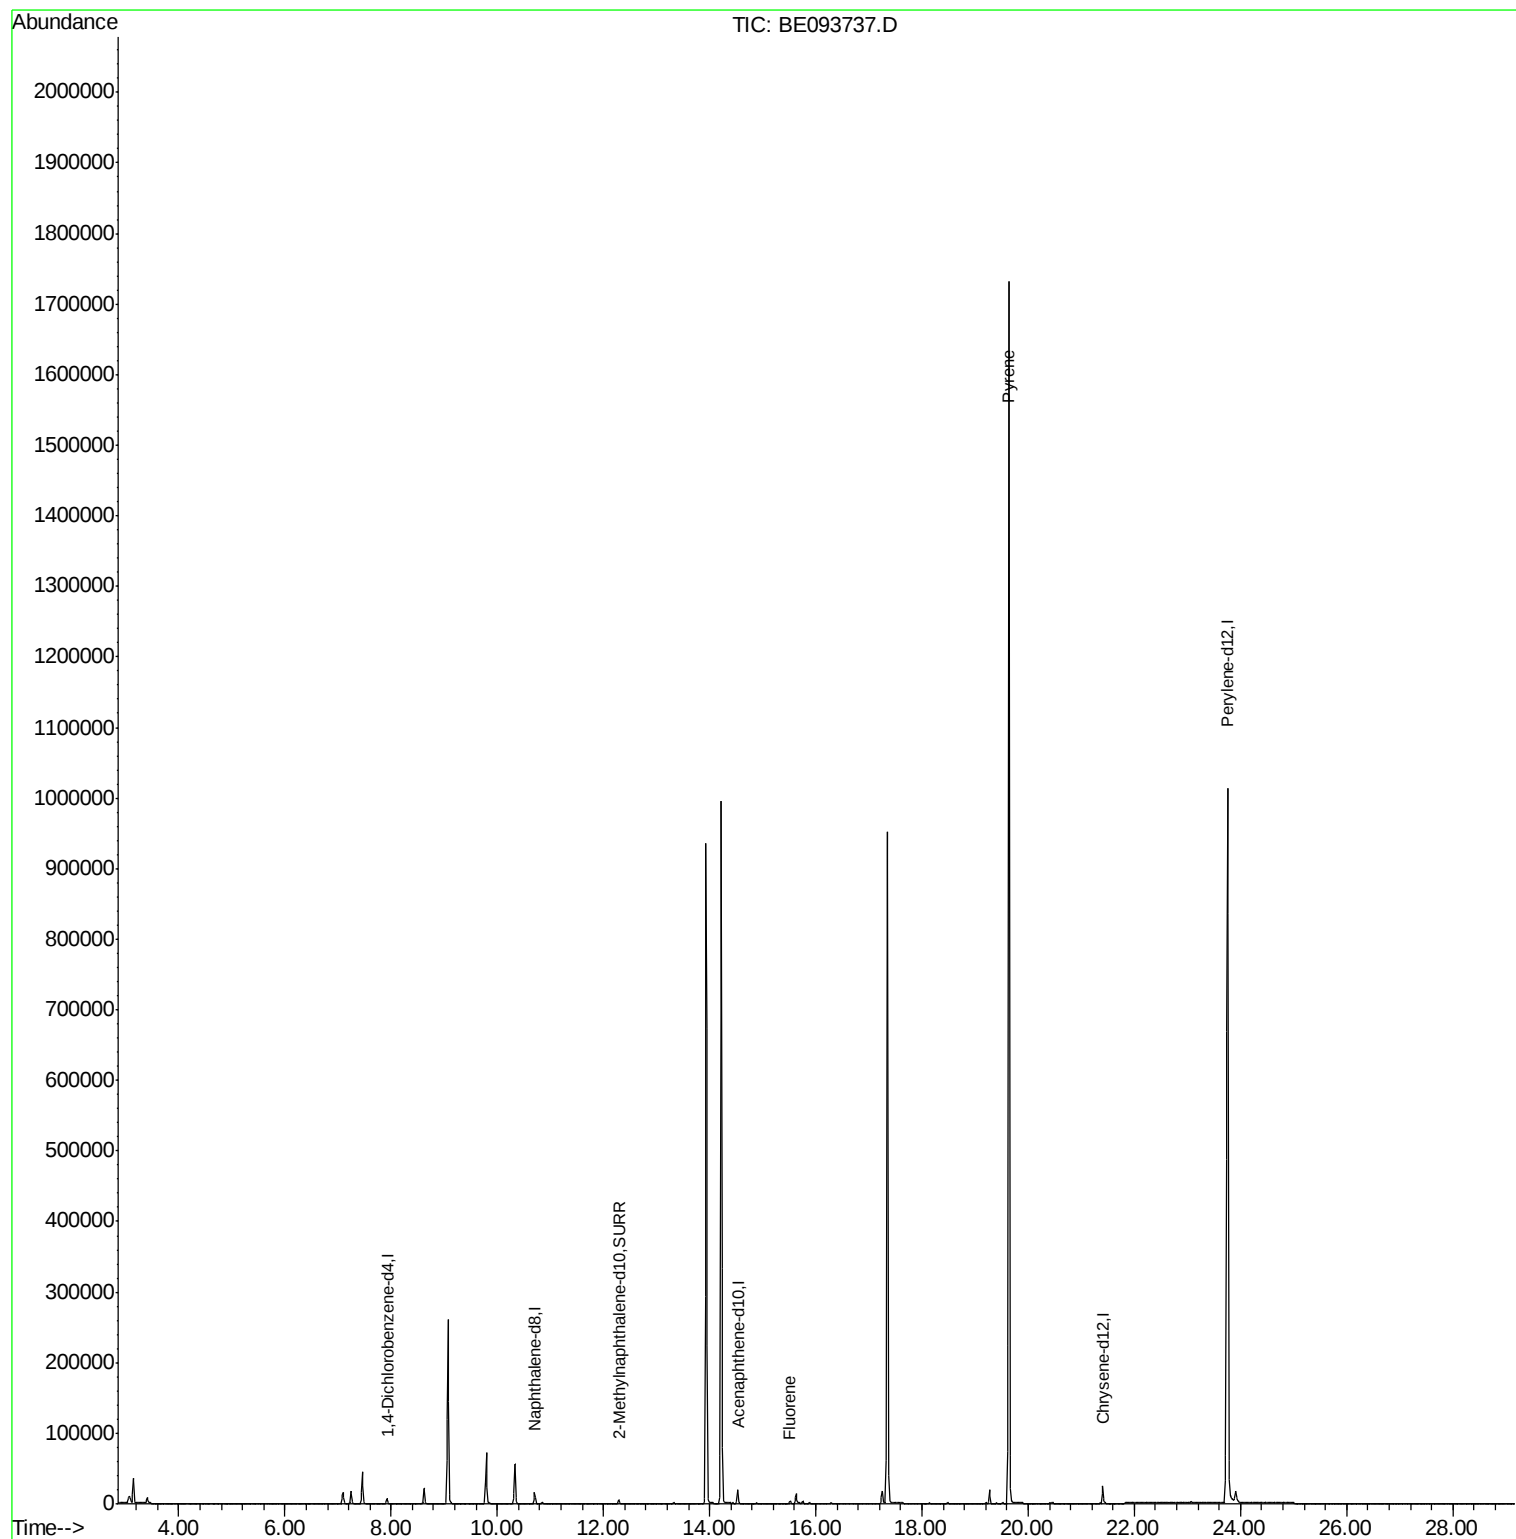

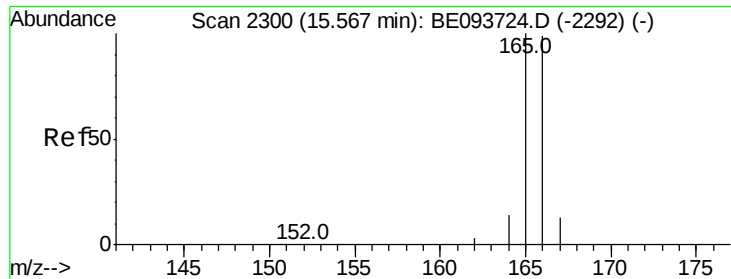

#9

Fluorene

Concen: 0.055 ng/ul

RT: 15.51 min Scan# 2292

Delta R.T. -0.05 min

Lab File: BE093737.D

Acq: 9 Aug 2017 3:20

Instrument :

BNA_E

ClientSampleId :

C0AC8





Tot Ion:166 Resp: 2491

Ion Ratio Lower Upper

166 100

165 7.8 73.4 110.2#

167 30.8 14.6 22.0#

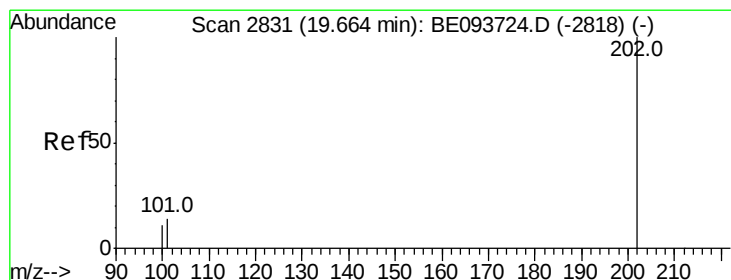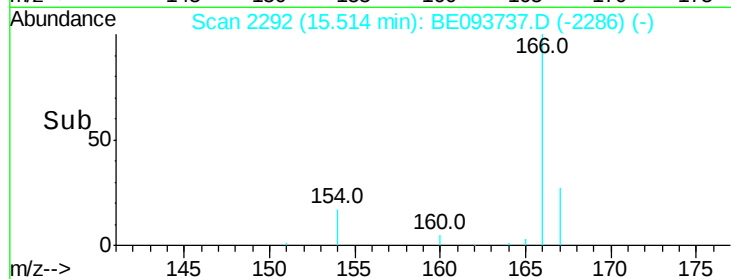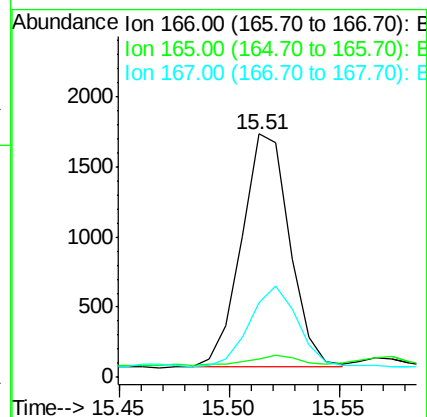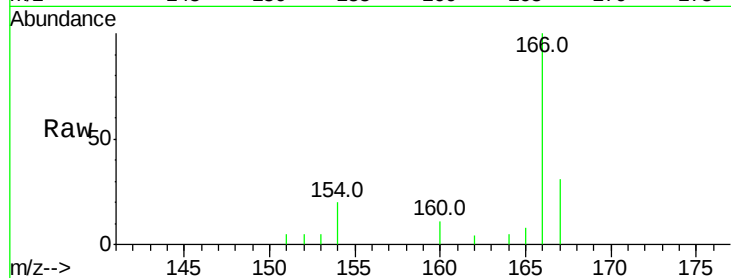

#17

Pyrene

Concen: 0.041 ng/ul

RT: 19.64 min Scan# 2824

Delta R.T. -0.03 min

Lab File: BE093737.D

Acq: 9 Aug 2017 3:20

Tgt Ion:202 Resp: 2760

Ion Ratio Lower Upper

202 100

101 170.0 18.2 27.4#

100 993.5 15.6 23.4#

