




Data Path : Z:\HPCHEM1\BNA E\DATA\BE080817\
 Data File : BE093719.D
 Acq On : 8 Aug 2017 16:12
 Operator : SJ/JU
 Sample : I4504-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 C0AE3

Manual Integrations
 APPROVED

Sohil
 8/9/2017 7:14:26 PM

Quant Time: Aug 09 04:22:17 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 09 04:20:36 2017
 Response via : Initial Calibration

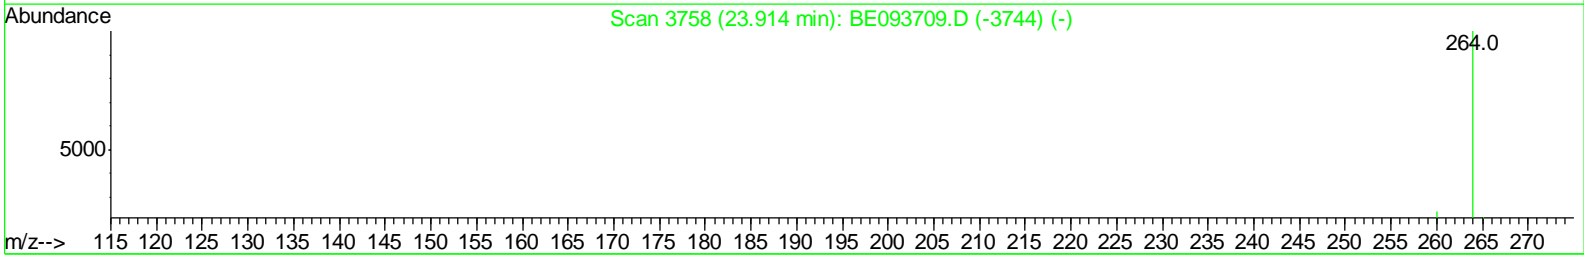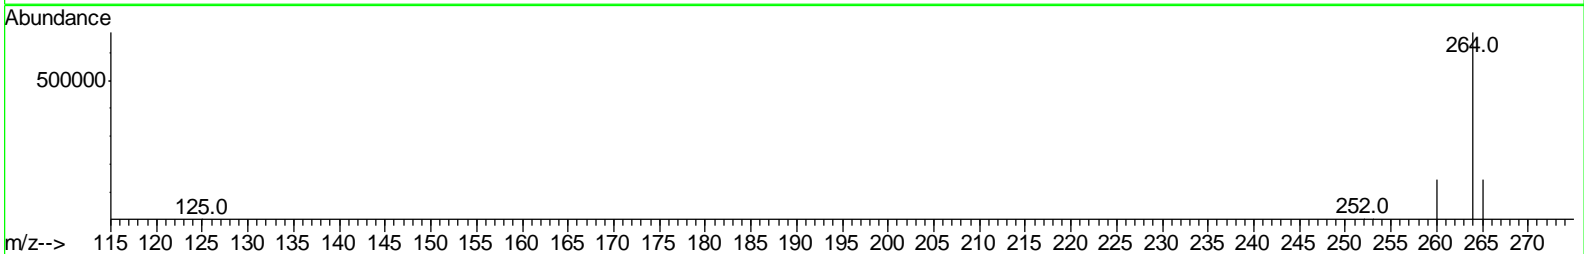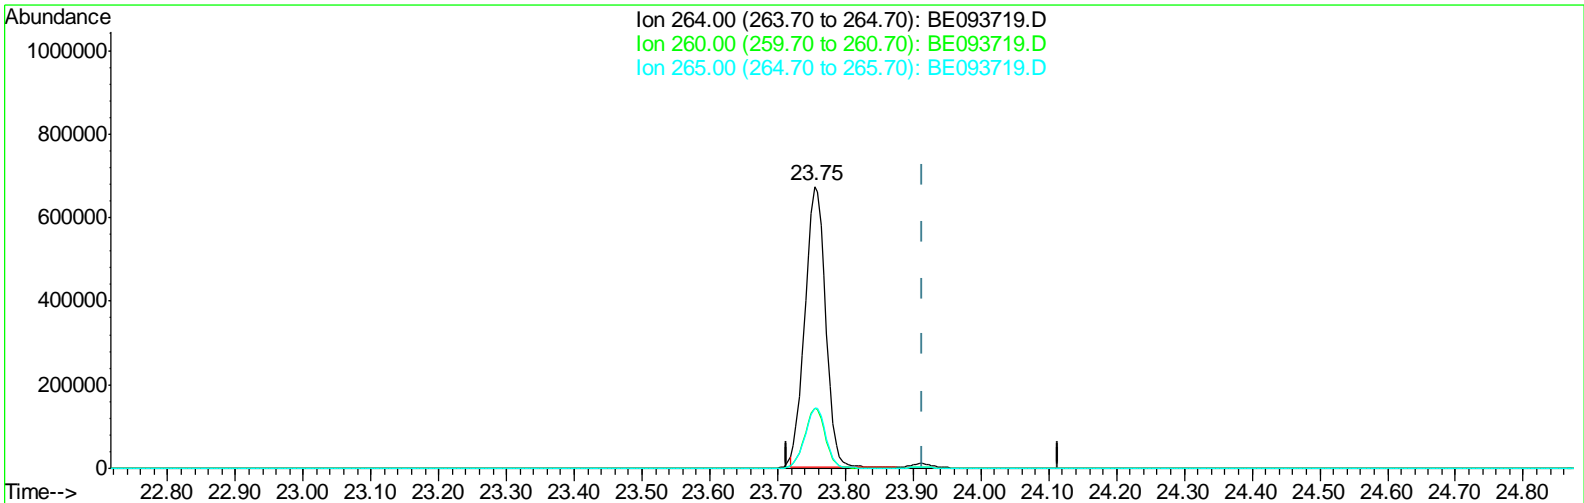

TIC: BE093719.D

(20) Perylene-d12 (I)
 23.755min (-0.159) 0.40ng/ul
 response 1425911

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.46#
265.00	103.50	21.56#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE080817\
 Data File : BE093719.D
 Acq On : 8 Aug 2017 16:12
 Operator : SJ/JU
 Sample : I4504-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 C0AE3

Manual Integrations
 APPROVED

Sohil
 8/9/2017 7:14:26 PM

Quant Time: Aug 09 04:22:17 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 09 04:20:36 2017
 Response via : Initial Calibration

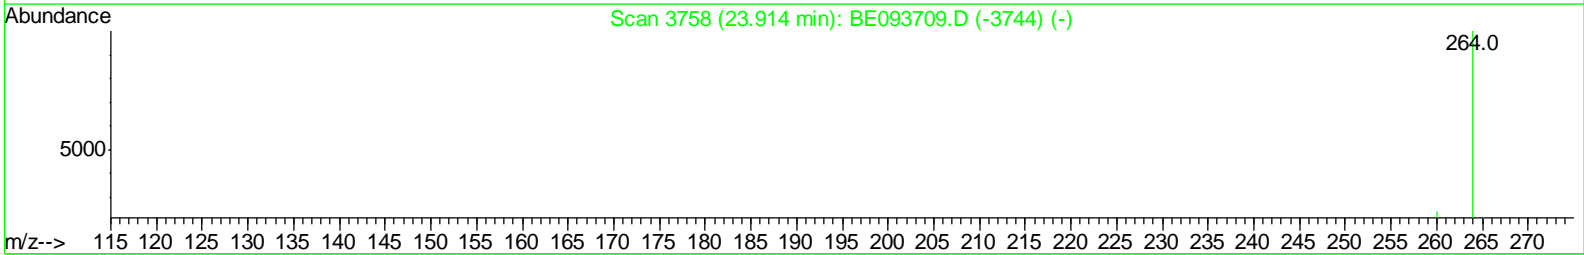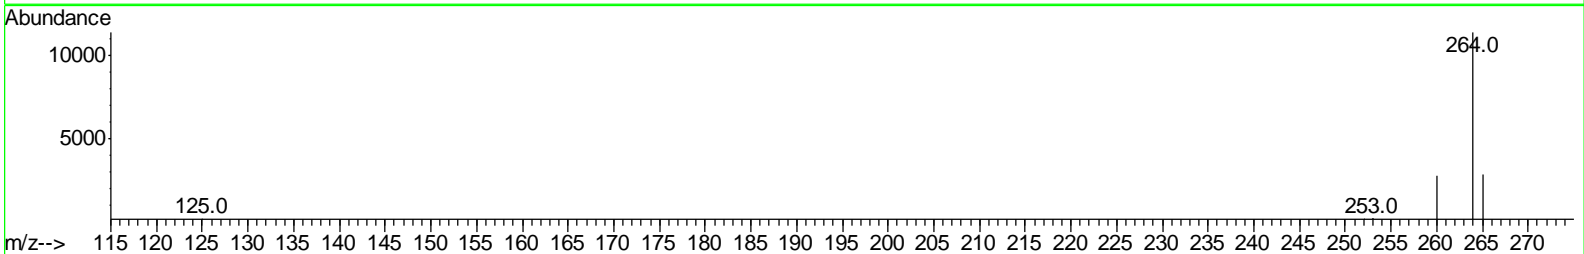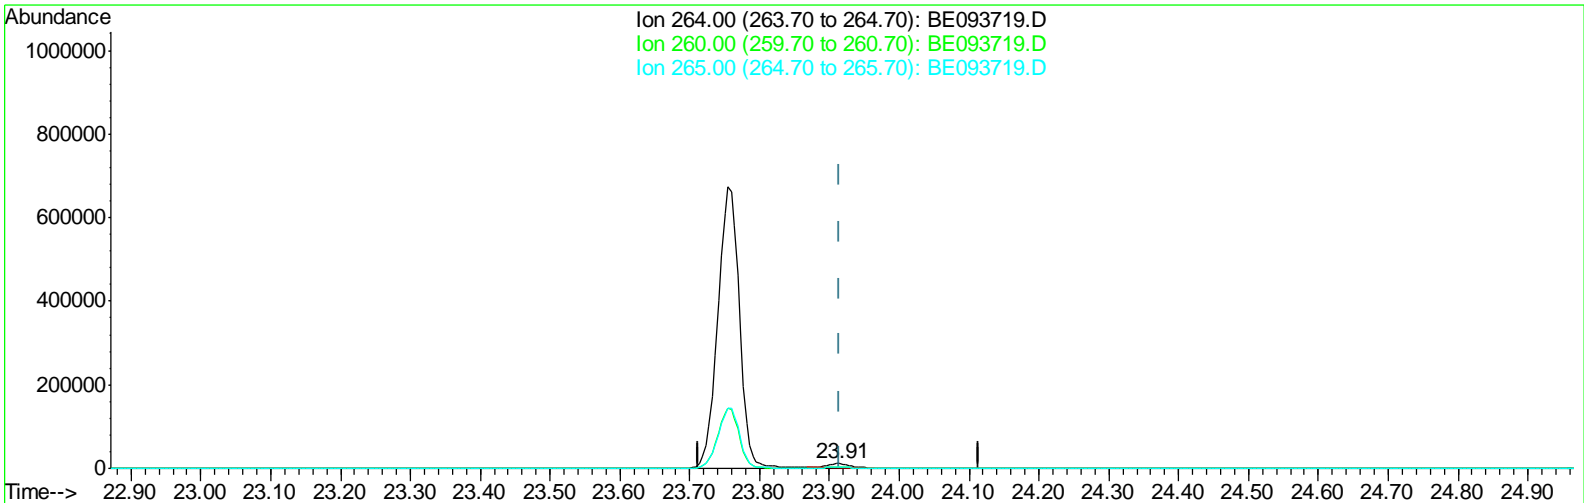

TIC: BE093719.D

(20) Perylene-d12 (I)

23.914min (-0.000) 0.40ng/ul m

response 20359

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	24.33
265.00	103.50	24.79#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE080817\
 Data File : BE093719.D
 Acq On : 8 Aug 2017 16:12
 Operator : SJ/JU
 Sample : I4504-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_E
ClientSampleId :
 C0AE3

Manual Integrations
APPROVED
 Sohil
 8/9/2017 7:14:26 PM

Quant Time: Aug 09 05:09:50 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 09 04:20:36 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.92	152	3529	0.40	ng/ul	0.00
2) Naphthalene-d8	10.71	136	18033	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.53	164	10994	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.26	188	24050	0.40	ng/ul	0.00
16) Chrysene-d12	21.41	240	23841	0.40	ng/ul	0.00
20) Perylene-d12	23.91	264	20359m	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.29	152	6887	0.24	ng/ul	0.00
14) Fluoranthene-d10	19.27	212	18338	0.24	ng/ul	0.00

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE080817\
 Data File : BE093719.D
 Acq On : 8 Aug 2017 16:12
 Operator : SJ/JU
 Sample : I4504-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_E
ClientSampled :
 C0AE3

Manual Integrations
APPROVED
 Sohil
 8/9/2017 7:14:26 PM

Quant Time: Aug 09 05:09:50 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 09 04:20:36 2017
 Response via : Initial Calibration

