




Data Path : Z:\HPCHEM1\BNA E\DATA\BE080817\
Data File : BE093721.D
Acq On : 8 Aug 2017 17:27
Operator : SJ/JU
Sample : I4504-09
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AE8

Manual Integrations
APPROVED

Sohil
8/9/2017 7:14:31 PM

Quant Time: Aug 09 04:22:29 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 09 04:20:36 2017
Response via : Initial Calibration

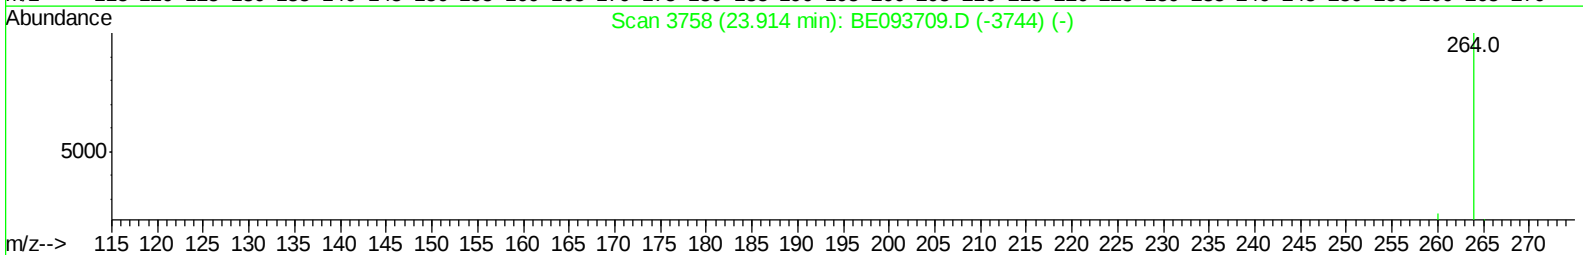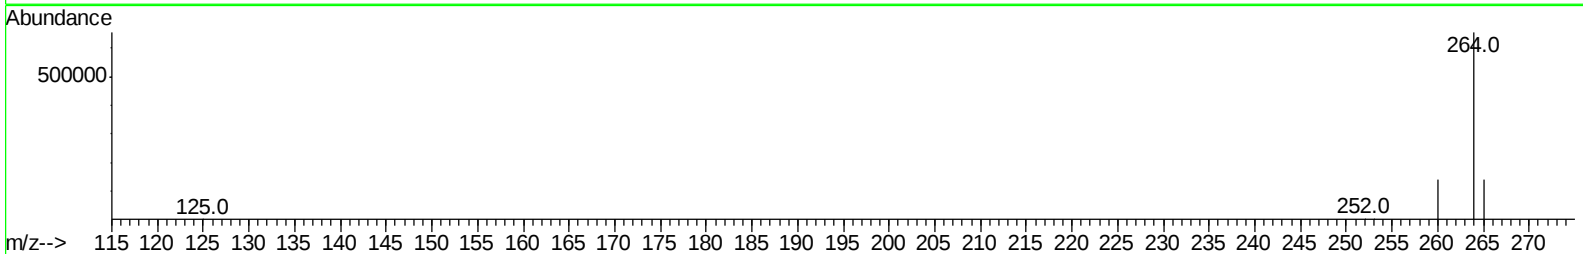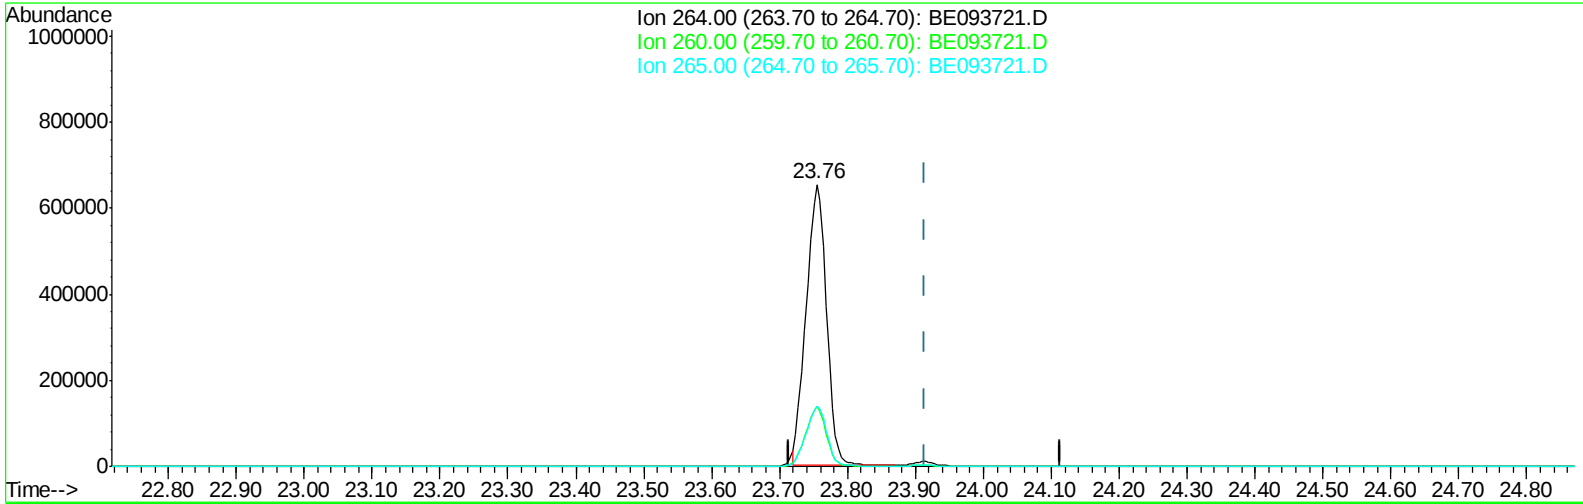

TIC: BE093721.D

(20) Perylene-d12 (I)

23.755min (-0.159) 0.40ng/ul

response 1360286

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.31#
265.00	103.50	21.56#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE080817\
 Data File : BE093721.D
 Acq On : 8 Aug 2017 17:27
 Operator : SJ/JU
 Sample : I4504-09
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AE8

Manual Integrations
 APPROVED

Sohil
 8/9/2017 7:14:31 PM

Quant Time: Aug 09 04:22:29 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 09 04:20:36 2017
 Response via : Initial Calibration

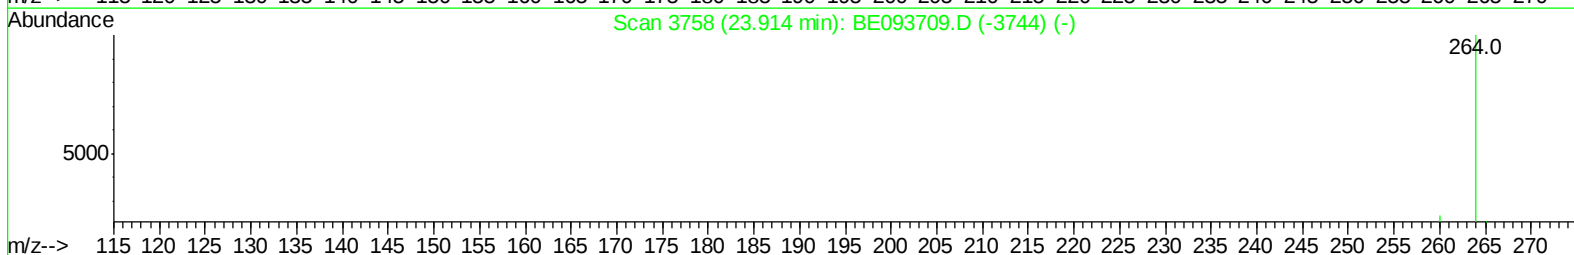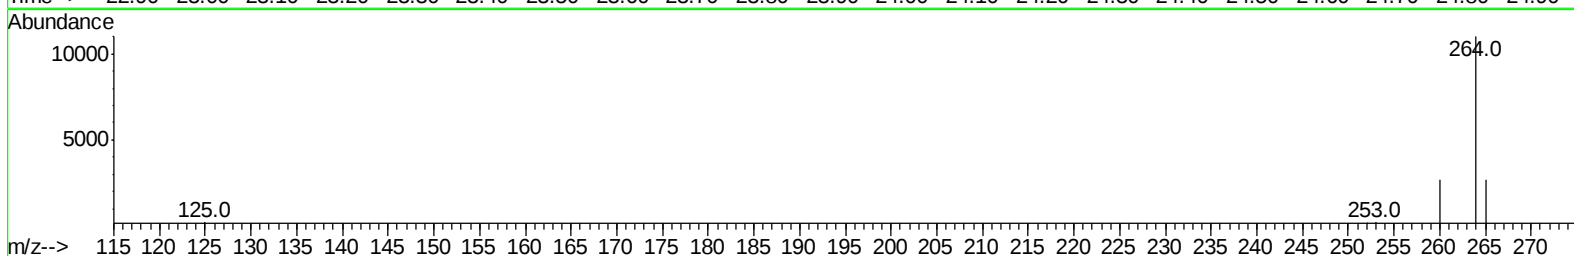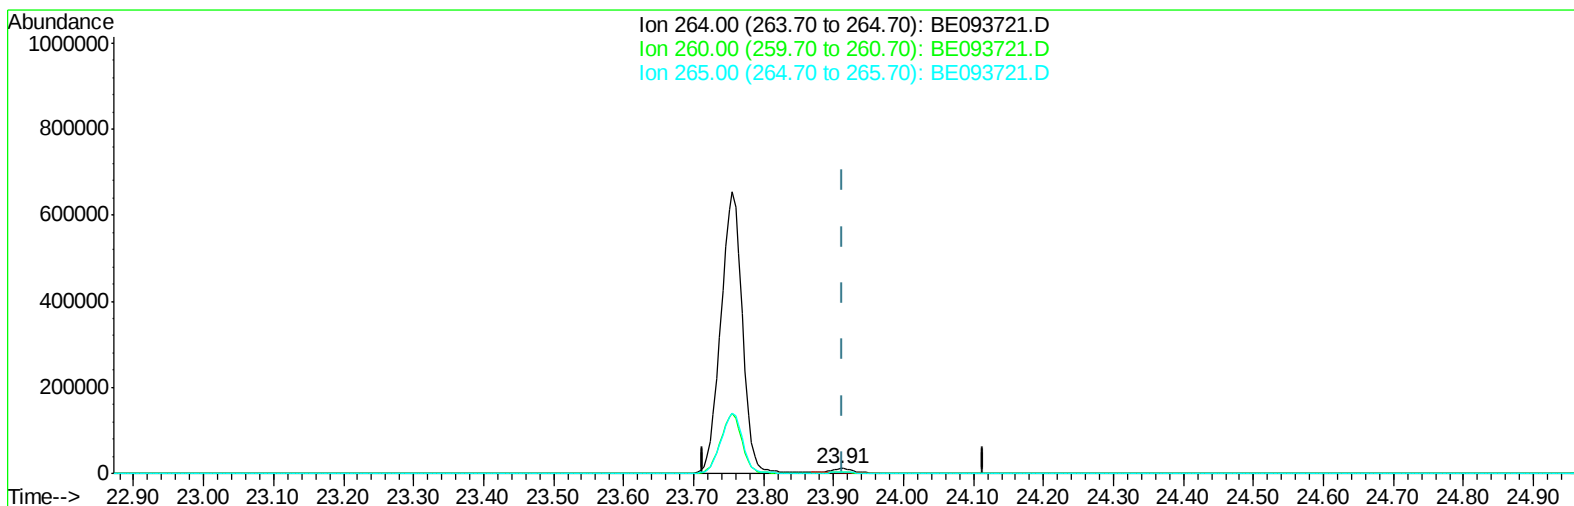

TIC: BE093721.D

(20) Perylene-d12 (I)

23.910min (-0.004) 0.40ng/ul m

response 20153

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	24.17
265.00	103.50	24.29#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE080817\
 Data File : BE093721.D
 Acq On : 8 Aug 2017 17:27
 Operator : SJ/JU
 Sample : I4504-09
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AE8

Manual Integrations
 APPROVED

Sohil
 8/9/2017 7:14:31 PM

Quant Time: Aug 09 05:14:57 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 09 04:20:36 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.92	152	3424	0.40	ng/ul	0.00
2) Naphthalene-d8	10.71	136	17863	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.53	164	11025	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.26	188	23300	0.40	ng/ul	0.00
16) Chrysene-d12	21.41	240	22948	0.40	ng/ul	0.00
20) Perylene-d12	23.91	264	20153m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.29	152	7232	0.25	ng/ul	0.00
14) Fluoranthene-d10	19.27	212	18081	0.25	ng/ul	0.00
Target Compounds						
3) Naphthalene	10.75	128	3704	0.085	ng/ul#	96
5) 2-Methylnaphthalene	12.36	142	1647	0.052	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE080817\
Data File : BE093721.D
Acq On : 8 Aug 2017 17:27
Operator : SJ/JU
Sample : I4504-09
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AE8

Quant Time: Aug 09 05:14:57 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 09 04:20:36 2017
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
8/9/2017 7:14:31 PM

