




Data Path : Z:\HPCHEM1\BNA E\DATA\BE080817\
Data File : BE093734.D
Acq On : 9 Aug 2017 1:30
Operator : SJ/JU
Sample : I4557-06
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AC9

Manual Integrations
APPROVED

Sohil
8/9/2017 7:15:01 PM

Quant Time: Aug 09 05:33:56 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 09 05:31:57 2017
Response via : Initial Calibration

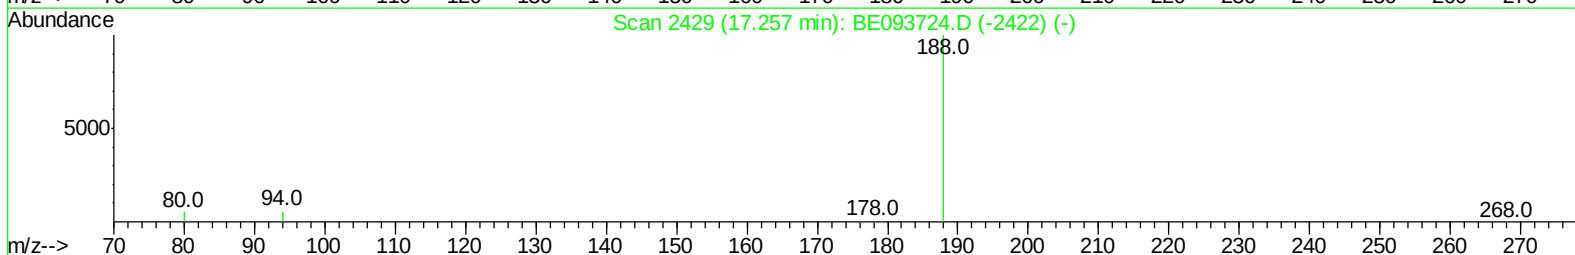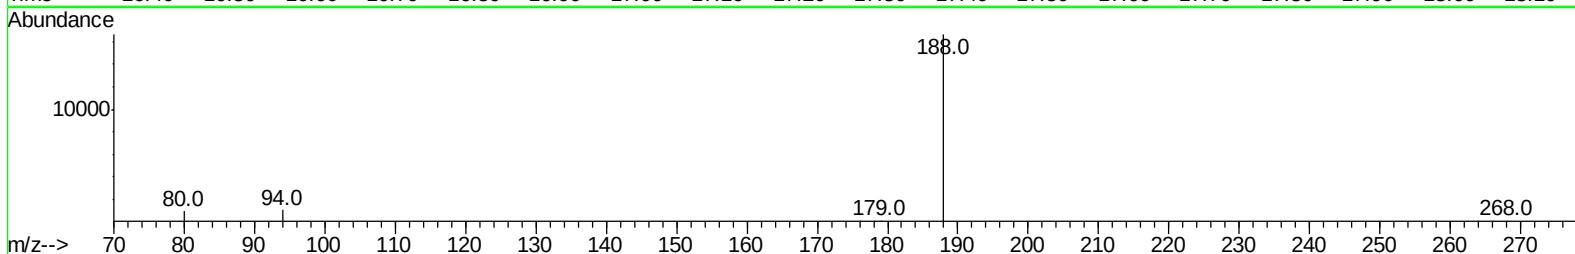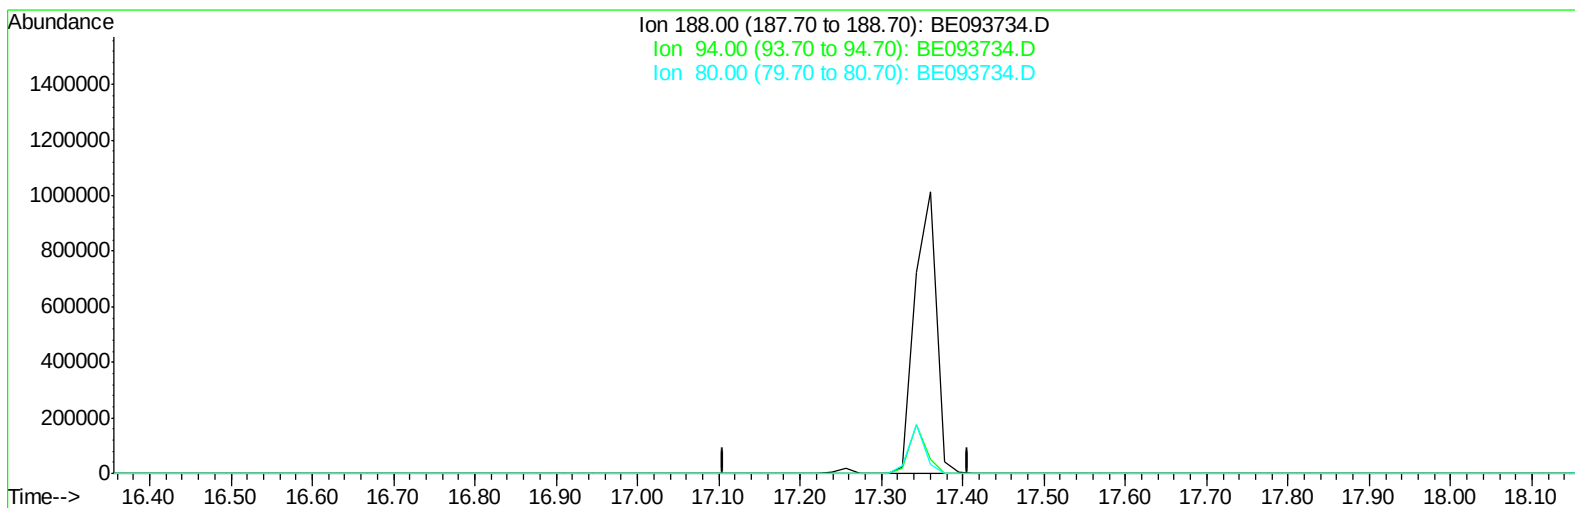

TIC: BE093734.D

(10) Phenanthrene-d10 (I)

17.257min (-17.257) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.00	0.00#
80.00	11.80	0.00#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE080817\
Data File : BE093734.D
Acq On : 9 Aug 2017 1:30
Operator : SJ/JU
Sample : I4557-06
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AC9

Manual Integrations
APPROVED

Sohil
8/9/2017 7:15:01 PM

Quant Time: Aug 09 05:33:56 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 09 05:31:57 2017
Response via : Initial Calibration

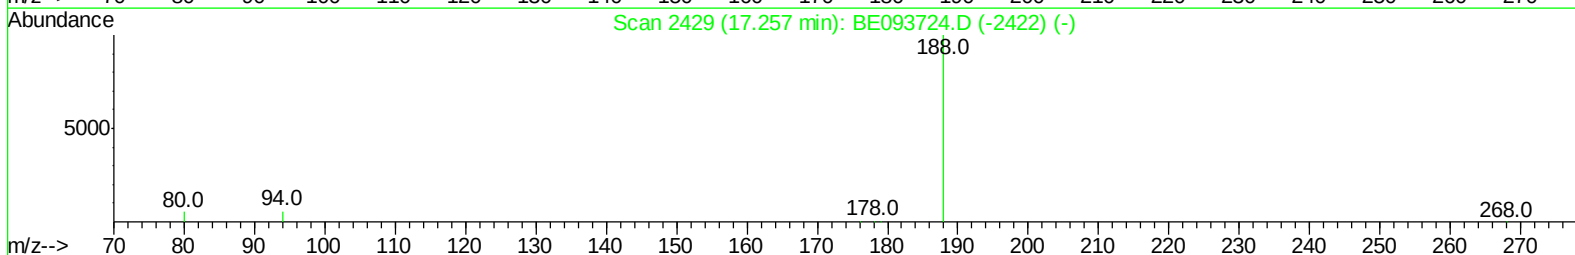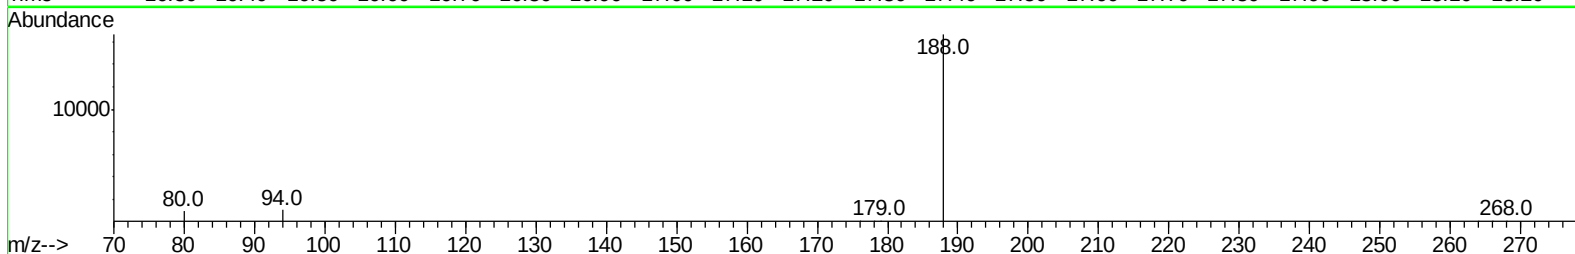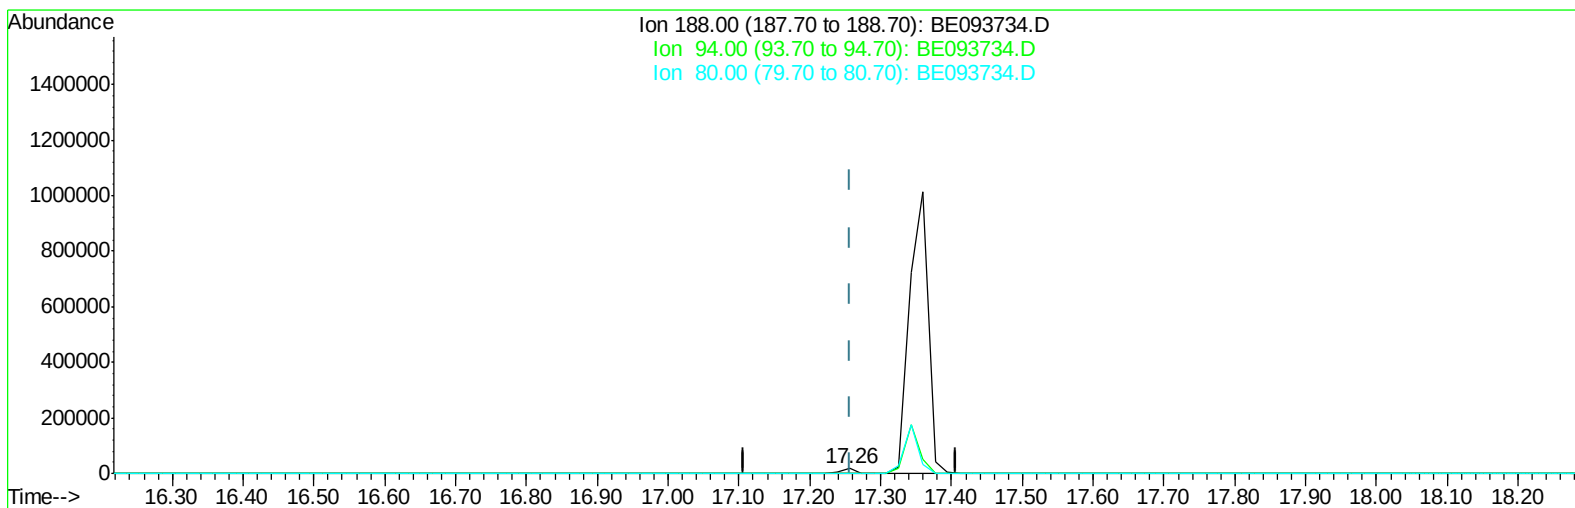

TIC: BE093734.D

(10) Phenanthrene-d10 (I)

17.256min (-0.001) 0.40ng/ul m

response 25566

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	6.20#
80.00	11.80	5.61#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE080817\
Data File : BE093734.D
Acq On : 9 Aug 2017 1:30
Operator : SJ/JU
Sample : I4557-06
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AC9

Manual Integrations
APPROVED

Sohil
8/9/2017 7:15:01 PM

Quant Time: Aug 09 06:47:05 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 09 05:31:57 2017
Response via : Initial Calibration

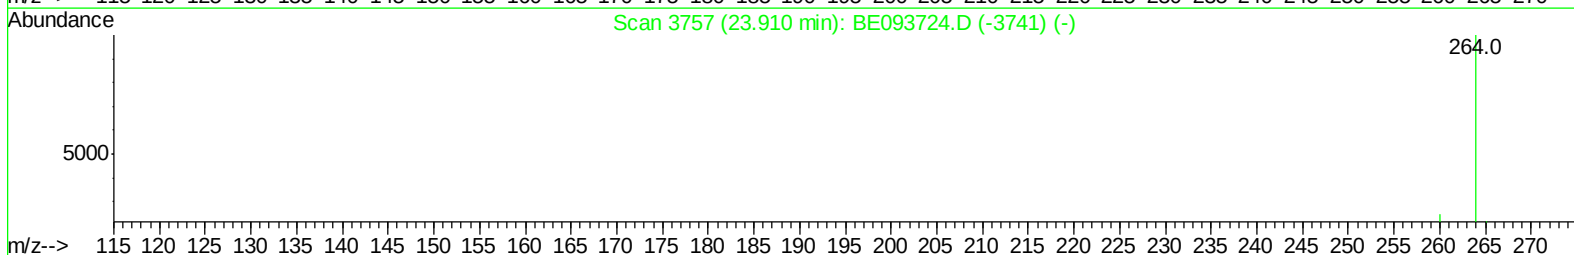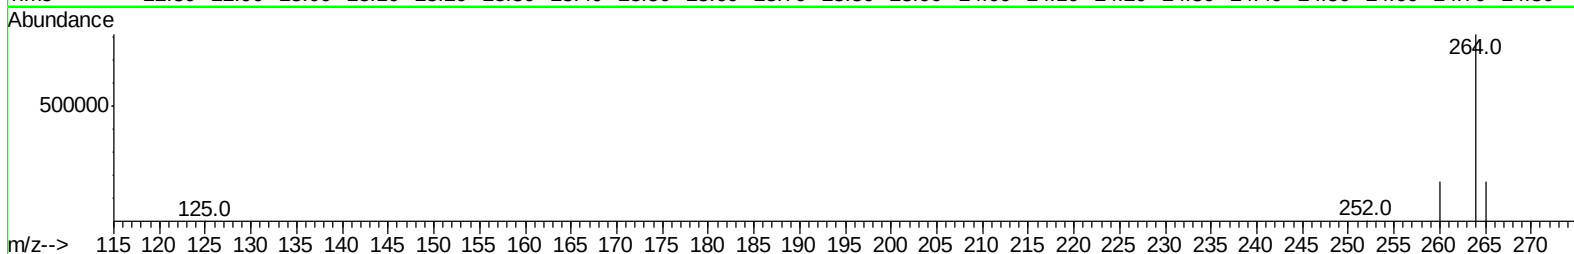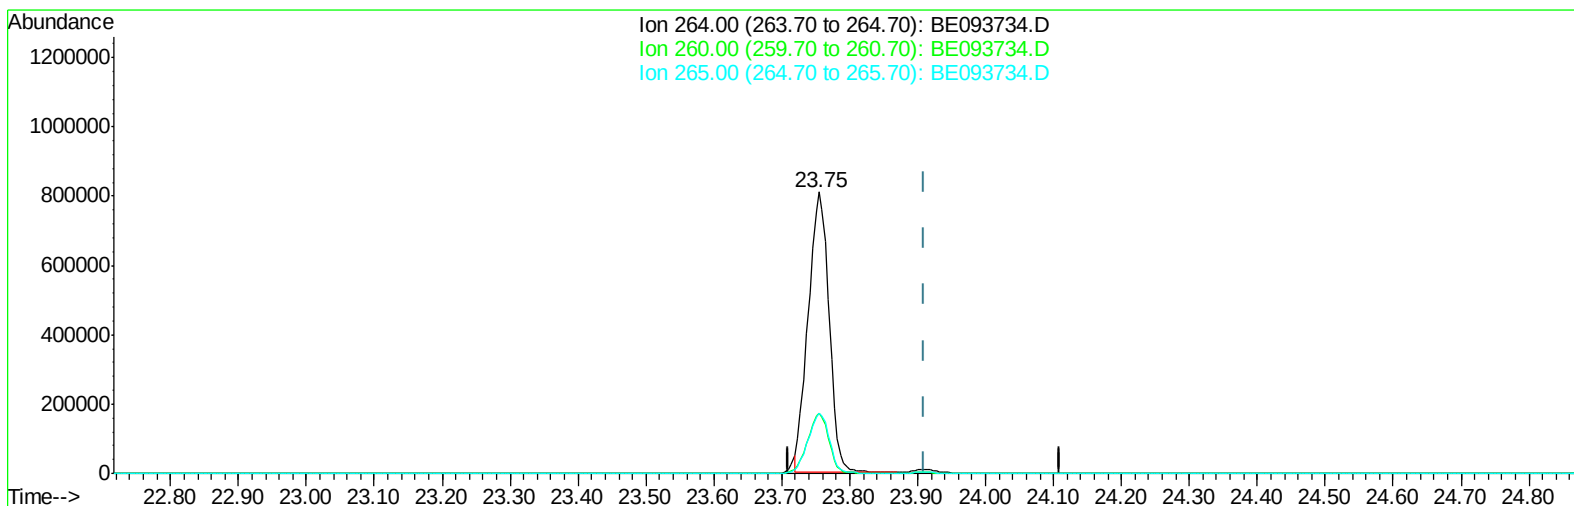

TIC: BE093734.D

(20) Perylene-d12 (I)

23.755min (-0.155) 0.40ng/ul

response 1728332

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.44#
265.00	103.50	21.49#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE080817\
 Data File : BE093734.D
 Acq On : 9 Aug 2017 1:30
 Operator : SJ/JU
 Sample : I4557-06
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AC9

Manual Integrations
 APPROVED

Sohil
 8/9/2017 7:15:01 PM

Quant Time: Aug 09 06:47:05 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 09 05:31:57 2017
 Response via : Initial Calibration

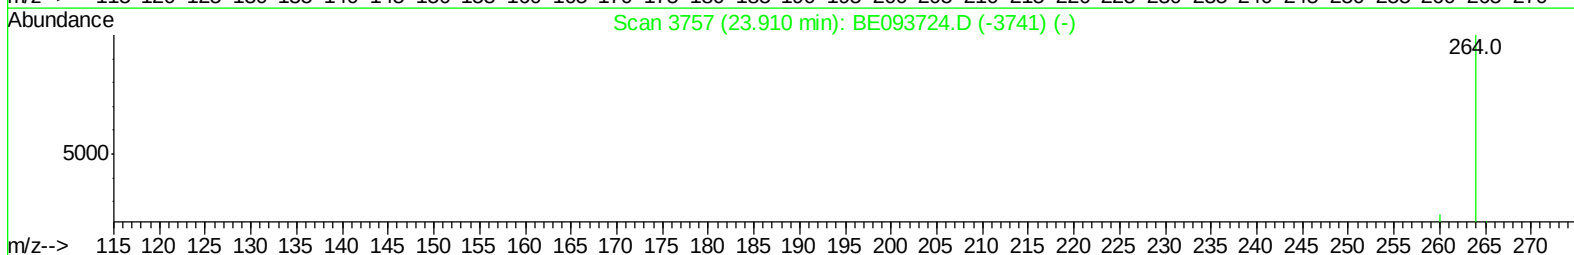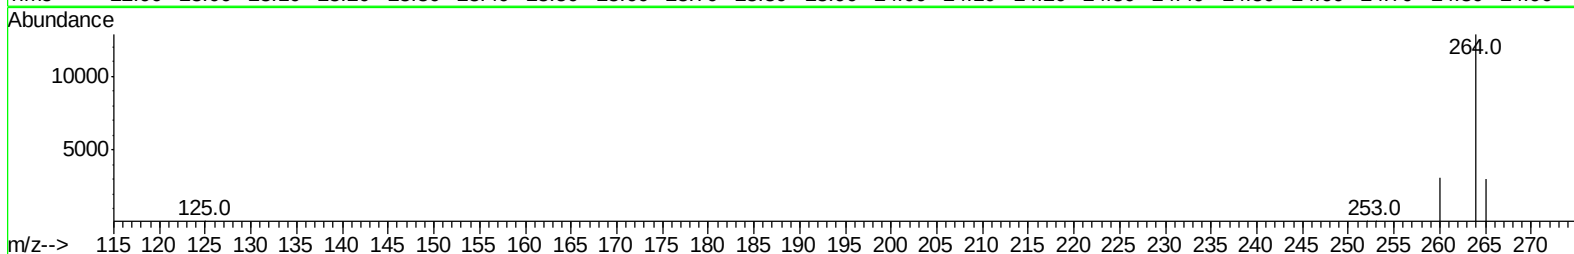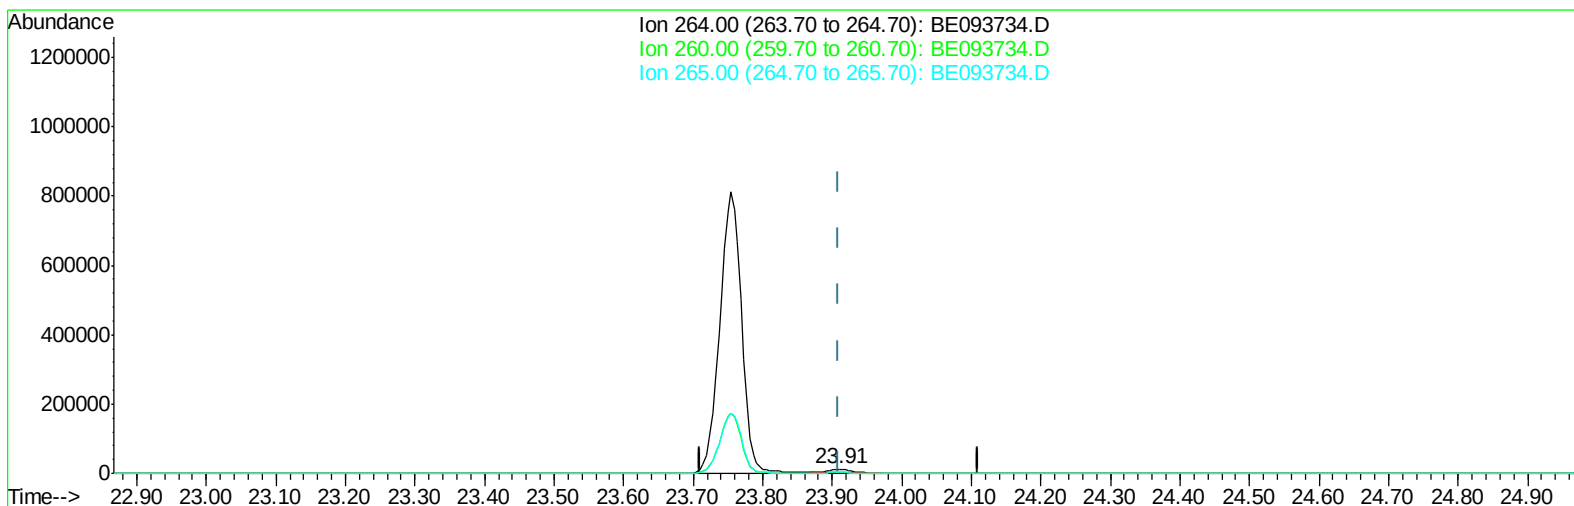

TIC: BE093734.D

(20) Perylene-d12 (I)

23.910min (-0.000) 0.40ng/ul m

response 22252

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	24.25
265.00	103.50	23.76#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE080817\
 Data File : BE093734.D
 Acq On : 9 Aug 2017 1:30
 Operator : SJ/JU
 Sample : I4557-06
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AC9

Manual Integrations
 APPROVED

Sohil
 8/9/2017 7:15:01 PM

Quant Time: Aug 09 06:48:45 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 09 05:31:57 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.92	152	3700	0.40	ng/ul	0.00
2) Naphthalene-d8	10.71	136	19472	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.52	164	12121	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.26	188	25566m	0.40	ng/ul	0.00
16) Chrysene-d12	21.41	240	25066	0.40	ng/ul	0.00
20) Perylene-d12	23.91	264	22252m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.29	152	8566	0.27	ng/ul	0.00
14) Fluoranthene-d10	19.27	212	22629	0.28	ng/ul	0.00
Target Compounds						
3) Naphthalene	10.75	128	8589	0.181	ng/ul#	93
5) 2-Methylnaphthalene	12.36	142	2394	0.069	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE080817\
Data File : BE093734.D
Acq On : 9 Aug 2017 1:30
Operator : SJ/JU
Sample : I4557-06
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AC9

Manual Integrations
APPROVED

Sohil
8/9/2017 7:15:01 PM

Quant Time: Aug 09 06:48:45 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 09 05:31:57 2017
Response via : Initial Calibration

