
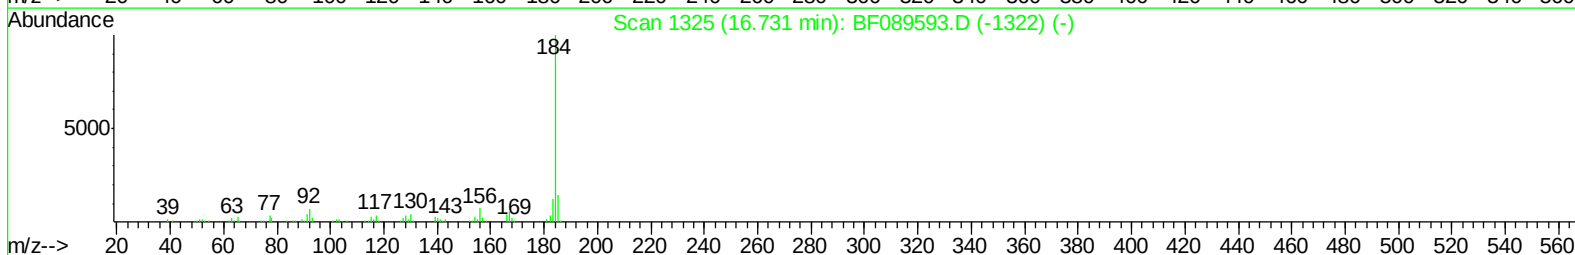
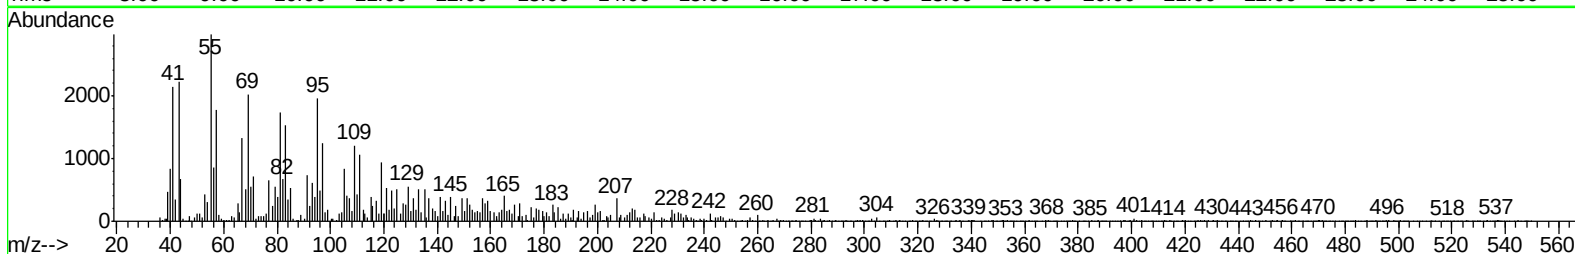


Data Path : Z:\HPCHEM1\BNA_E\Data\BE080916\
 Data File : BE092233.D
 Acq On : 9 Aug 2016 14:25
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 10 07:10:51 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF080416.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 05 01:39:23 2016
 Response via : Initial Calibration

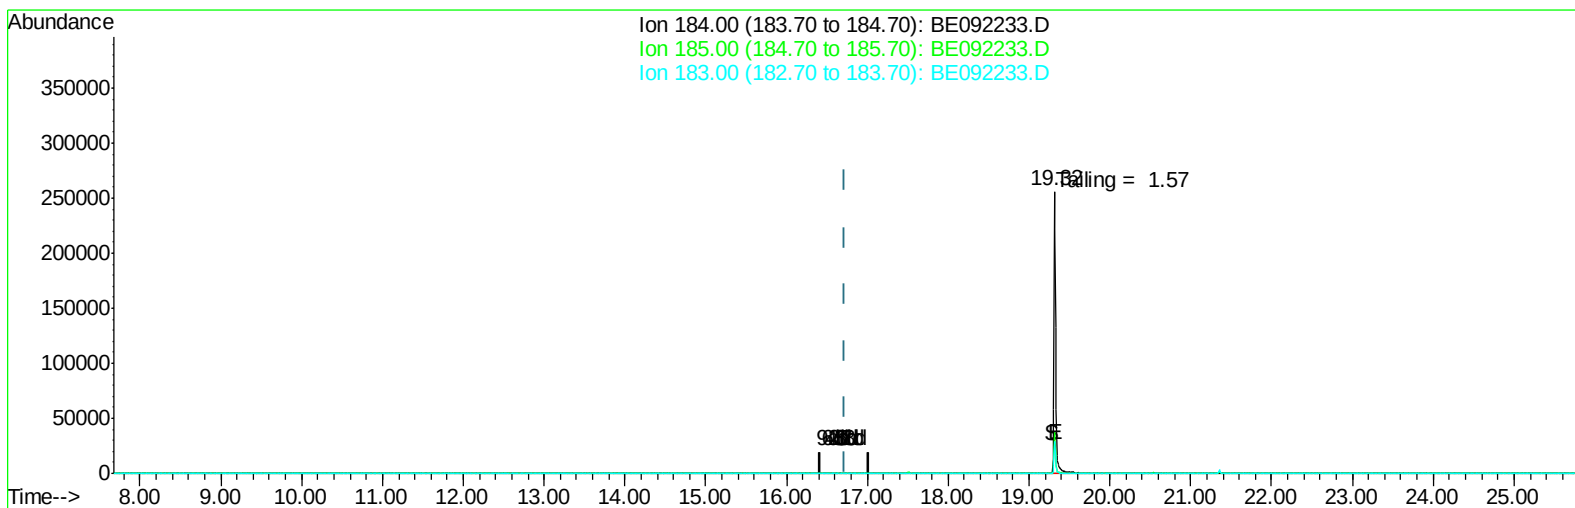

TIC: BE092233.D

(76) Benzidine




16.689min (-0.042) 27.41ng

response 59

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	164.54#
183.00	12.30	187.94#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\Data\BE080916\
Data File : BE092233.D
Acq On : 9 Aug 2016 14:25
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 10 07:10:51 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF080416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 05 01:39:23 2016
Response via : Initial Calibration

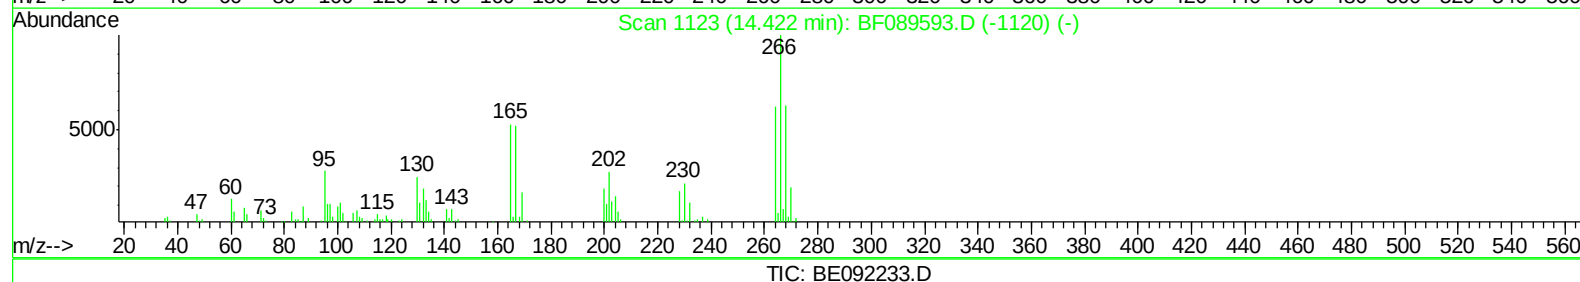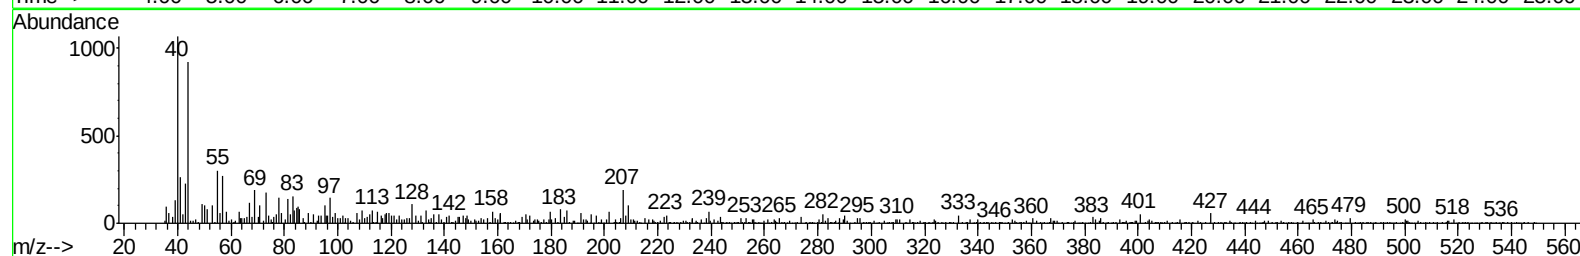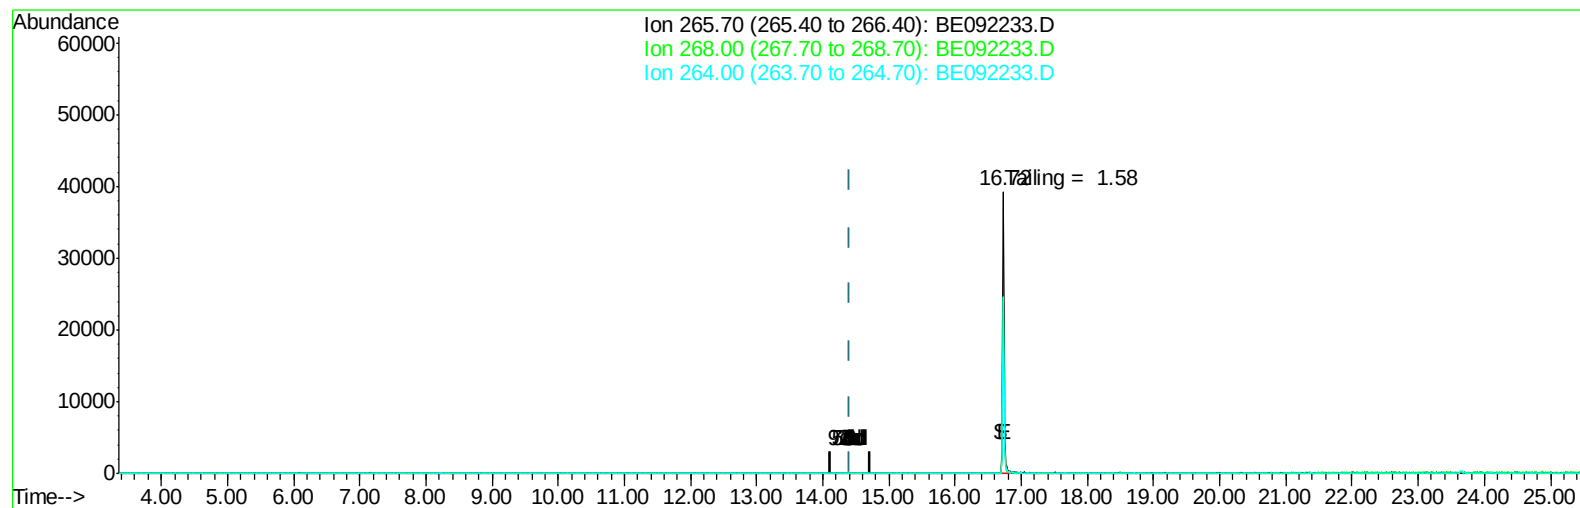

TIC: BE092233.D

(69) Pentachlorophenol (C)
14.398min (-0.024) 224.81ng
response 53

Ion	Exp%	Act%
265.70	100	100
268.00	63.20	9.09#
264.00	61.90	50.00
0.00	0.00	0.00