


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE080916\
 Data File : BE092233.D
 Acq On : 9 Aug 2016 14:25
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE080916.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 10 11:12:32 2016

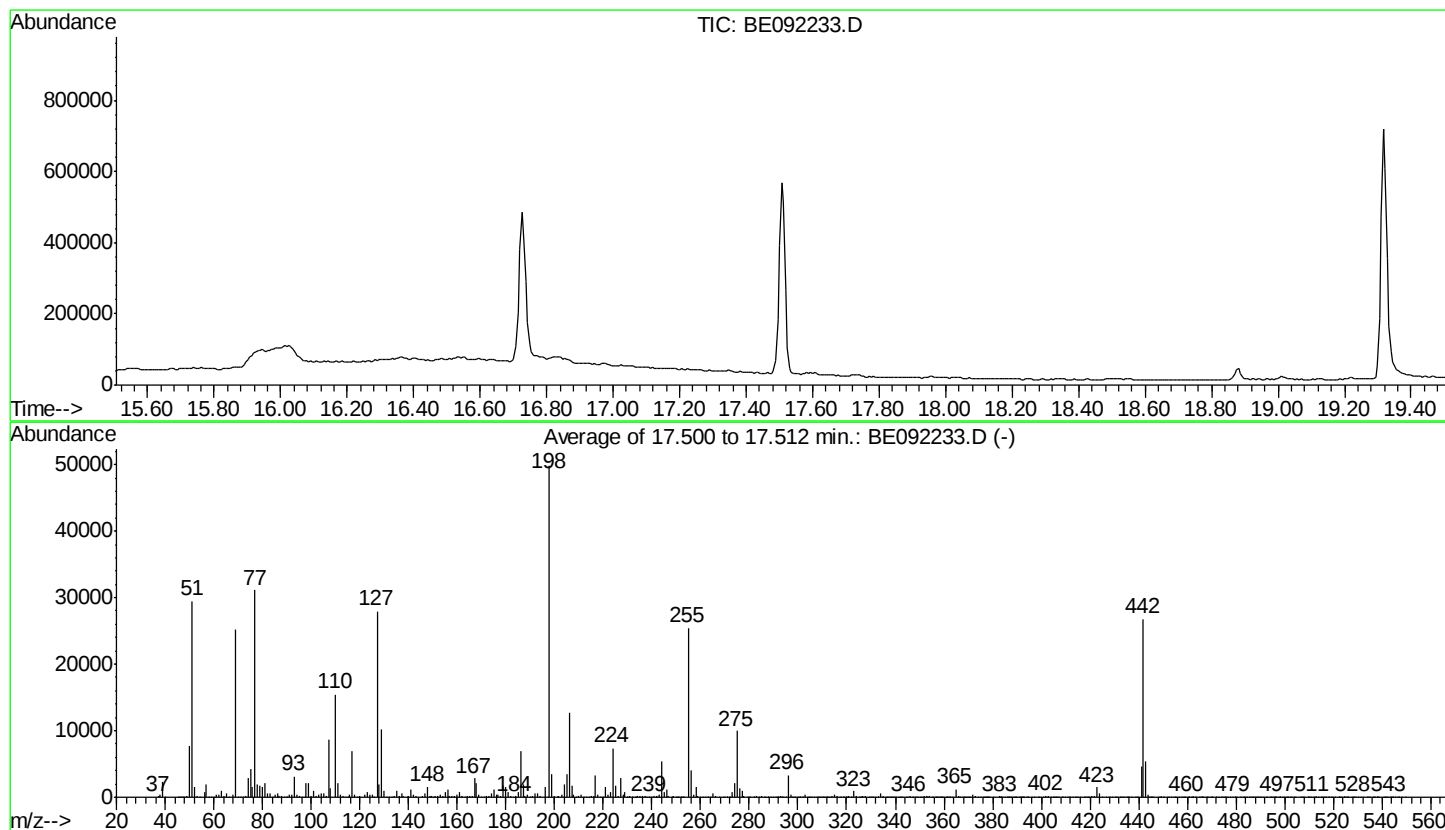

AutoFind: Scans 2538, 2539, 2540; Background Corrected with Scan 2531

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	59.1	29469	PASS
68	69	0.00	2	1.5	369	PASS
69	198	0.00	100	50.4	25131	PASS
70	69	0.00	2	0.4	102	PASS
127	198	10	80	56.0	27911	PASS
197	198	0.00	2	0.1	68	PASS
198	198	100	100	100.0	49834	PASS
199	198	5	9	7.1	3549	PASS
275	198	10	60	20.0	9952	PASS
365	198	1	100	2.4	1210	PASS
441	442	0.01	24	17.3	4627	PASS
442	198	50	100	53.8	26798	PASS
443	442	15	24	19.8	5317	PASS