

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080918\
 Data File : BE097244.D
 Acq On : 9 Aug 2018 10:49
 Operator : SJ/JU
 Sample : PB111788BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Aug 09 16:04:32 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 08 23:25:58 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	1198	0.40	ng/ul	0.00
2) Naphthalene-d8	10.13	136	6363	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.02	164	3939	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.87	188	741437	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-20.97
20) Perylene-d12	23.21	264	13648	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.72	152	3444	0.34	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds				Ovalue		
9) Fluorene	15.03	166	1120	0.079	ng/ul#	21
23) Benzo(a)pyrene	23.08	252	2835	0.076	ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080918\
Data File : BE097244.D
Acq On : 9 Aug 2018 10:49
Operator : SJ/JU
Sample : PB111788BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Aug 09 16:04:32 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 08 23:25:58 2018
Response via : Initial Calibration

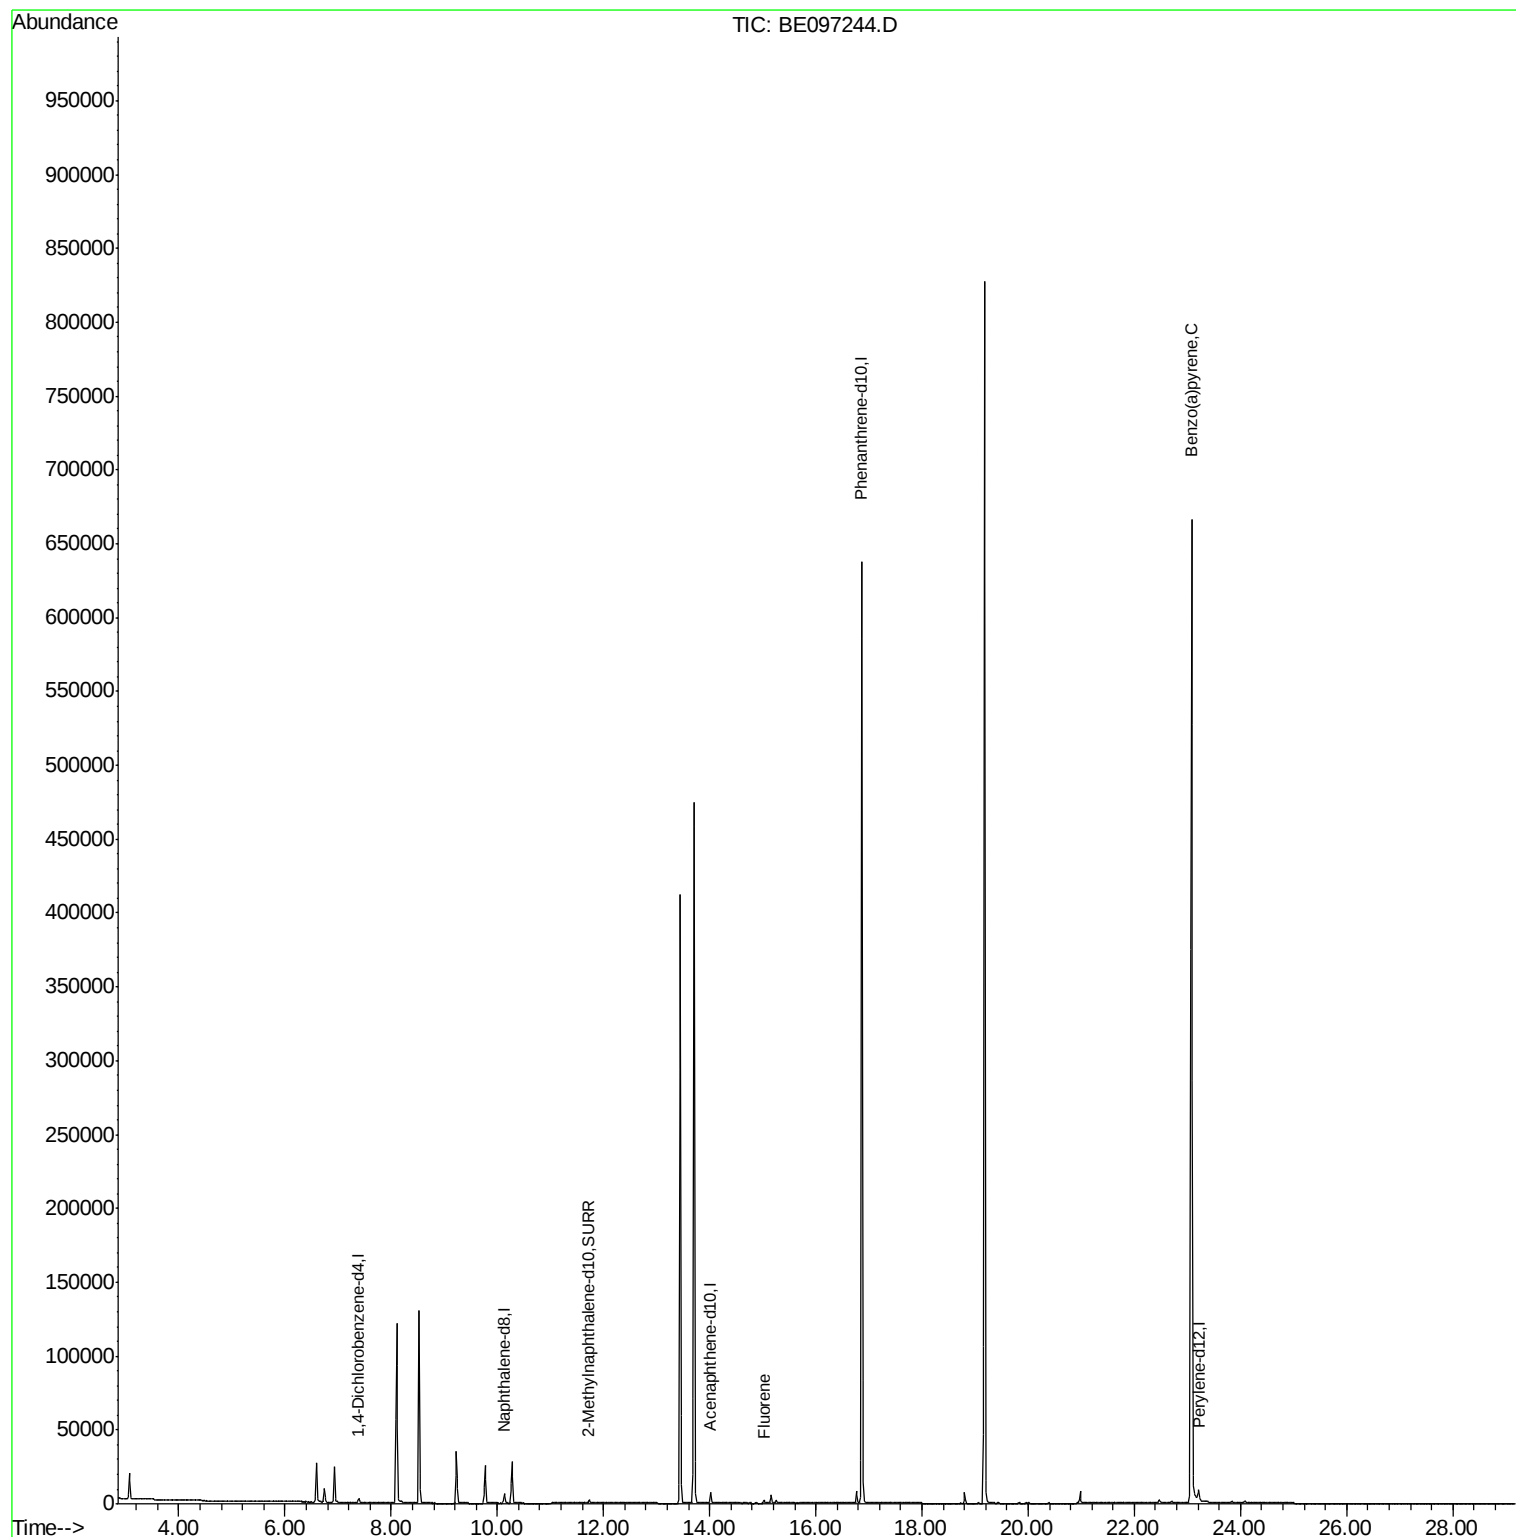

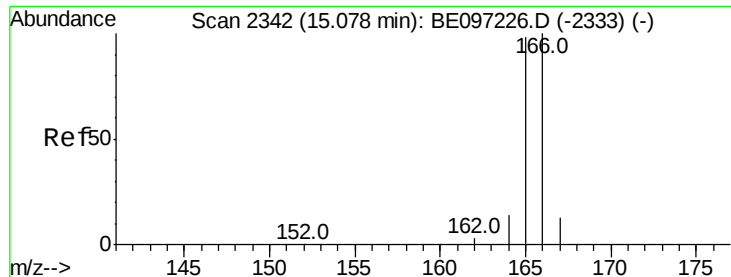

#9

Fluorene

Concen: 0.079 ng/ul

RT: 15.03 min Scan# 2334

Delta R.T. -0.05 min

Lab File: BE097244.D

Acq: 9 Aug 2018 10:49

Instrument :

BNA_E

ClientSampleId :





Tot Ion:166 Resp: 1120

Ion Ratio Lower Upper

166 100

165 10.1 73.4 110.2#

167 39.1 14.6 22.0#

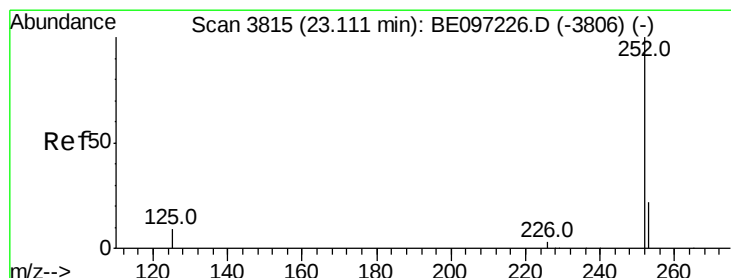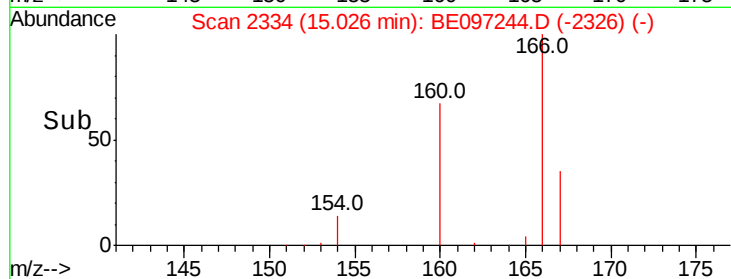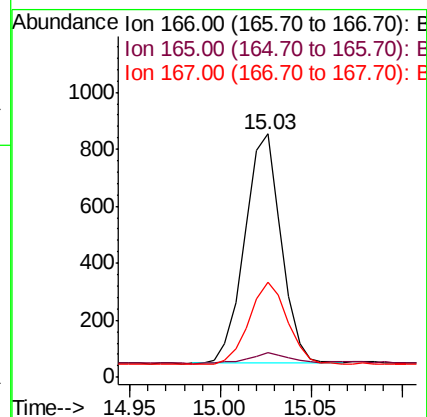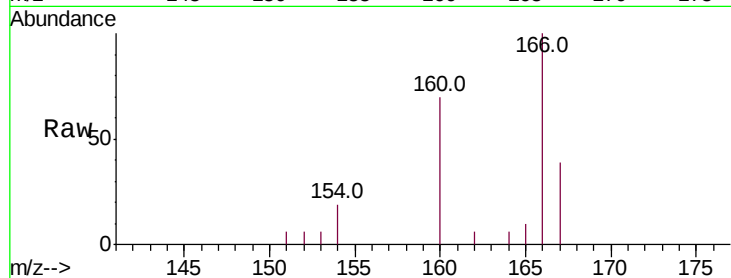

#23

Benzo(a)pyrene

Concen: 0.076 ng/ul

RT: 23.08 min Scan# 3809

Delta R.T. -0.03 min

Lab File: BE097244.D

Acq: 9 Aug 2018 10:49

Tgt Ion:252 Resp: 2835

Ion Ratio Lower Upper

252 100

253 34.3 28.5 42.7

125 19.9 18.1 27.1

