


Data Path : Z:\HPCHEM1\BNA E\DATA\BE081015\
 Data File : BE090405.D
 Acq On : 10 Aug 2015 11:34
 Operator : TP/UM
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE080515.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 06 12:28:08 2015

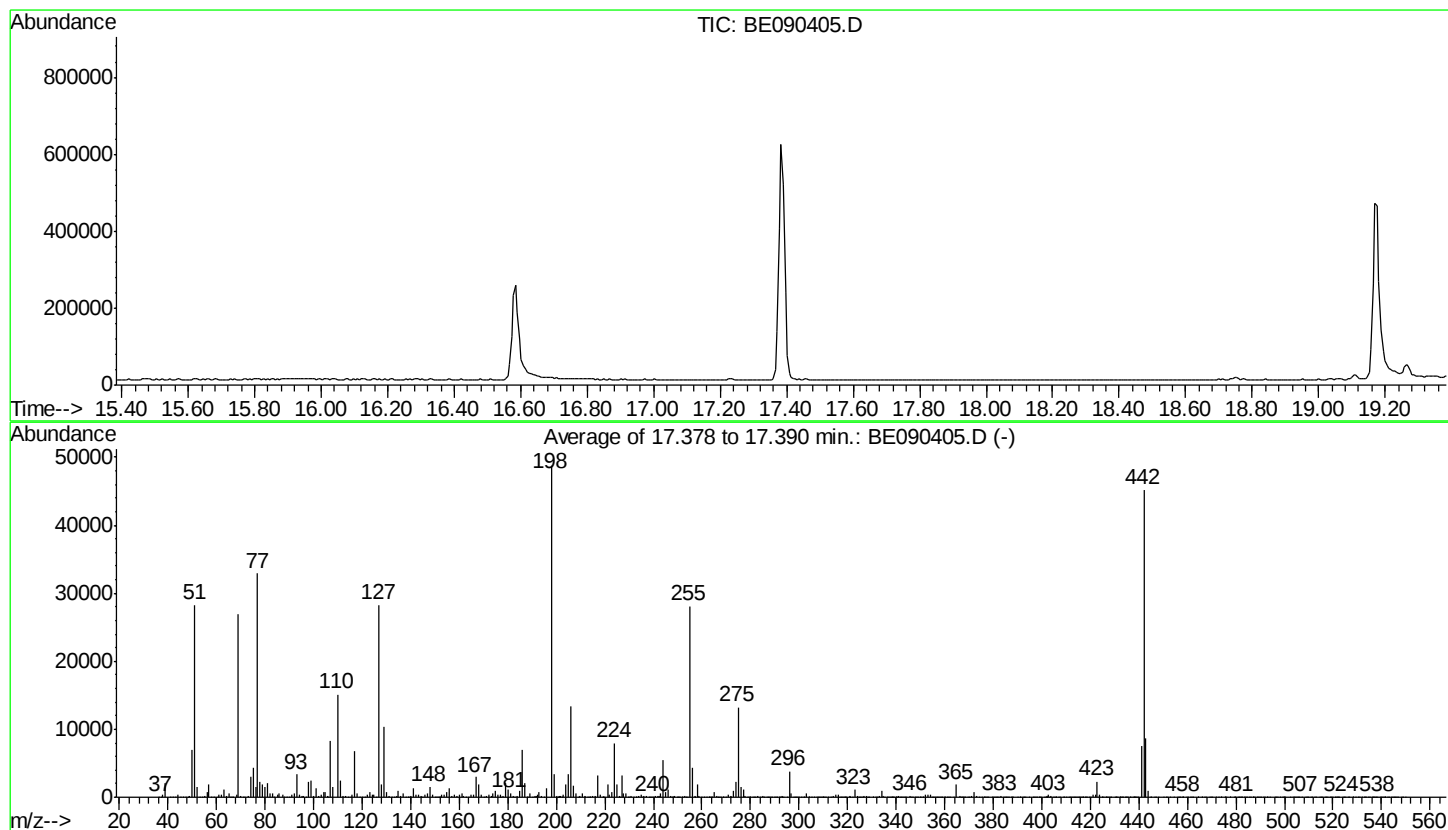

AutoFind: Scans 2517, 2518, 2519; Background Corrected with Scan 2508

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	58.1	28338	PASS
68	69	0.00	2	1.1	300	PASS
69	198	0.00	100	55.4	27015	PASS
70	69	0.00	2	0.6	149	PASS
127	198	10	80	58.1	28325	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	48770	PASS
199	198	5	9	7.0	3409	PASS
275	198	10	60	27.1	13221	PASS
365	198	1	100	3.7	1812	PASS
441	442	0.01	24	16.8	7624	PASS
442	198	50	100	92.8	45265	PASS
443	442	15	24	19.3	8728	PASS