


Data Path : Z:\HPCHEM1\BNA E\DATA\BE081015\
Data File : BE090415.D
Acq On : 10 Aug 2015 23:48
Operator : TP/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE080515.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Aug 06 12:28:08 2015

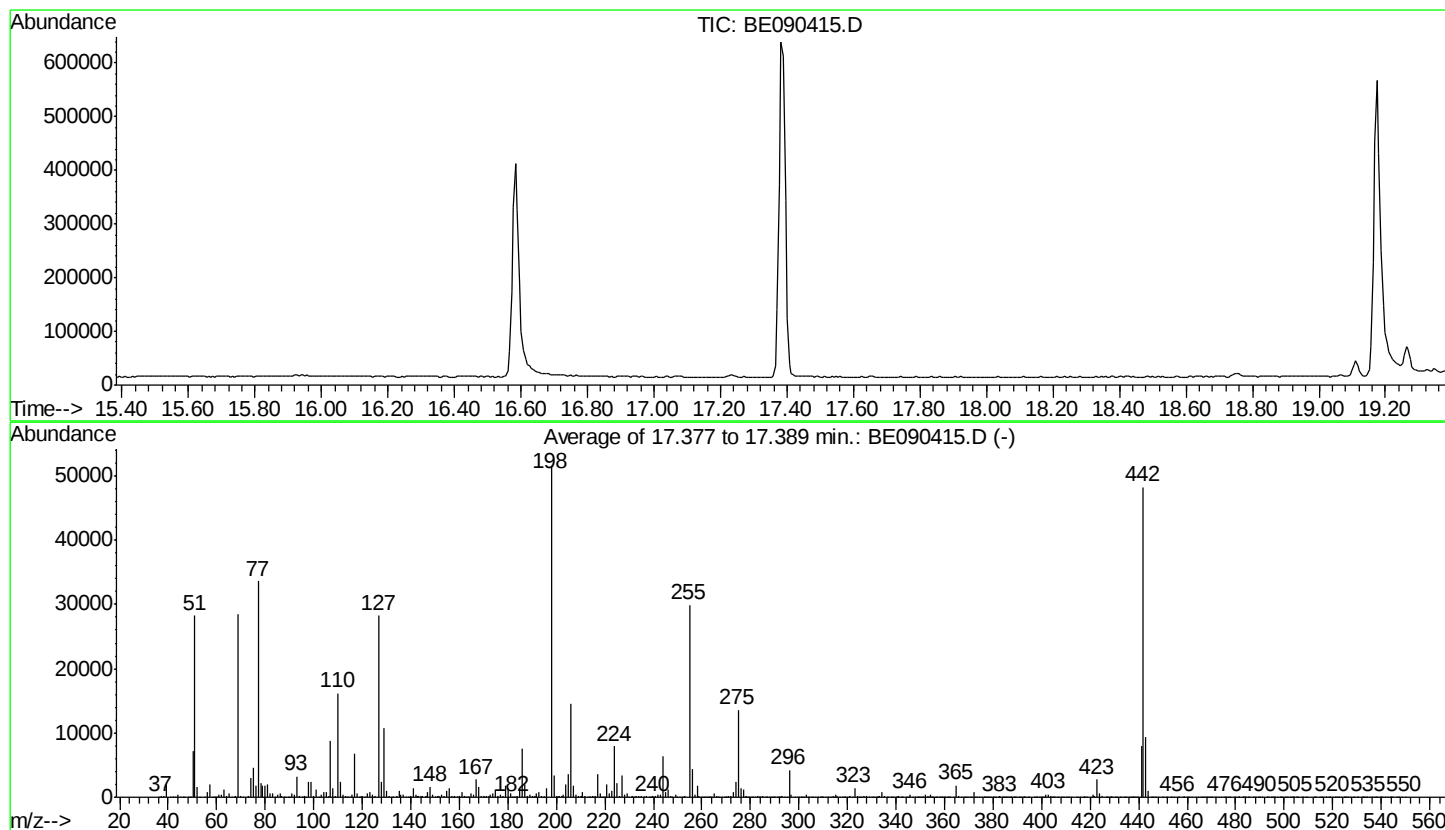

AutoFind: Scans 2517, 2518, 2519; Background Corrected with Scan 2508

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.7	28206	PASS
68	69	0.00	2	0.8	216	PASS
69	198	0.00	100	55.3	28551	PASS
70	69	0.00	2	0.6	171	PASS
127	198	10	80	54.7	28192	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	51583	PASS
199	198	5	9	6.8	3489	PASS
275	198	10	60	26.3	13562	PASS
365	198	1	100	3.5	1794	PASS
441	442	0.01	24	16.6	8019	PASS
442	198	50	100	93.6	48284	PASS
443	442	15	24	19.3	9331	PASS