
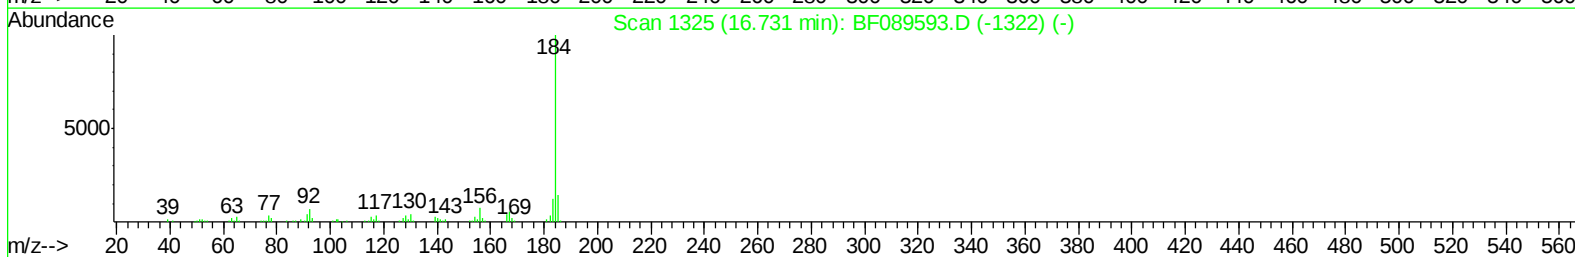
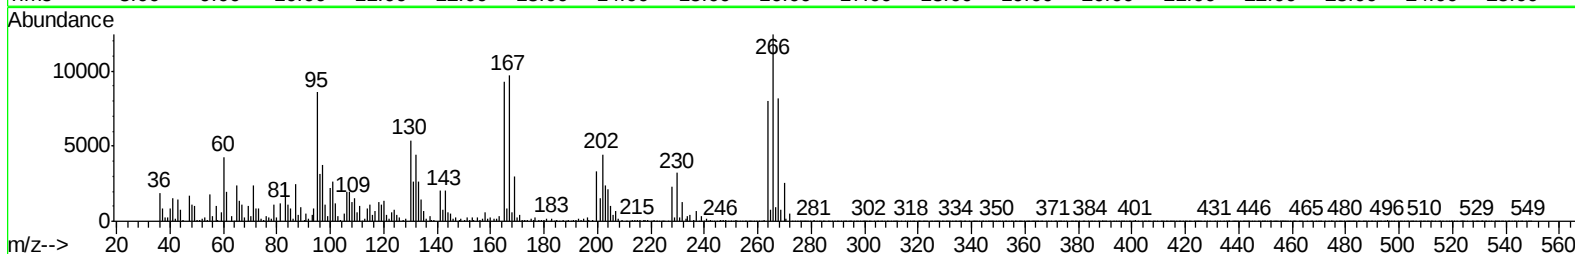


Data Path : Z:\HPCHEM1\BNA_E\Data\BE081016\
Data File : BE092244.D
Acq On : 10 Aug 2016 8:28
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 11 07:43:15 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF080416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 05 01:39:23 2016
Response via : Initial Calibration

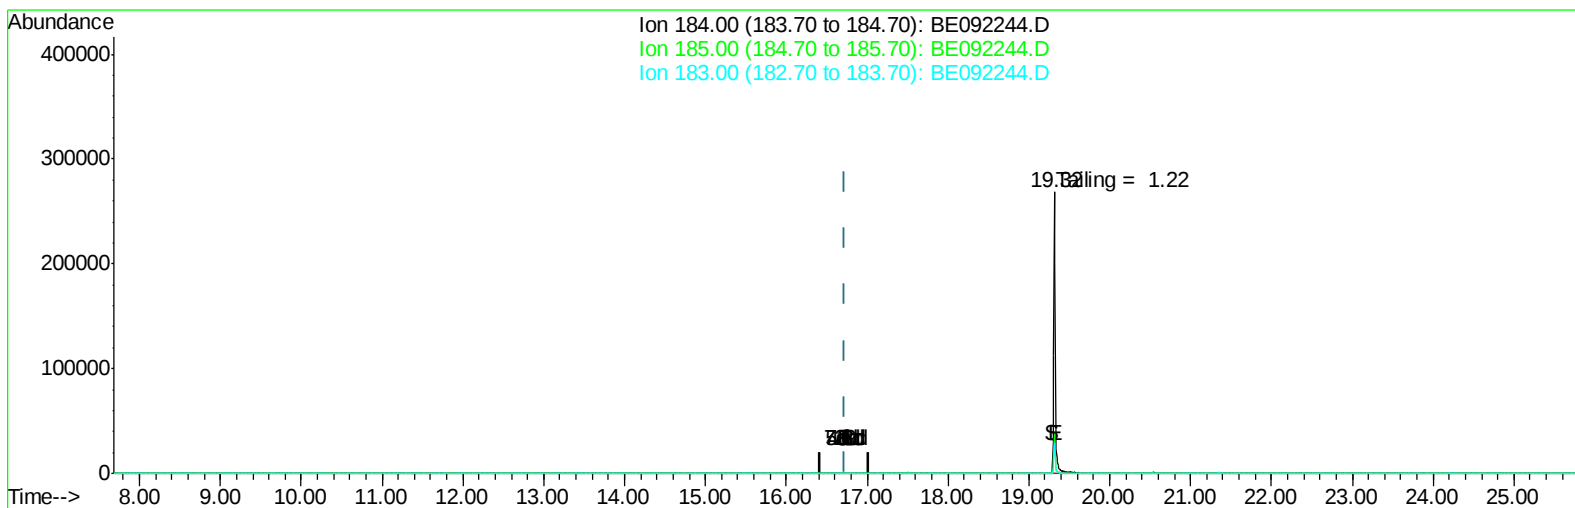

TIC: BE092244.D

(76) Benzidine




16.713min (-0.018) 117.82ng

response 75

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	66.22#
183.00	12.30	243.24#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\Data\BE081016\
Data File : BE092244.D
Acq On : 10 Aug 2016 8:28
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 11 07:43:15 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF080416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 05 01:39:23 2016
Response via : Initial Calibration

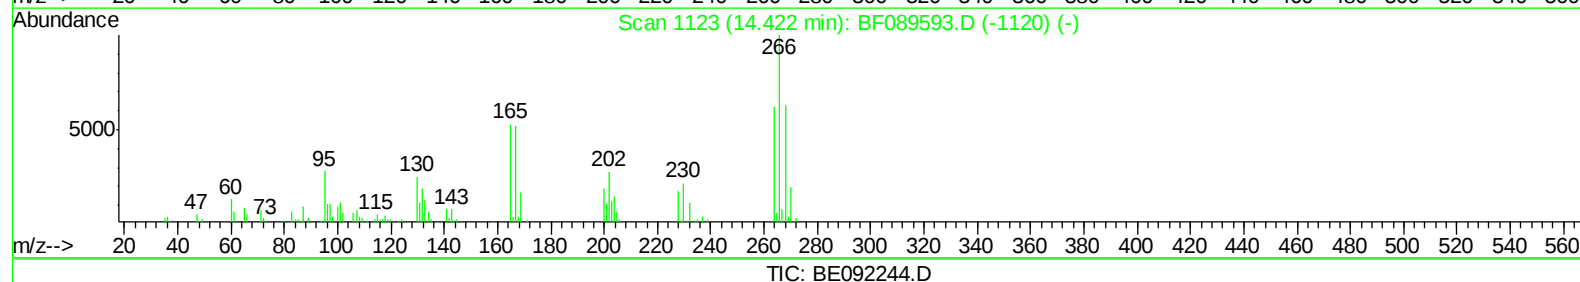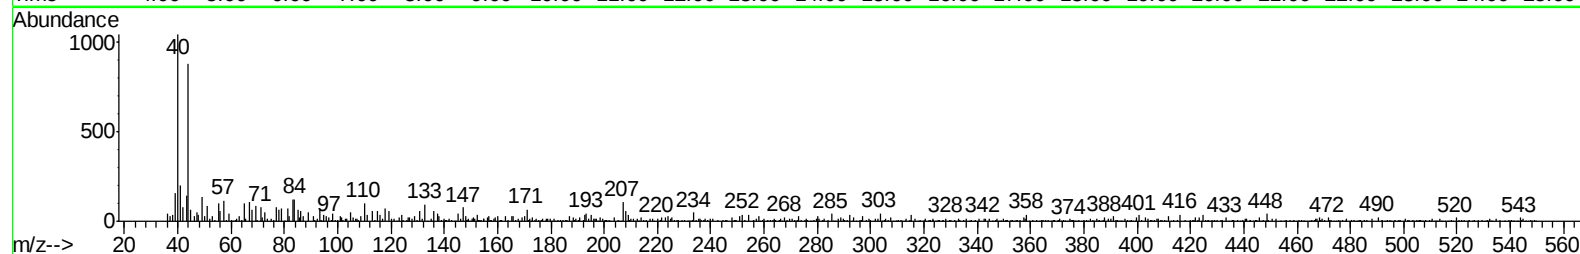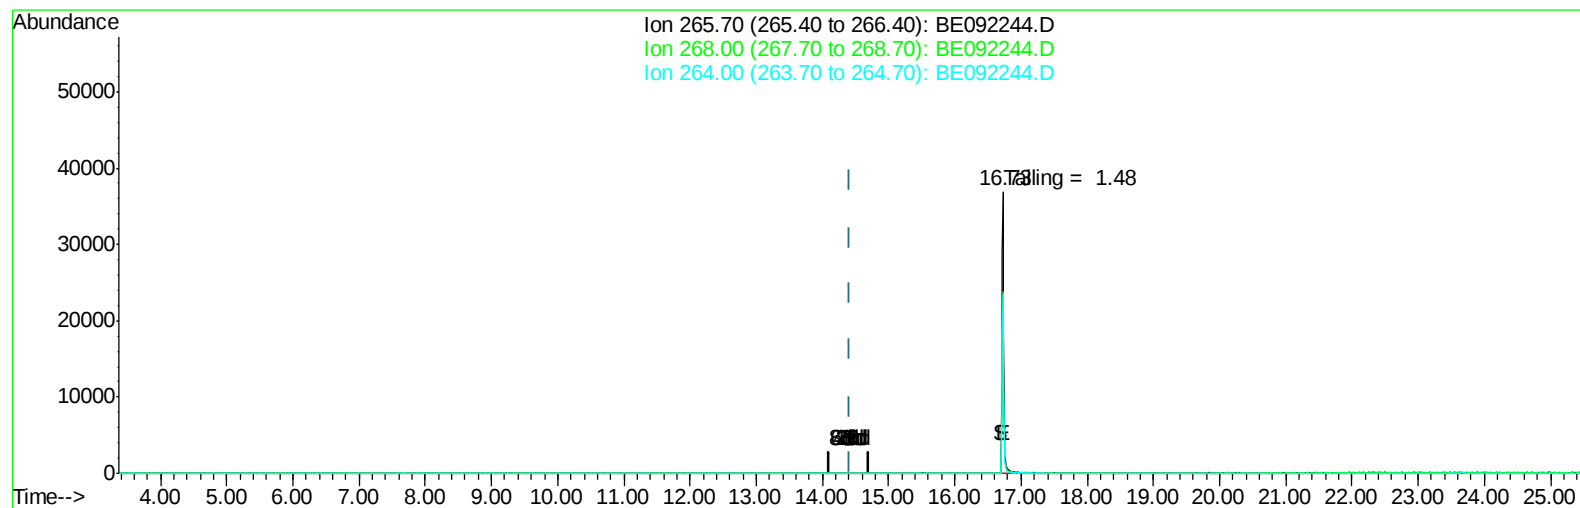

(69) Pentachlorophenol (C)

14.410min (-0.012) 63.17ng

response 19

Ion	Exp%	Act%
265.70	100	100
268.00	63.20	150.00#
264.00	61.90	133.33#
0.00	0.00	0.00