


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE081016\
Data File : BE092244.D
Acq On : 10 Aug 2016 8:28
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE080916.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Aug 10 11:12:32 2016

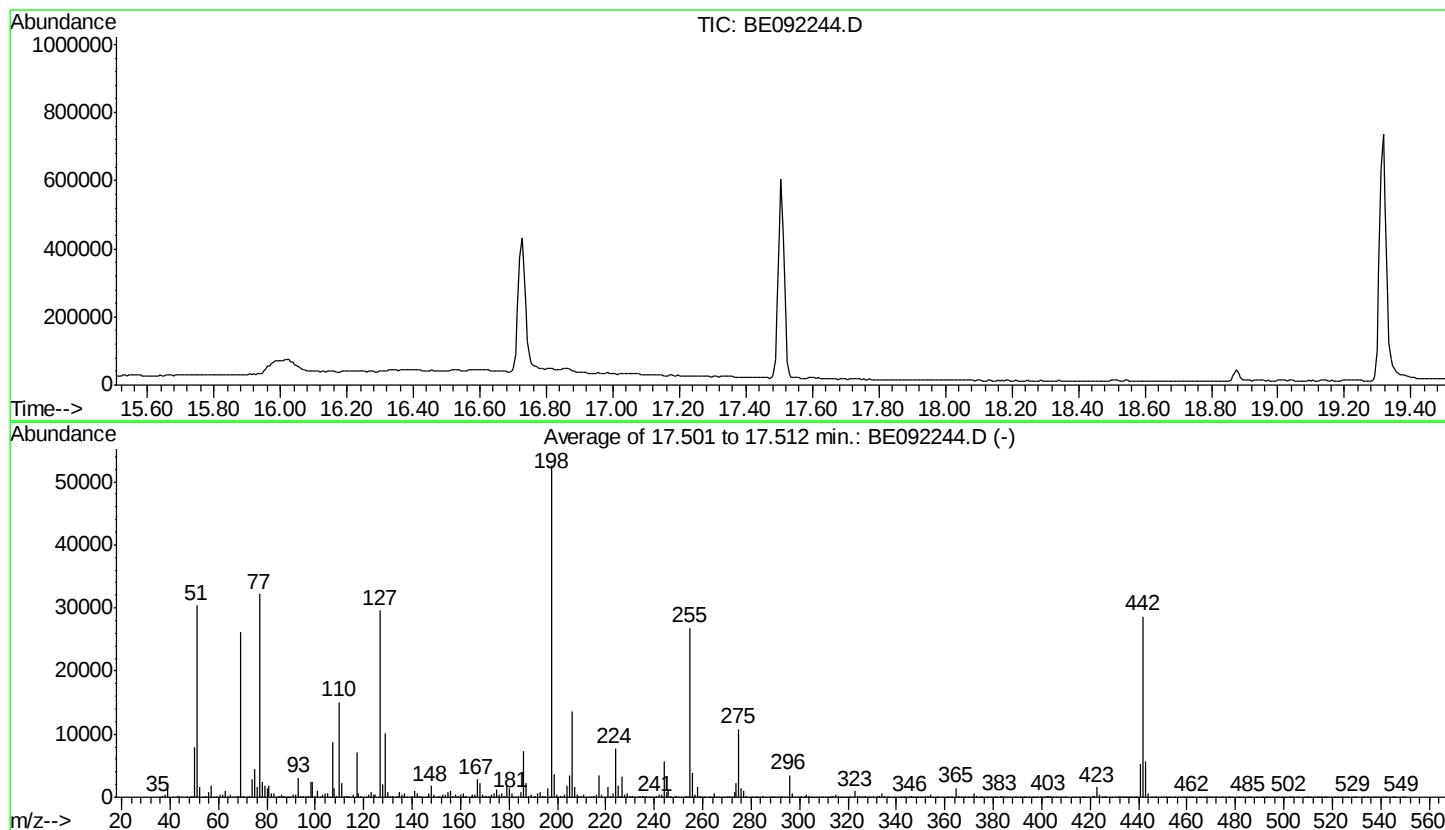

AutoFind: Scans 2538, 2539, 2540; Background Corrected with Scan 2531

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.9	30424	PASS
68	69	0.00	2	1.1	278	PASS
69	198	0.00	100	49.8	26162	PASS
70	69	0.00	2	0.7	180	PASS
127	198	10	80	56.2	29563	PASS
197	198	0.00	2	0.2	94	PASS
198	198	100	100	100.0	52558	PASS
199	198	5	9	6.9	3626	PASS
275	198	10	60	20.5	10762	PASS
365	198	1	100	2.8	1451	PASS
441	442	0.01	24	18.7	5345	PASS
442	198	50	100	54.5	28620	PASS
443	442	15	24	20.2	5771	PASS