


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE081017\
Data File : BE093741.D
Acq On : 10 Aug 2017 10:21
Operator : SJ/JU
Sample : PB101278BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
SBLK78

Manual Integrations
APPROVED

sohil
8/14/2017 7:01:41 PM

Quant Time: Aug 11 17:42:03 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE072417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 11 06:07:04 2017
Response via : Initial Calibration

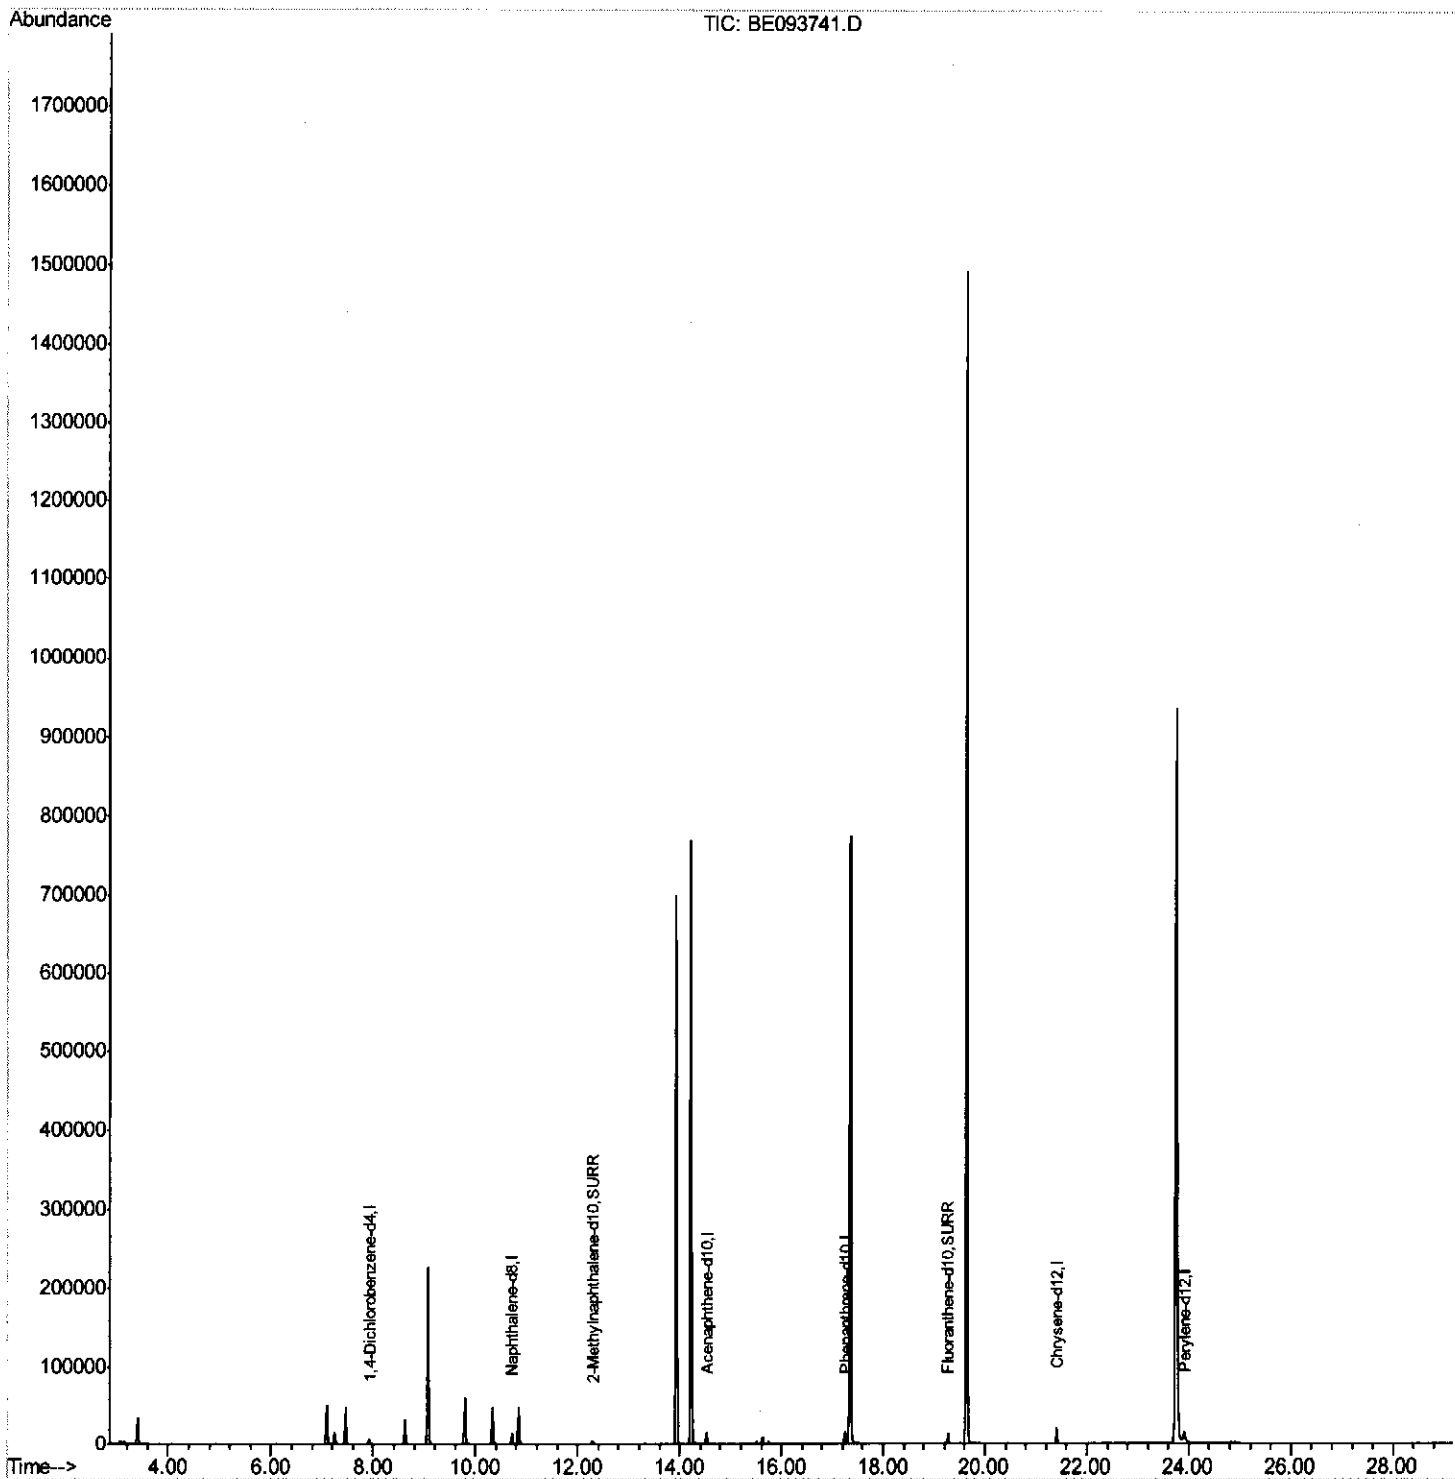

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\DATA\BE081017\
 Data File : BE093741.D
 Acq On : 10 Aug 2017 10:21
 Operator : SJ/JU
 Sample : PB101278BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 SBLK78

Manual Integrations
 APPROVED

sohil
 8/14/2017 7:01:41 PM

Quant Time: Aug 11 17:29:19 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 11 06:07:04 2017
 Response via : Initial Calibration

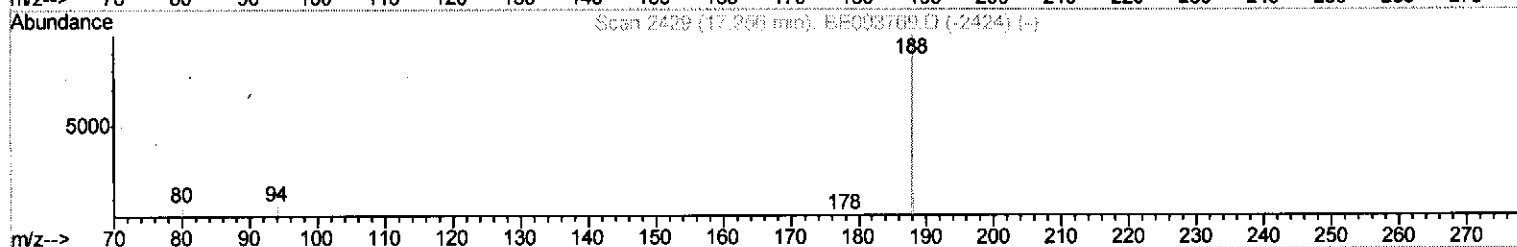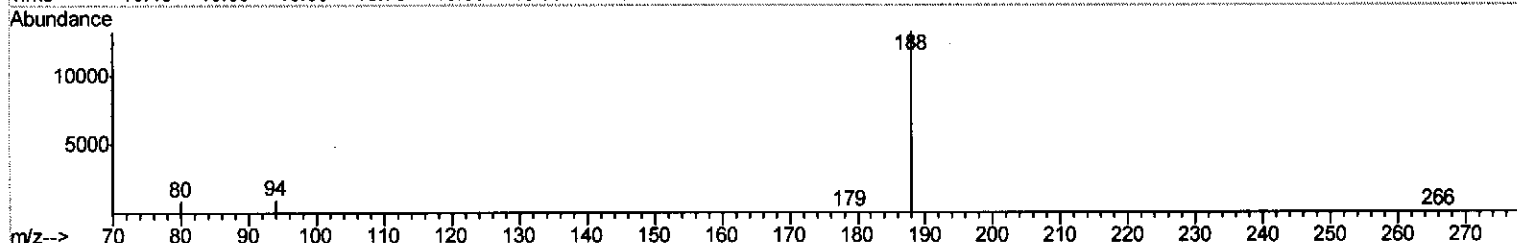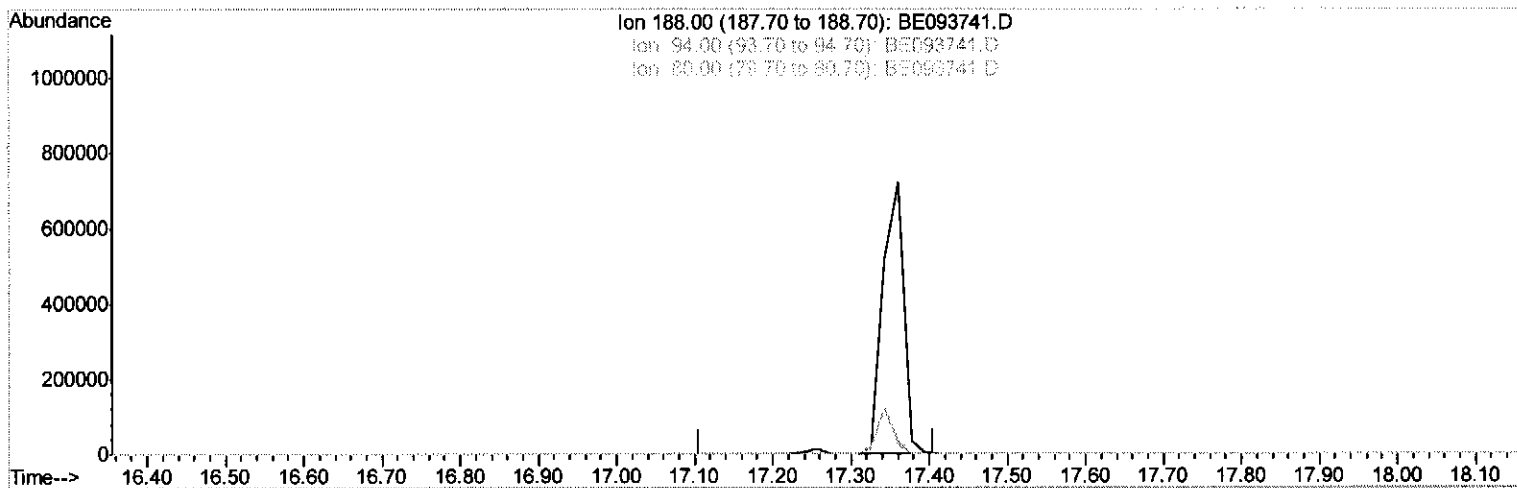

TIC: BE093741.D

(10) Phenanthrene-d10 (I)
 17.256min (-17.256) 0.00ng/ul
 response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.00	0.00#
80.00	11.80	0.00#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_E\DATA\BE081017\
Data File : BE093741.D
Acq On : 10 Aug 2017 10:21
Operator : SJ/JU
Sample : PB101278BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
SBLK78

Manual Integrations
APPROVED

sohil
8/14/2017 7:01:41 PM

Quant Time: Aug 11 17:29:19 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE072417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 11 06:07:04 2017
Response via : Initial Calibration

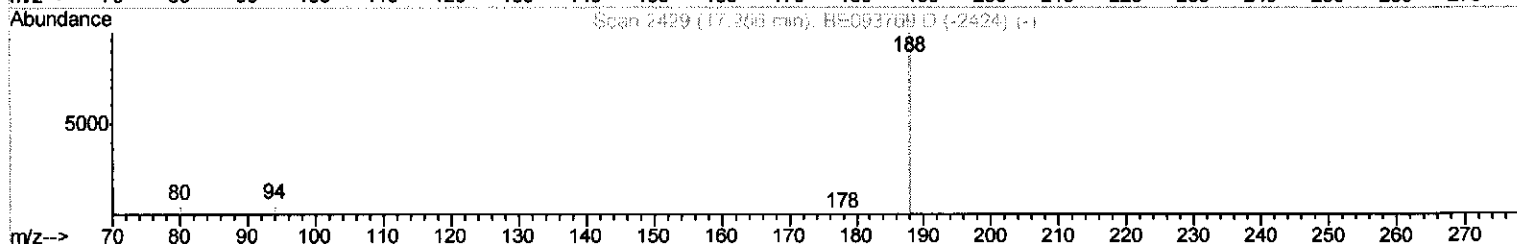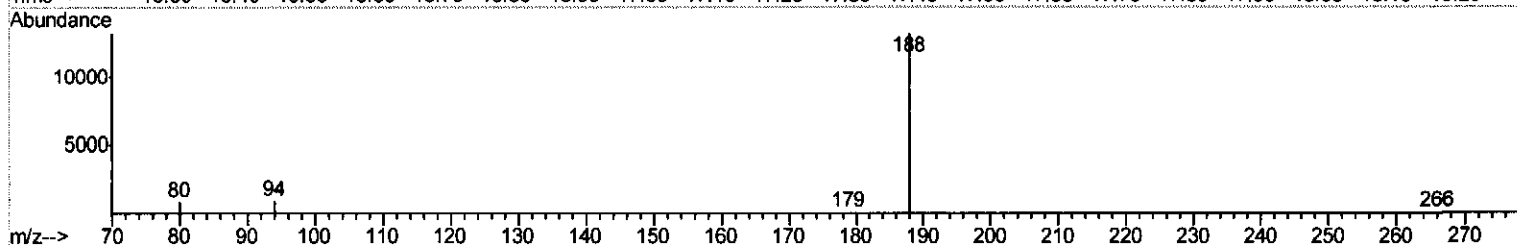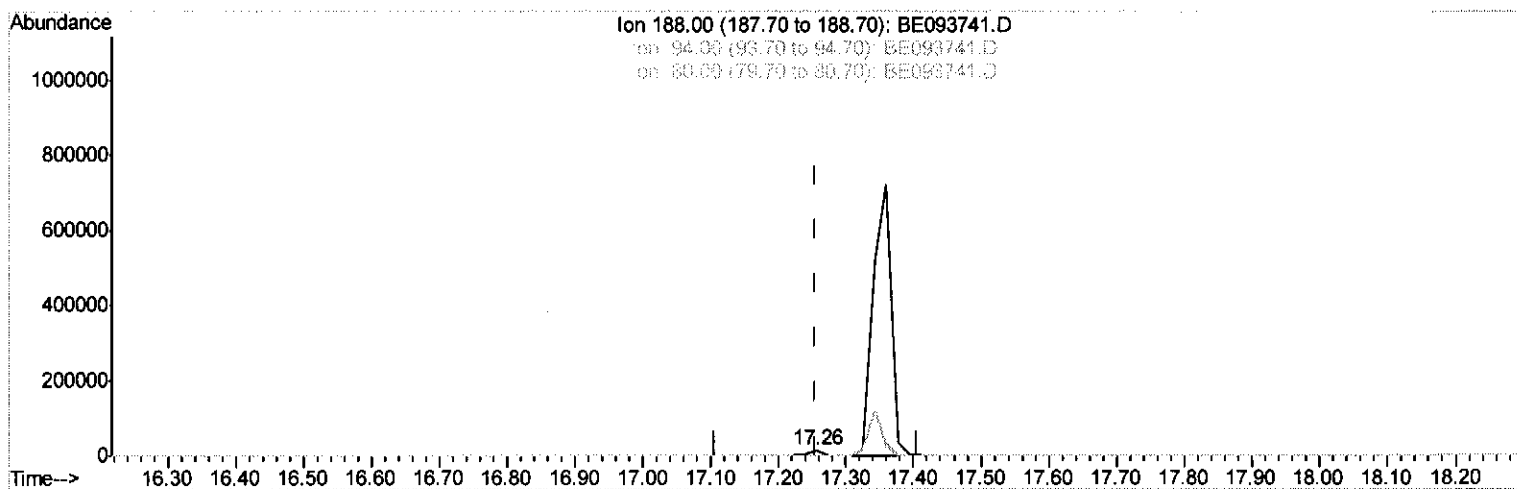

TIC: BE093741.D

(10) Phenanthrene-d10 (I)

17.256min (+0.000) 0.40ng/ul m

response 19632

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	7.02#
80.00	11.80	6.40#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\DATA\BE081017\
Data File : BE093741.D
Acq On : 10 Aug 2017 10:21
Operator : SJ/JU
Sample : PB101278BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
SBLK78

Manual Integrations
APPROVED

sohil
8/14/2017 7:01:41 PM

Quant Time: Aug 11 17:40:55 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE072417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 11 06:07:04 2017
Response via : Initial Calibration

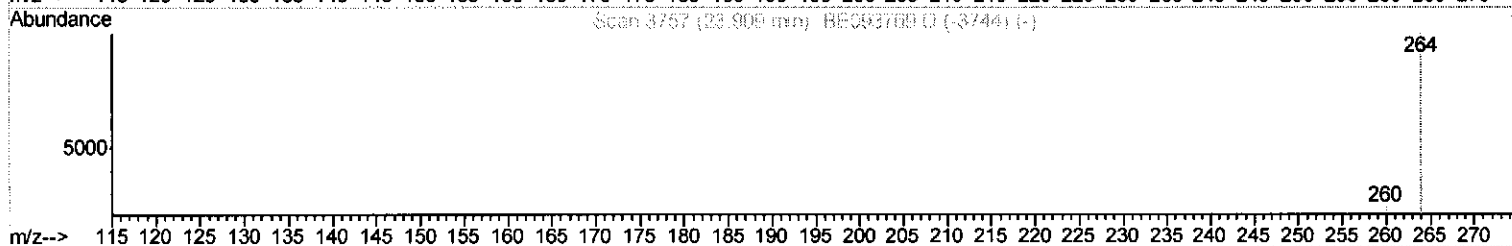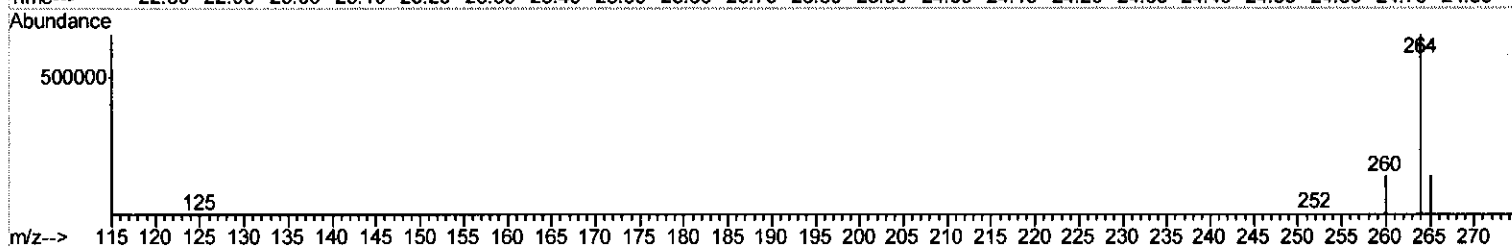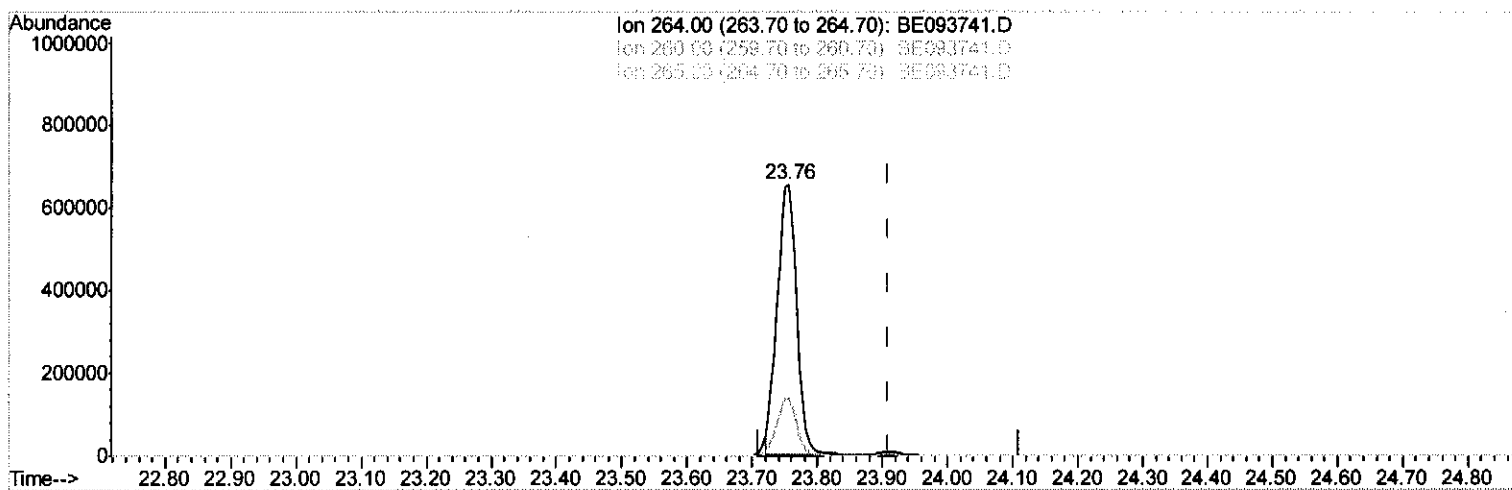

TIC: BE093741.D

(20) Perylene-d12 (I)

23.756min (-0.154) 0.40ng/ul

response 1376235

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.15#
265.00	103.50	21.57#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\DATA\BE081017\
 Data File : BE093741.D
 Acq On : 10 Aug 2017 10:21
 Operator : SJ/JU
 Sample : PB101278BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 SBLK78

Manual Integrations
 APPROVED

sohil
 8/14/2017 7:01:41 PM

Quant Time: Aug 11 17:40:55 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 11 06:07:04 2017
 Response via : Initial Calibration

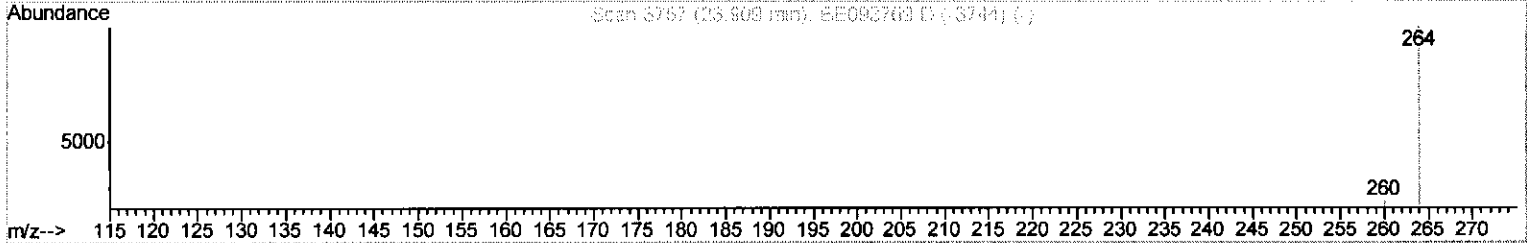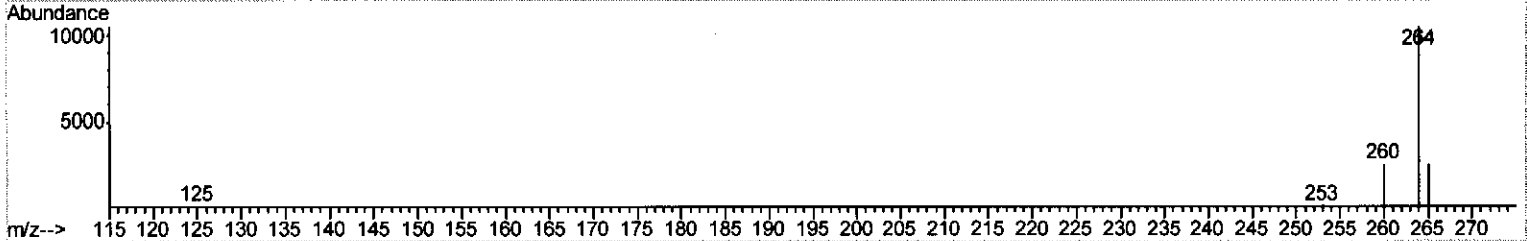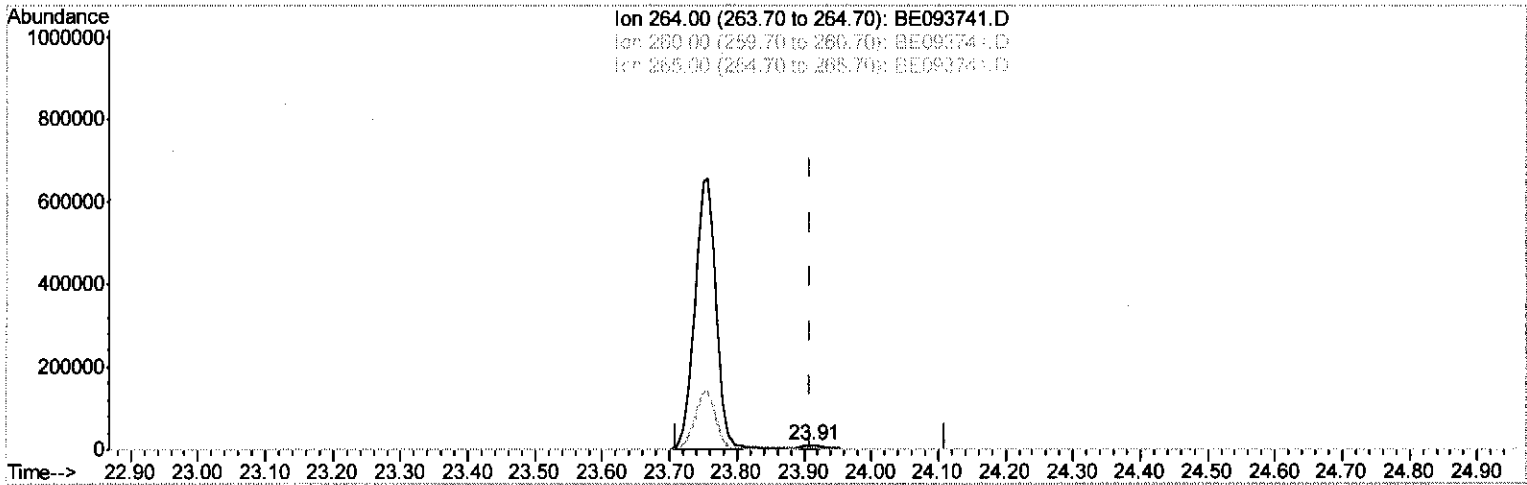

TIC: BE093741.D

(20) Perylene-d12 (I)

23.910min (+0.001) 0.40ng/ul m

SJL 8/14/17

response 17398

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	24.47
265.00	103.50	24.67#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE081017\
Data File : BE093741.D
Acq On : 10 Aug 2017 10:21
Operator : SJ/JU
Sample : PB101278BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK78

Manual Integrations
APPROVED

sohil
8/14/2017 7:01:41 PM

Quant Time: Aug 11 17:42:03 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE072417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 11 06:07:04 2017
Response via : Initial Calibration

Internal Standards	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.92	152		2880	0.40	ng/ul	0.00
2) Naphthalene-d8	10.71	136		14381	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.53	164		8718	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.26	188		19632m	0.40	ng/ul	0.00
16) Chrysene-d12	21.41	240		20287	0.40	ng/ul	0.00
20) Perylene-d12	23.91	264		17398m	0.40	ng/ul	0.00

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.29	152		6065	0.26	ng/ul	0.00
14) Fluoranthene-d10	19.27	212		16004	0.26	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed