


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE081017\
Data File : BE093751.D
Acq On : 10 Aug 2017 17:45
Operator : SJ/JU
Sample : I4455-04
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
C0AG3

Manual Integrations
APPROVED

sohil
8/14/2017 7:02:54 PM

Quant Time: Aug 11 18:12:59 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE072417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 11 06:07:04 2017
Response via : Initial Calibration

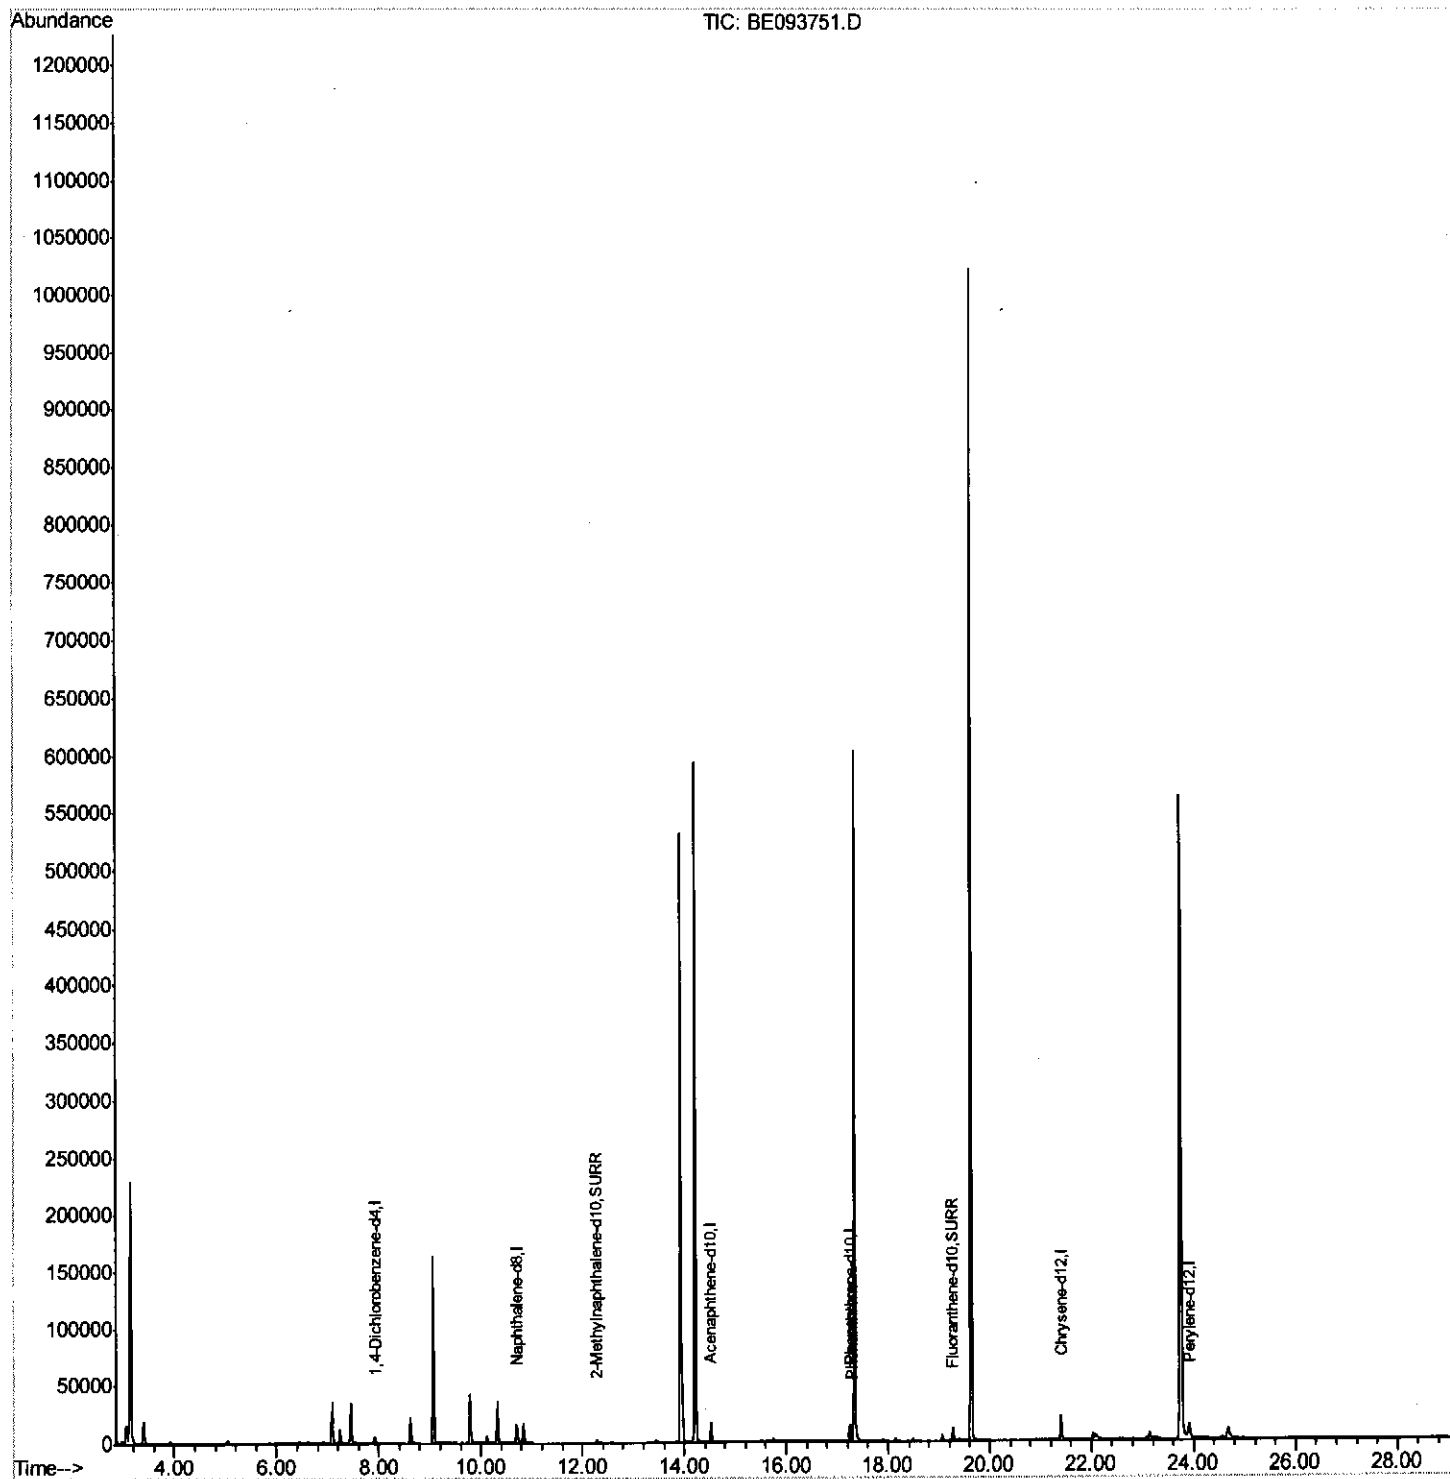

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\DATA\BE081017\
 Data File : BE093751.D
 Acq On : 10 Aug 2017 17:45
 Operator : SJ/JU
 Sample : I4455-04
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AG3

Manual Integrations
 APPROVED

sohil
 8/14/2017 7:02:54 PM

Quant Time: Aug 11 17:30:09 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 11 06:07:04 2017
 Response via : Initial Calibration

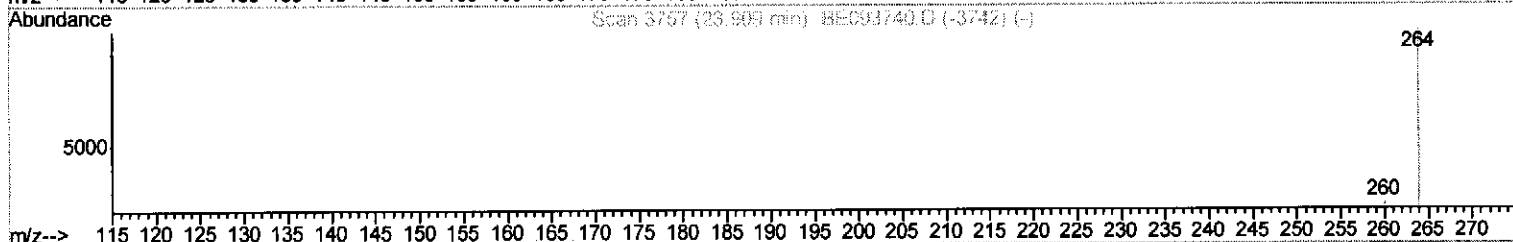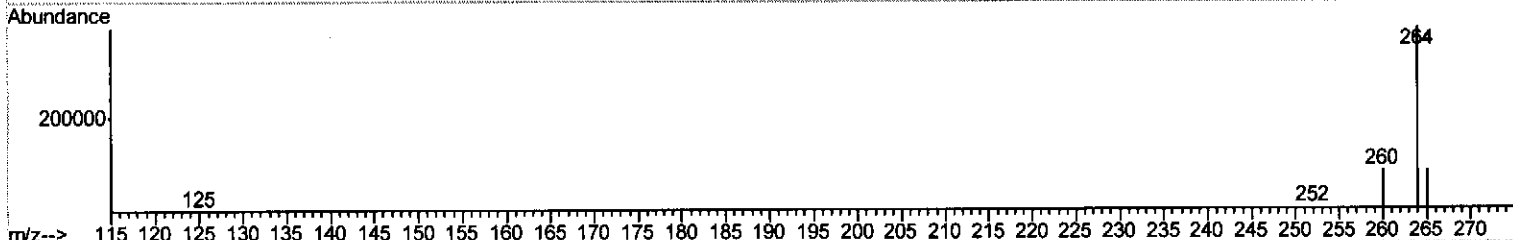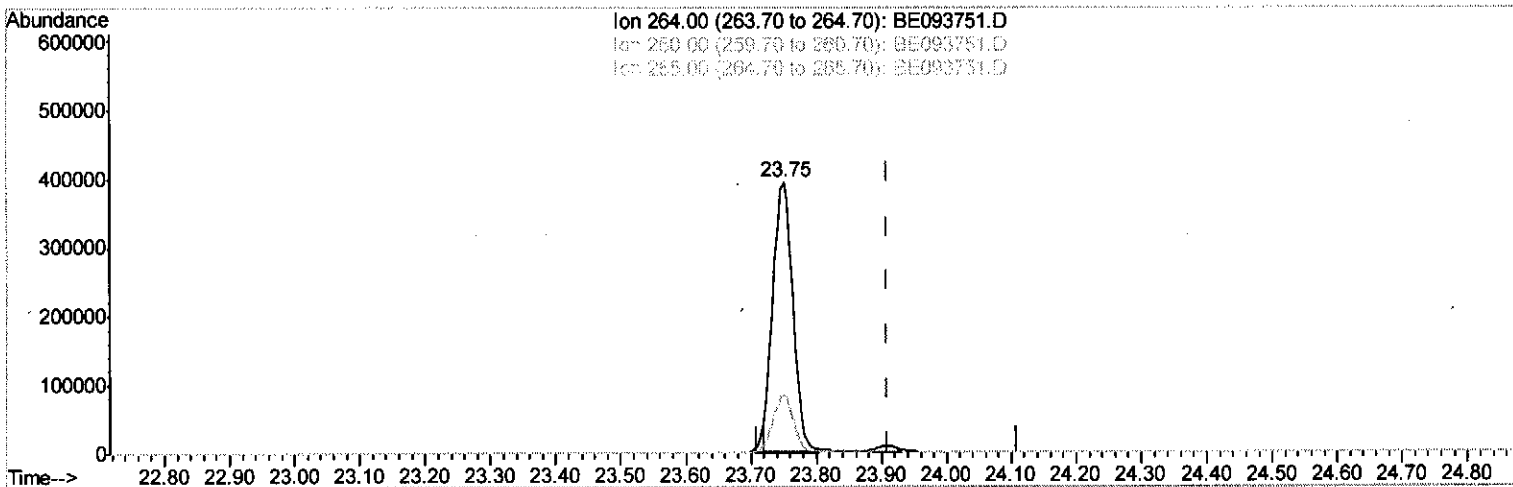

TIC: BE093751.D

(20) Perylene-d12 (I)

23.751min (-0.159) 0.40ng/ul

response 825318

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.07#
265.00	103.50	21.56#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\DATA\BE081017\
 Data File : BE093751.D
 Acq On : 10 Aug 2017 17:45
 Operator : SJ/JU
 Sample : I4455-04
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 C0AG3

Manual Integrations
 APPROVED

sohil
 8/14/2017 7:02:54 PM

Quant Time: Aug 11 17:30:09 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 11 06:07:04 2017
 Response via : Initial Calibration

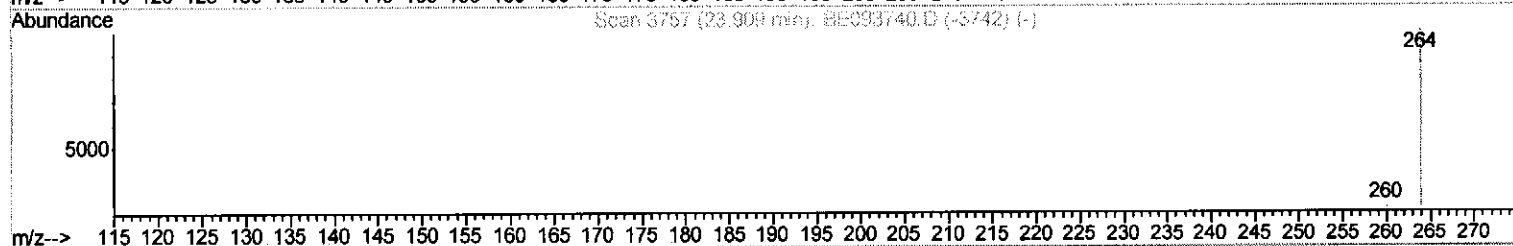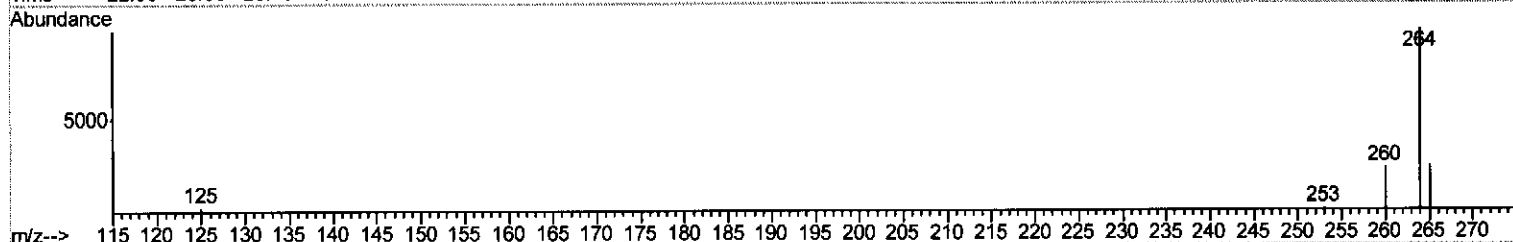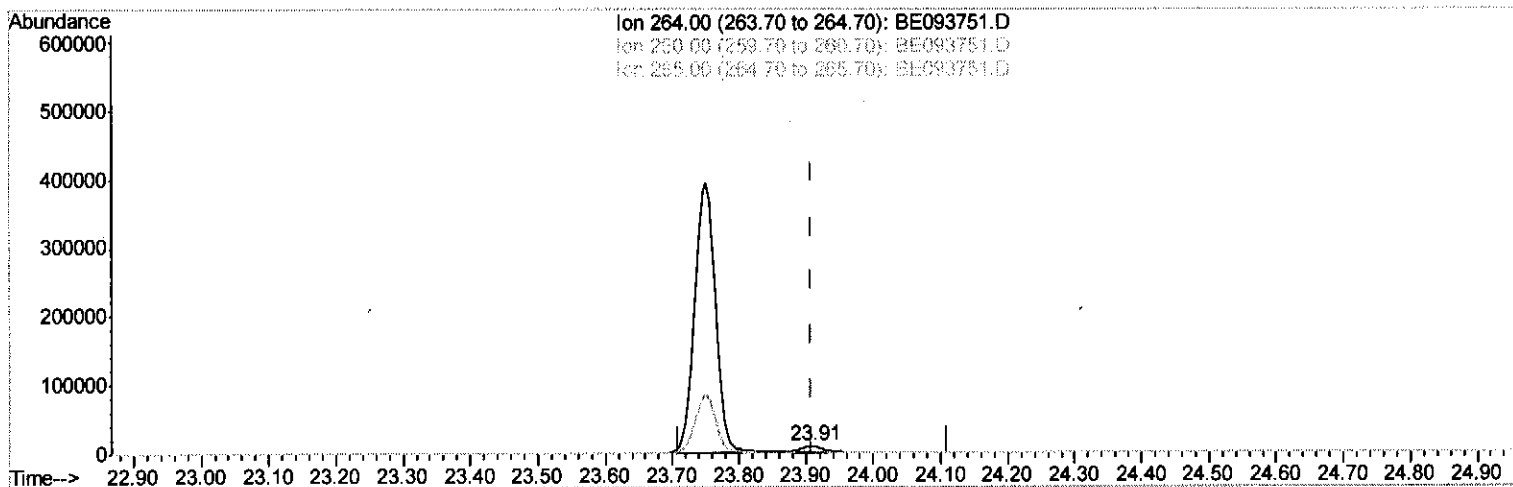

TIC: BE093751.D

(20) Perylene-d12 (I)

23.910min (+0.001) 0.40ng/ul m

response 17752

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	24.78
265.00	103.50	25.93#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE081017\
Data File : BE093751.D
Acq On : 10 Aug 2017 17:45
Operator : SJ/JU
Sample : I4455-04
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
C0AG3

Manual Integrations
APPROVED

sohil
8/14/2017 7:02:54 PM

Quant Time: Aug 11 18:12:59 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE072417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 11 06:07:04 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.92	152	3117	0.40	ng/ul	0.00
2) Naphthalene-d8	10.70	136	16075	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.53	164	9507	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.26	188	20325	0.40	ng/ul	0.00
16) Chrysene-d12	21.41	240	21686	0.40	ng/ul	0.00
20) Perylene-d12	23.91	264	17752m	0.40	ng/ul	0.00

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.28	152	4728	0.18	ng/ul	0.00
14) Fluoranthene-d10	19.27	212	11908	0.19	ng/ul	0.00

Target Compounds

					Qvalue	
12) Phenanthrene	17.29	178	1562	0.028	ng/ul#	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed