


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE081017\
Data File : BE093762.D
Acq On : 11 Aug 2017 1:10
Operator : SJ/JU
Sample : I4529-18
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
C0AB9

Manual Integrations
APPROVED

sohil
8/14/2017 7:04:20 PM

Quant Time: Aug 11 18:43:50 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE072417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 11 06:07:04 2017
Response via : Initial Calibration

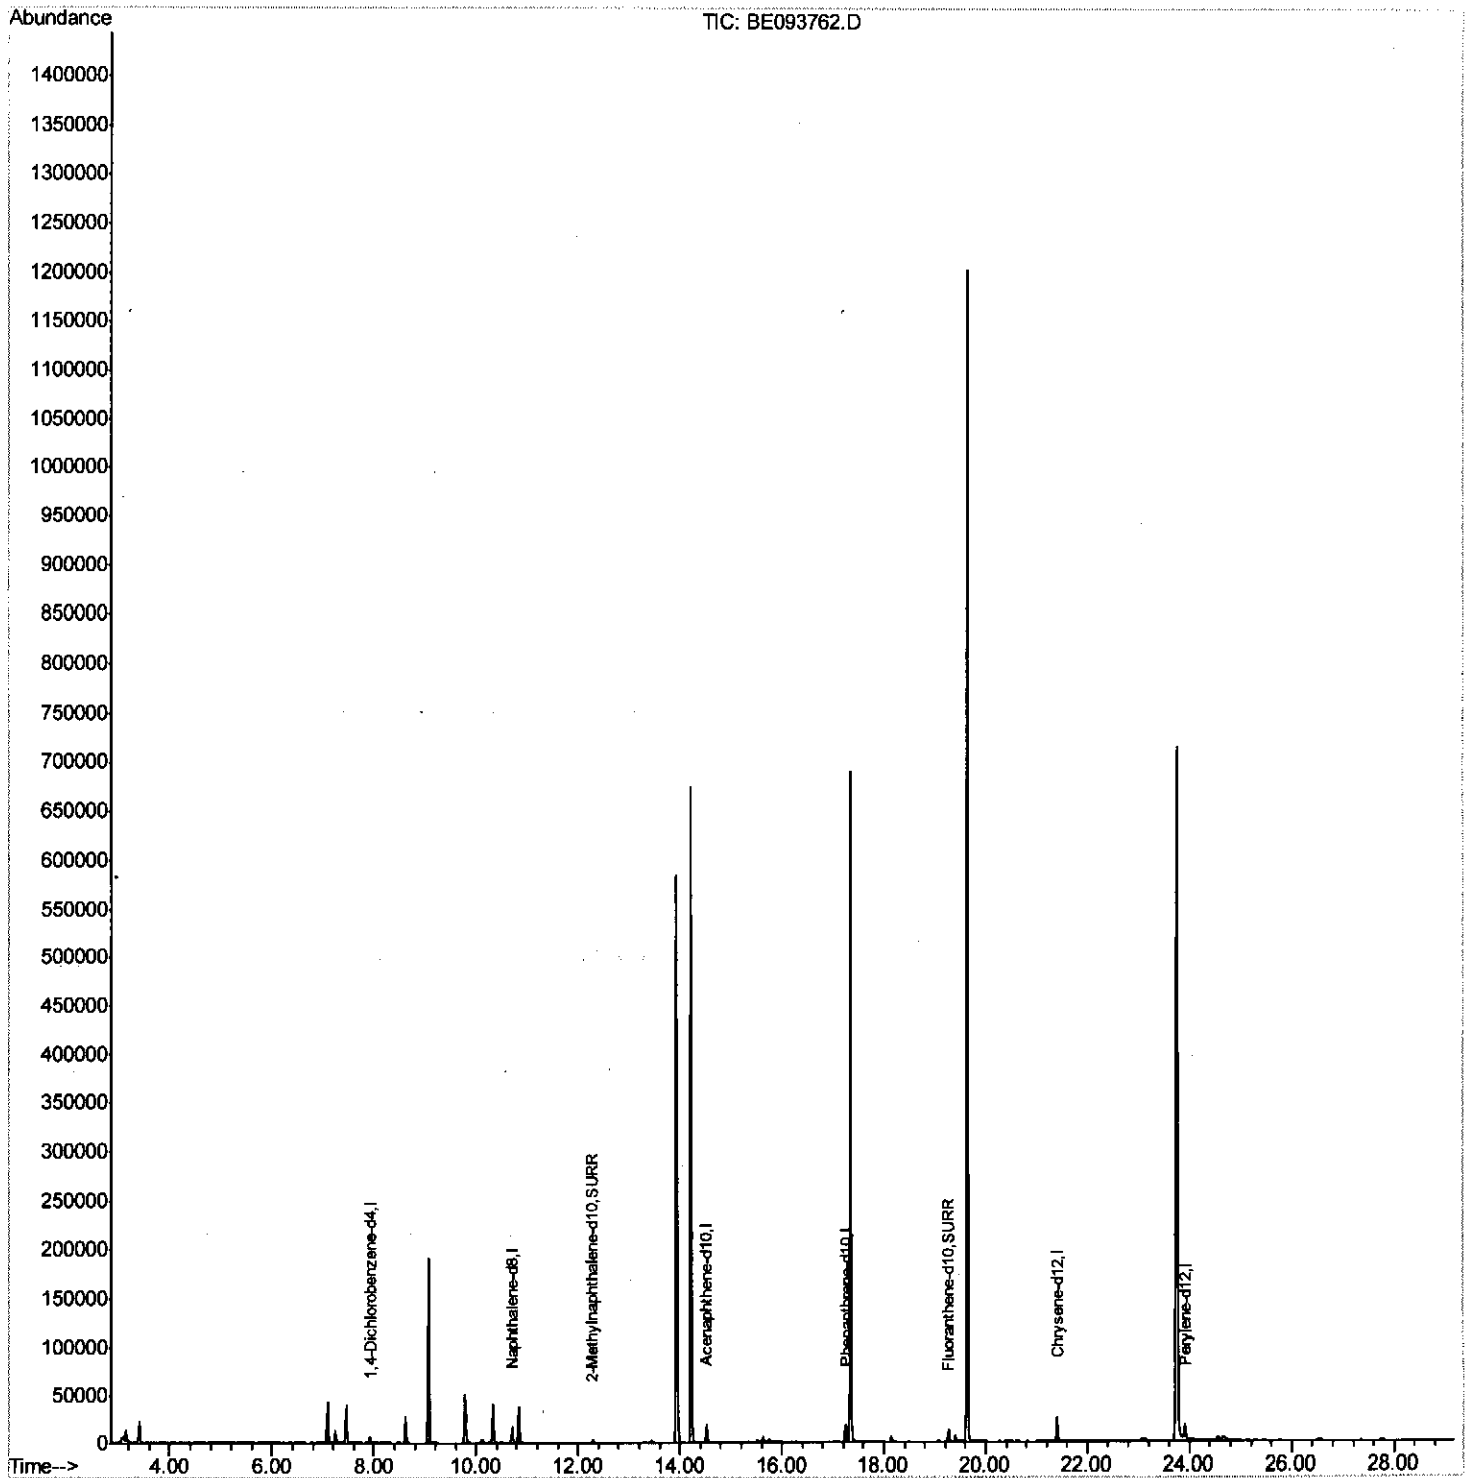




Data Path : Z:\HPCHEM1\BNA_E\DATA\BE081017\
Data File : BE093762.D
Acq On : 11 Aug 2017 1:10
Operator : SJ/JU
Sample : I4529-18
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AB9

Manual Integrations
APPROVED

sohil
8/14/2017 7:04:20 PM

Quant Time: Aug 11 17:31:02 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE072417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 11 06:07:04 2017
Response via : Initial Calibration

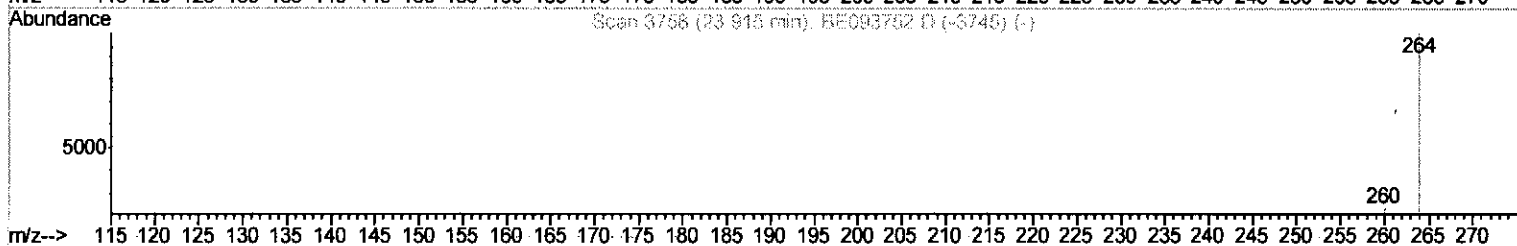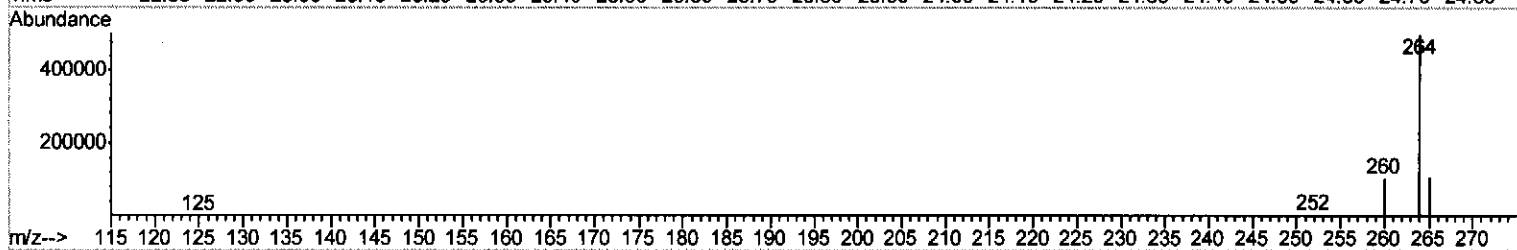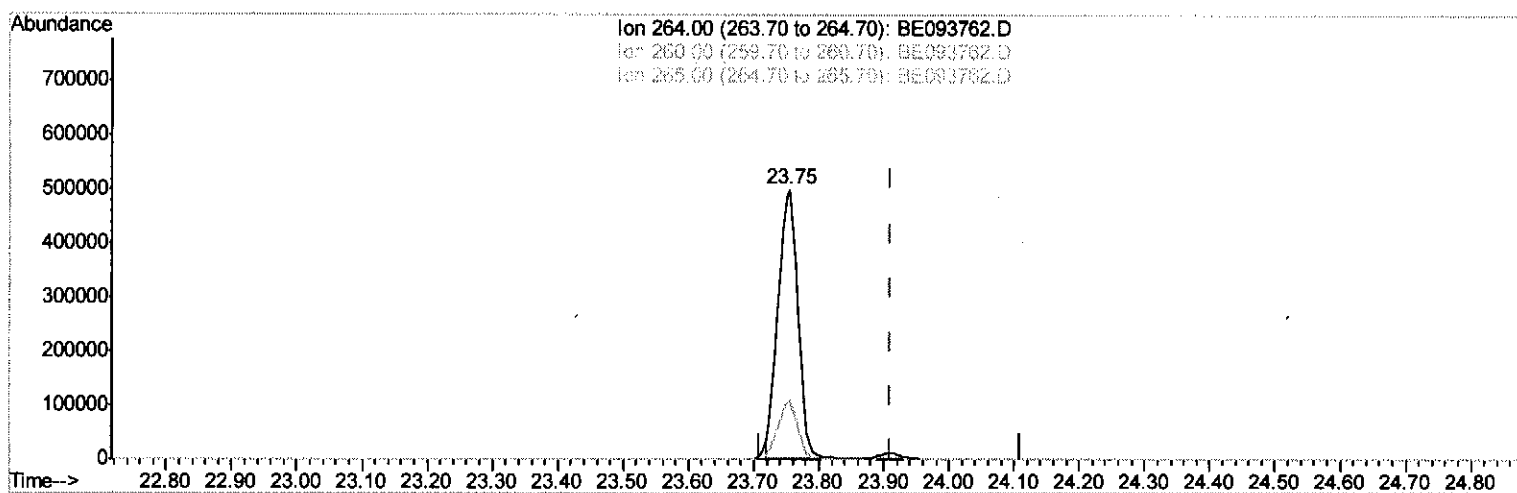

TIC: BE093762.D

(20) Perylene-d12 (I)

23.755min (-0.155) 0.40ng/ul

response 1057878

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	20.87#
265.00	103.50	21.68#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\DATA\BE081017\
Data File : BE093762.D
Acq On : 11 Aug 2017 1:10
Operator : SJ/JU
Sample : I4529-18
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
C0AB9

Manual Integrations
APPROVED

sohil
8/14/2017 7:04:20 PM

Quant Time: Aug 11 17:31:02 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE072417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 11 06:07:04 2017
Response via : Initial Calibration

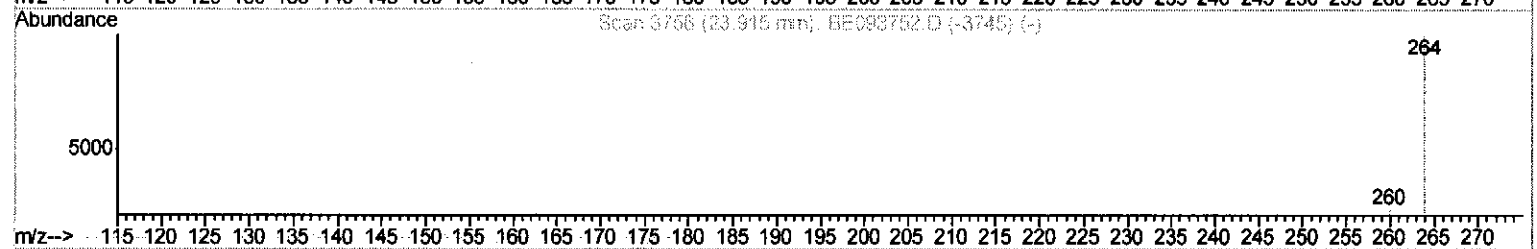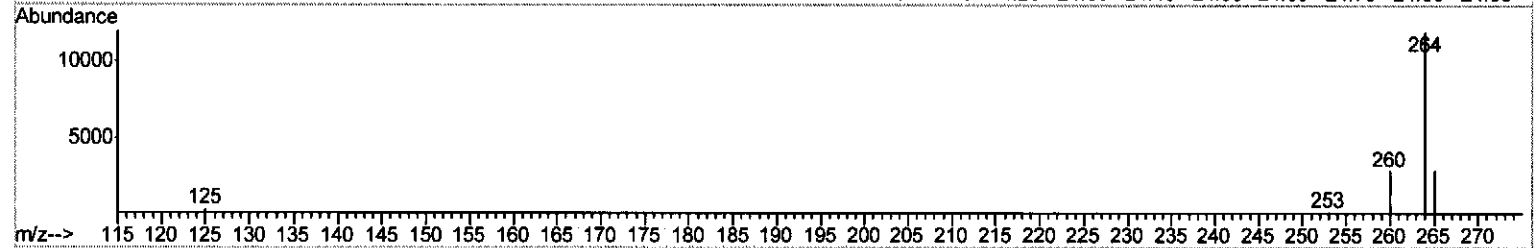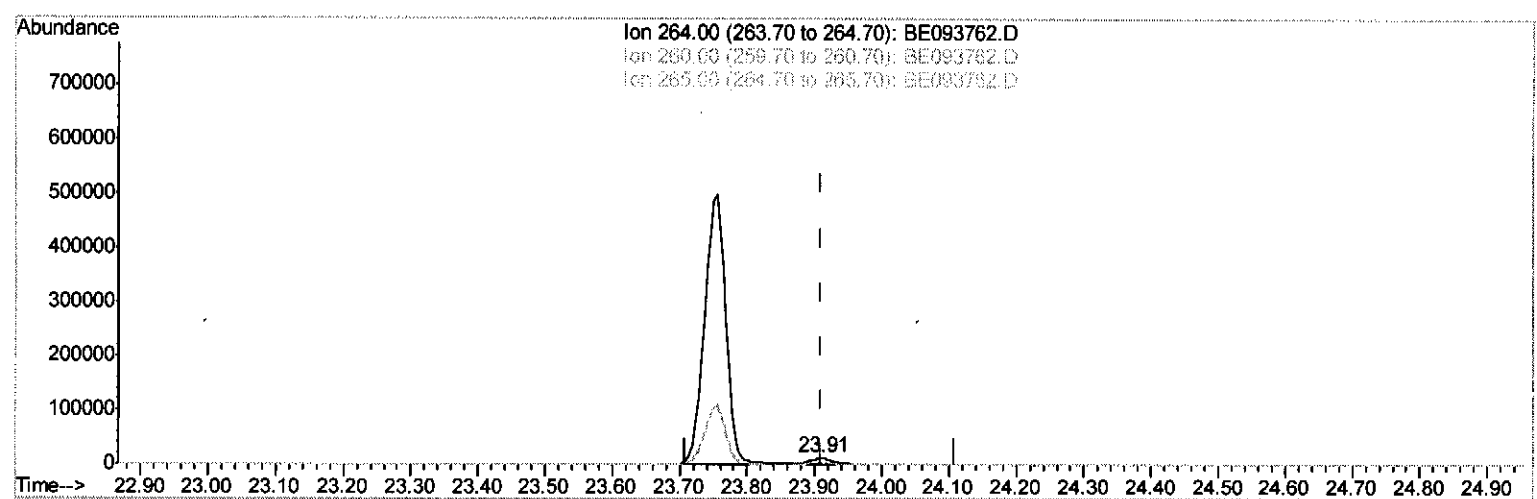

TIC: BE093762.D

(20) Perylene-d12 (I)

23.910min (+0.000) 0.40ng/ul m *JUS 8/14/17*

response 21514

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	24.49
265.00	103.50	24.75#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE081017\
Data File : BE093762.D
Acq On : 11 Aug 2017 1:10
Operator : SJ/JU
Sample : I4529-18
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AB9

Manual Integrations
APPROVED

sohil
8/14/2017 7:04:20 PM

Quant Time: Aug 11 18:43:50 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE072417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 11 06:07:04 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.92	152	3422	0.40	ng/ul	0.00
2) Naphthalene-d8	10.71	136	17917	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.52	164	11069	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.26	188	24572	0.40	ng/ul	0.00
16) Chrysene-d12	21.41	240	25027	0.40	ng/ul	0.00
20) Perylene-d12	23.91	264	21514m	0.40	ng/ul	0.00

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.29	152	5321	0.18	ng/ul	0.00
14) Fluoranthene-d10	19.27	212	14477	0.19	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed