

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE081115\
 Data File : BE090445.D
 Acq On : 12 Aug 2015 1:37
 Operator : UM/IZ
 Sample : SSTDCCC001
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SSTDCCC001

Manual Integrations
 APPROVED

MMDadoda
 8/12/2015 3:55:47 PM

Quant Time: Aug 12 06:42:22 2015
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE080515.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 06 12:28:08 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.58	152	21856	5.00	ng	-0.01
6) Naphthalene-d8	10.33	136	102498	5.00	ng	0.00
12) Acenaphthene-d10	14.19	164	61419	5.00	ng	0.00
18) Phenanthrene-d10	16.94	188	146201	5.00	ng	0.00
25) Chrysene-d12	21.09	240	163863	5.00	ng	0.00
32) Perylene-d12	23.40	264	144622	5.00	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.21	112	4466	1.36	ng	0.00
5) Phenol-d6	6.77	99	6928	1.19	ng	-0.01
7) Nitrobenzene-d5	8.72	82	7054	1.01	ng	-0.01
13) 2,4,6-Tribromophenol	15.71	330	1510	1.40	ng	0.00
14) 2-Fluorobiphenyl	12.82	172	17445	1.03	ng	0.00
27) Terphenyl-d14	19.56	244	26540	1.10	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.19	88	3070	1.08	ng	96
3) n-Nitrosodimethylamine	3.49	42	3538	1.05	ng	# 85
8) Nitrobenzene	8.77	77	7362	1.00	ng	99
9) Naphthalene	10.38	128	22886	1.01	ng	98
10) Hexachlorobutadiene	10.68	225	3931	1.09	ng	99
11) 2-Methylnaphthalene	12.00	142	14252	1.09	ng	98
15) Acenaphthylene	13.91	152	103647	1.04	ng	100
16) Acenaphthene	14.26	154	15610	1.01	ng	93
17) Fluorene	15.26	166	20500	1.02	ng	98
19) 4-Bromophenyl-phenylether	16.14	248	5604	0.99	ng	87
20) Hexachlorobenzene	16.27	284	27653	0.94	ng	98
21) Pentachlorophenol	16.61	266	1204	1.21	ng	98
22) Phenanthrene	16.98	178	36213	0.99	ng	100
23) Anthracene	17.07	178	32367	1.08	ng	100
24) Fluoranthene	18.98	202	37226	1.03	ng	99
26) Pyrene	19.35	202	38982	1.10	ng	100
28) Benzo(a)anthracene	21.08	228	38002	1.05	ng	100
29) Chrysene	21.13	228	44493m	1.01	ng	
30) Bis(2-ethylhexyl)phthalate	21.03	149	9482	1.11	ng	99
31) Indeno(1,2,3-cd)pyrene	25.79	276	32953	1.04	ng	96
33) Benzo(b)fluoranthene	22.70	252	29663	1.07	ng	100
34) Benzo(k)fluoranthene	22.74	252	38391m	0.95	ng	
35) Benzo(a)pyrene	23.29	252	26209	1.04	ng	99
36) Dibenzo(a,h)anthracene	25.80	278	24949	1.06	ng	99
37) Benzo(g,h,i)perylene	26.51	276	28321	1.06	ng	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE081115\
Data File : BE090445.D
Acq On : 12 Aug 2015 1:37
Operator : UM/IZ
Sample : SSTDCCC001
Misc :
ALS Vial : 2 Sample Multiplier: 1


Instrument :
BNA_E
ClientSampleId :
SSTDCCC001

Manual Integrations
APPROVED

MMDadoda
8/12/2015 3:55:47 PM

Quant Time: Aug 12 06:42:22 2015
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE080515.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 06 12:28:08 2015
Response via : Initial Calibration

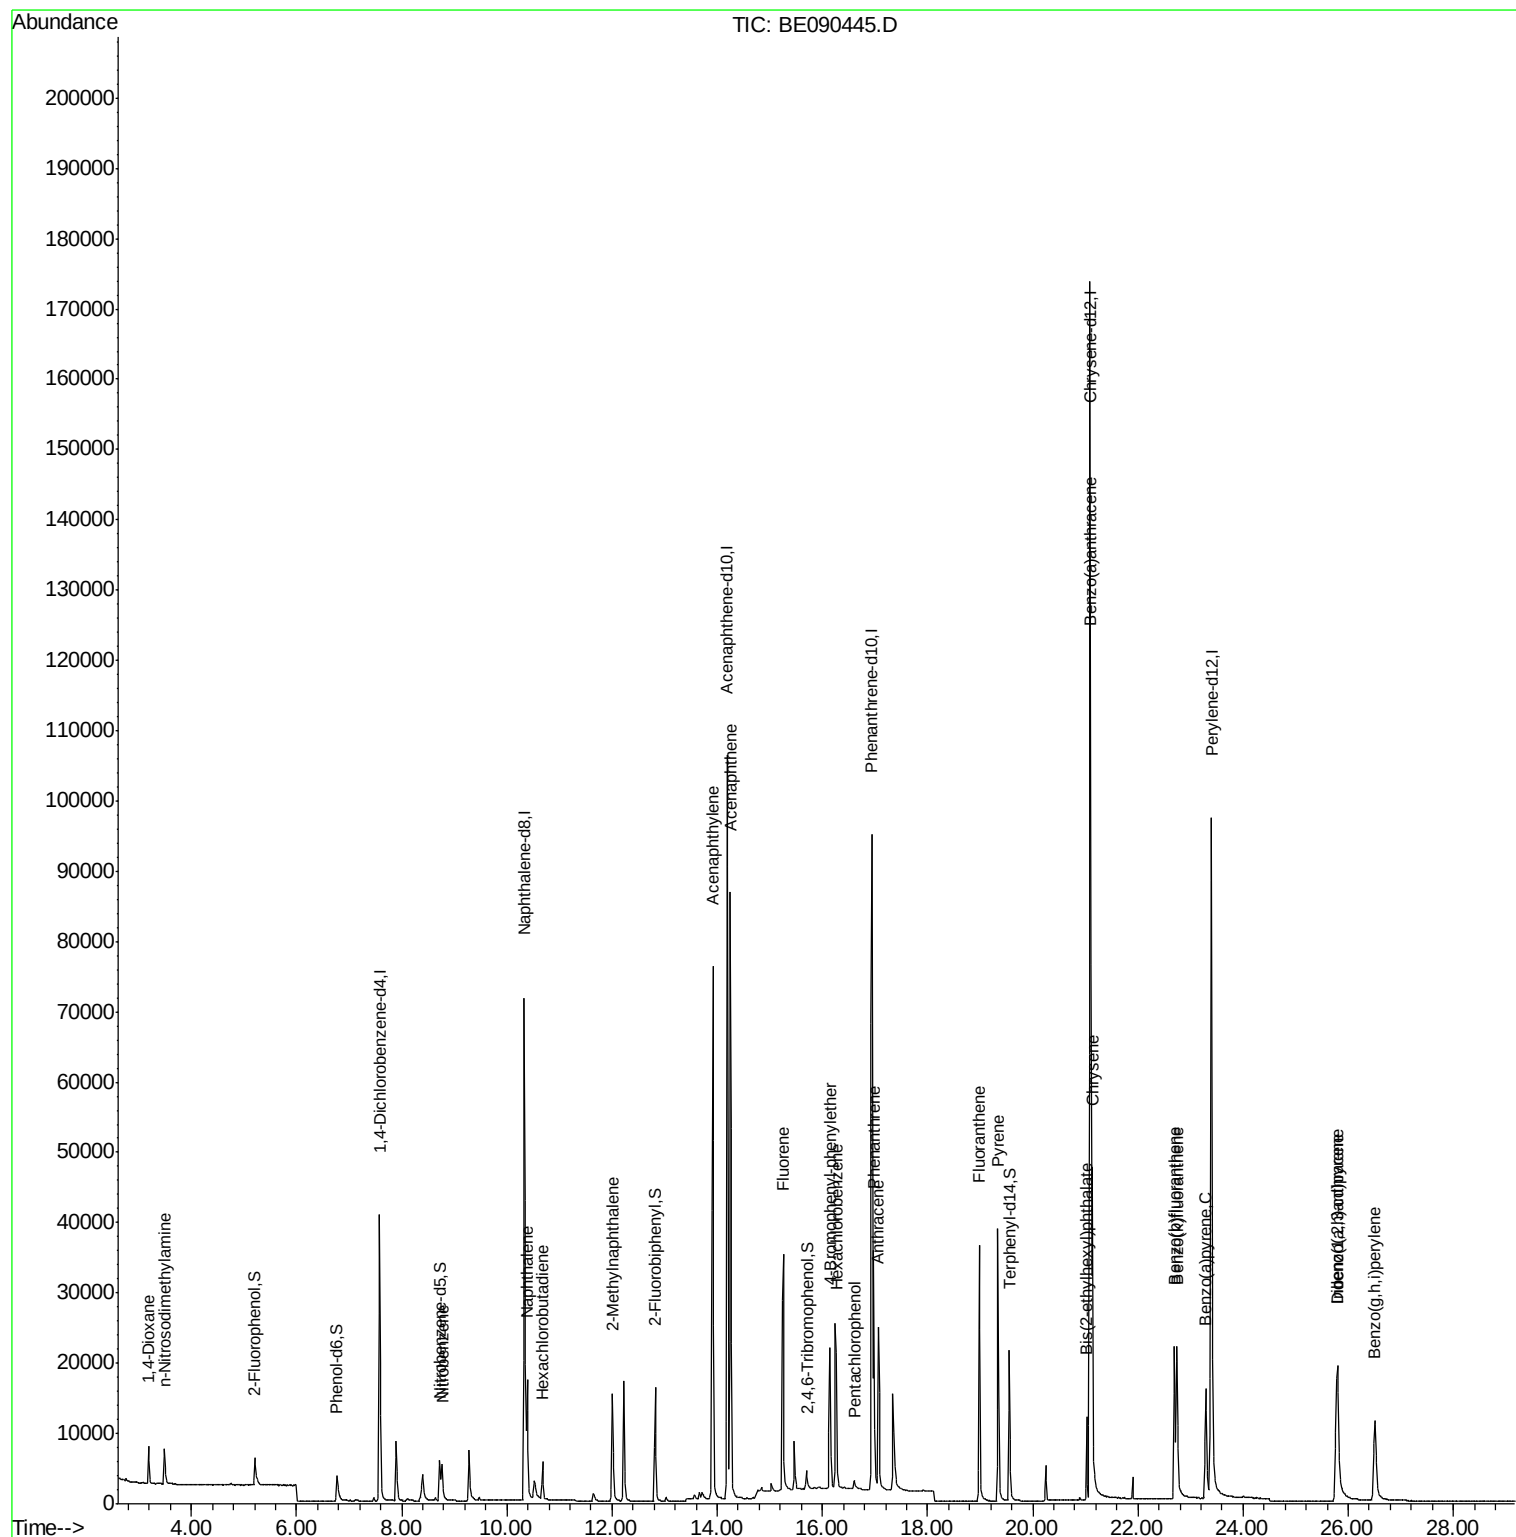


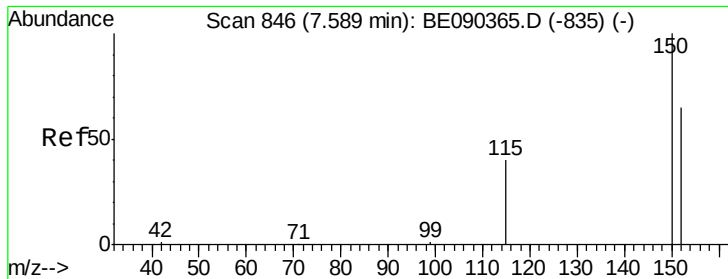

#1

1,4-Dichlorobenzene-d4
Concen: 5.00 ng
RT: 7.58 min Scan# 844
Delta R.T. -0.01 min
Lab File: BE090445.D
Acq: 12 Aug 2015 1:37




Instrument :
BNA_E
ClientSampleId :
SSTDCCC001

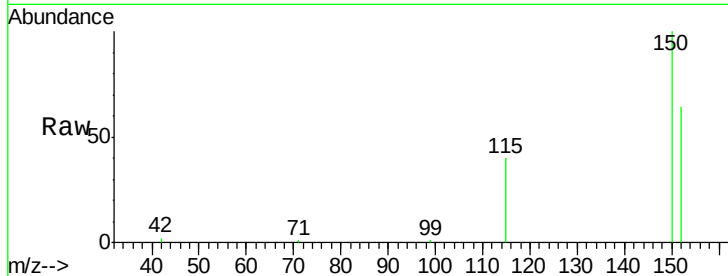

Tgt Ion	Ratio	Lower	Upper
152	100		
150	156.9	123.0	184.4
115	63.4	48.9	73.3

Manual Integrations
APPROVED




MMDadoda
8/12/2015 3:55:47 PM

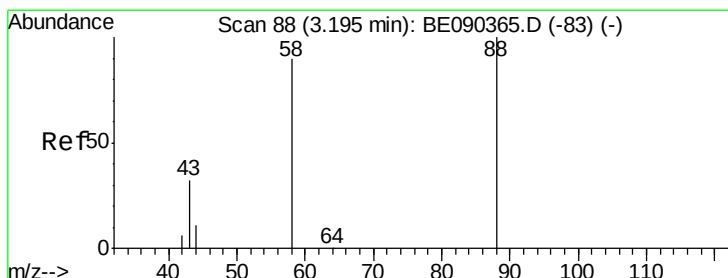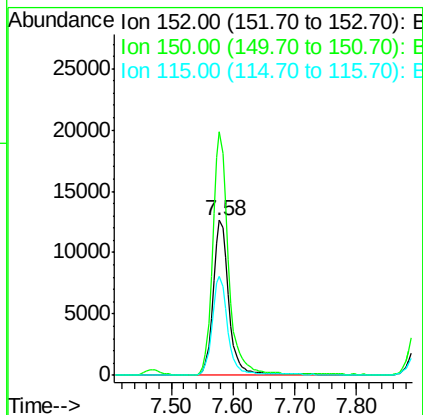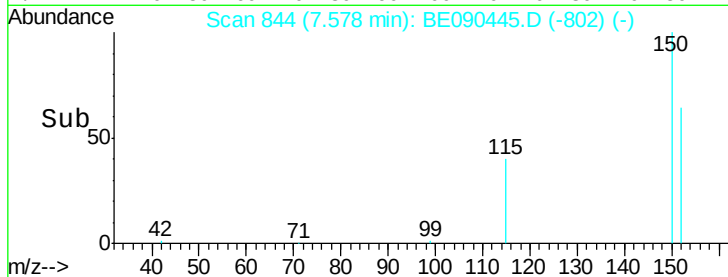


#2

1,4-Dioxane
Concen: 1.08 ng
RT: 3.19 min Scan# 87
Delta R.T. -0.01 min
Lab File: BE090445.D
Acq: 12 Aug 2015 1:37

Tgt Ion	Ratio	Lower	Upper
88	100		
58	84.4	70.0	105.0
43	32.0	28.4	42.6

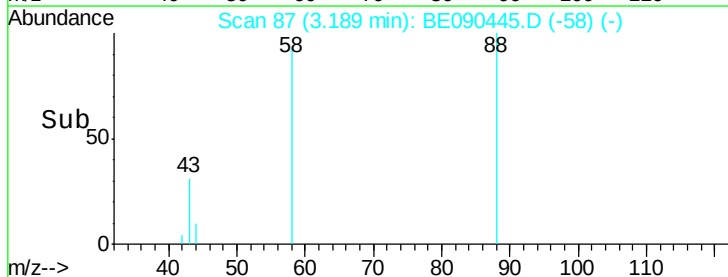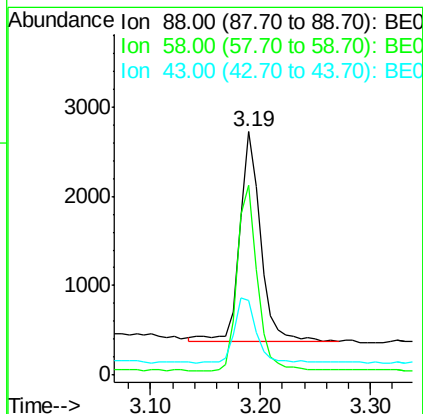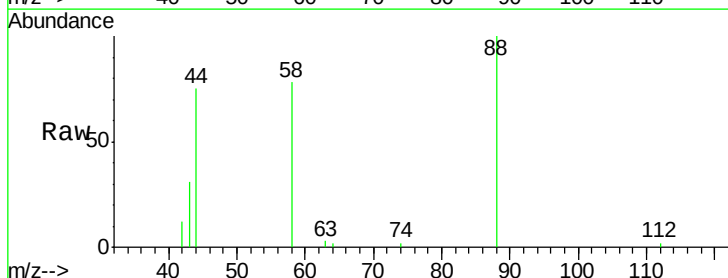

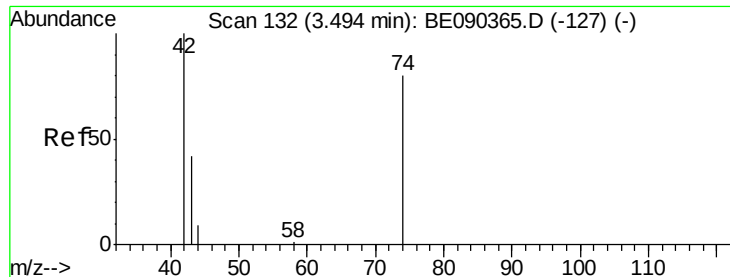

#3

n-Nitrosodimethylamine

Concen: 1.05 ng

RT: 3.49 min Scan# 131

Delta R.T. -0.01 min

Lab File: BE090445.D

Acq: 12 Aug 2015 1:37

Instrument :

BNA_E





ClientSampleId :

SSTDCCC001

Manual Integrations
APPROVED

MMDadoda
8/12/2015 3:55:47 PM

Tgt Ion:	42	Resp:	3538
Ion Ratio	Lower	Upper	
42	100		
74	108.3	75.2	112.8
44	16.5	8.7	13.1#

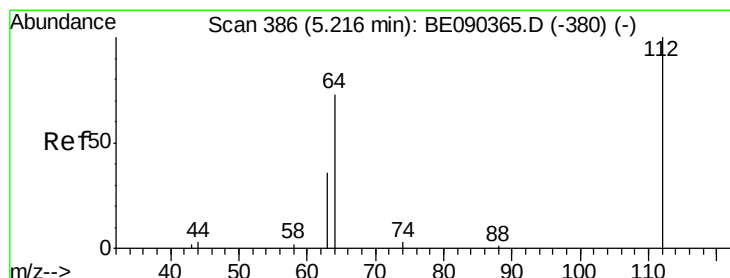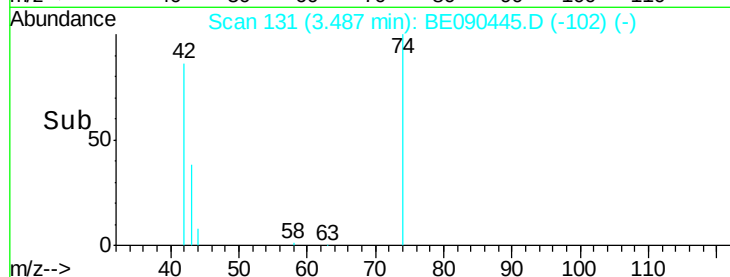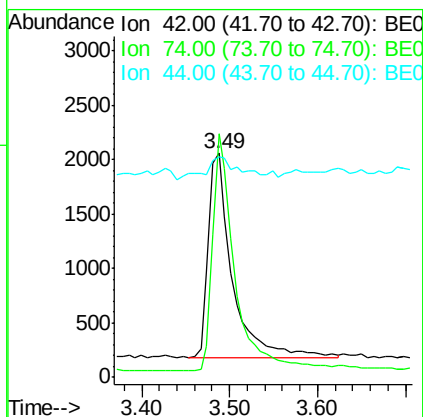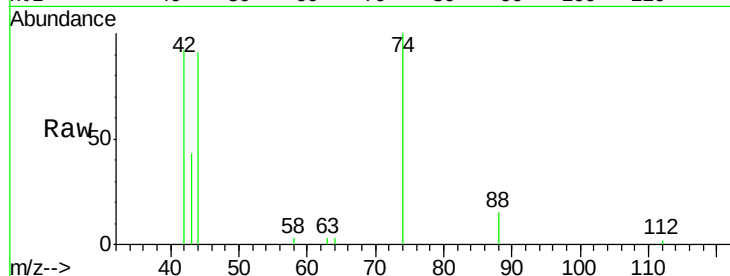

#4

2-Fluorophenol

Concen: 1.36 ng




RT: 5.21 min Scan# 385




Delta R.T. -0.01 min

Lab File: BE090445.D

Acq: 12 Aug 2015 1:37

Tgt Ion:	112	Resp:	4466
Ion Ratio	Lower	Upper	
112	100		
64	70.9	37.1	55.7#
63	36.6	19.5	29.3#

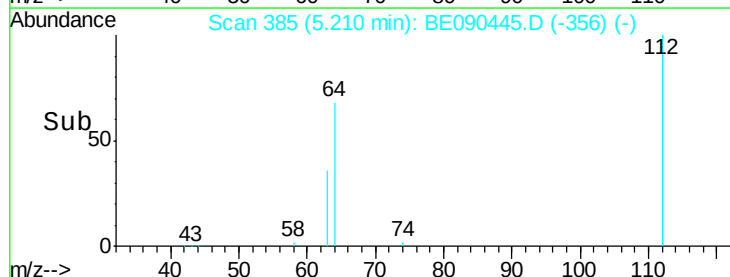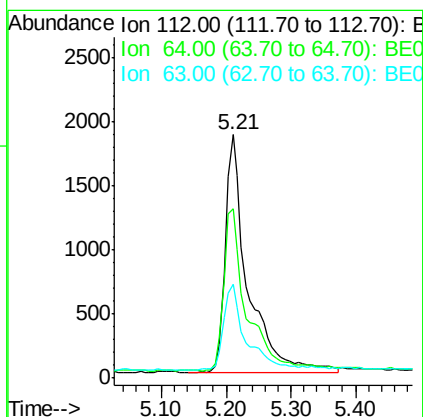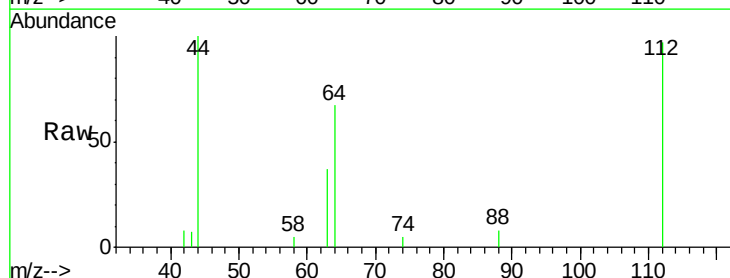

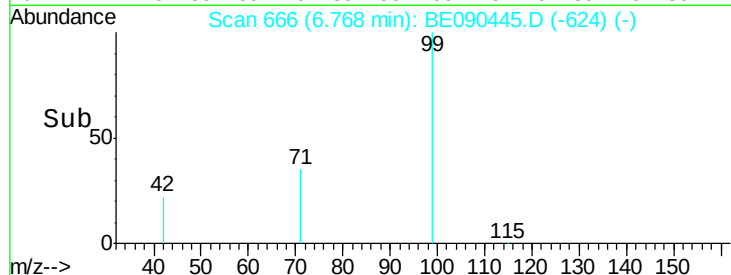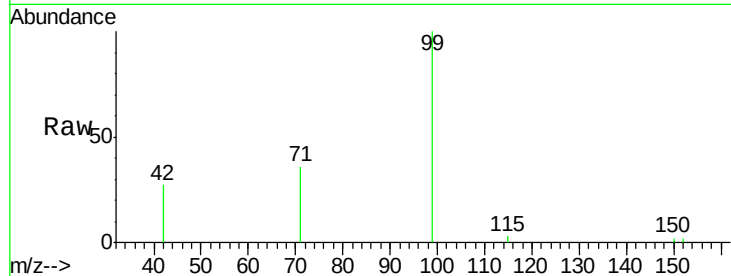

#5

Phenol-d6

Concen: 1.19 ng

RT: 6.77 min Scan# 666

Delta R.T. -0.01 min

Lab File: BE090445.D

Acq: 12 Aug 2015 1:37

Tgt Ion:	99	Resp:	6928
Ion Ratio	Lower	Upper	
99	100		
42	22.1	18.2	27.4
71	34.5	27.4	41.0

Instrument :





BNA_E

ClientSampleId :

SSTDCCC001

Manual Integrations
APPROVED

MMDadoda
8/12/2015 3:55:47 PM

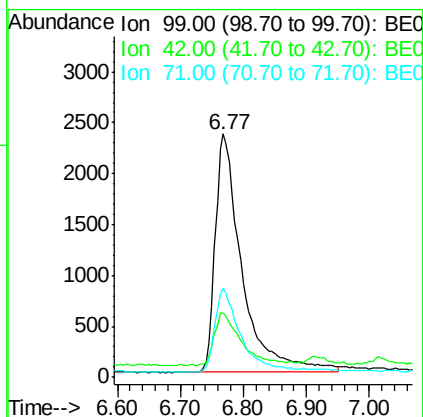

#6

Naphthalene-d8

Concen: 5.00 ng


RT: 10.33 min Scan# 1370


Delta R.T. -0.01 min

Lab File: BE090445.D

Acq: 12 Aug 2015 1:37

Tgt Ion:	136	Resp:	102498
Ion Ratio	Lower	Upper	
136	100		
137	10.9	8.7	13.1
54	12.3	9.4	14.0
68	8.6	6.5	9.7

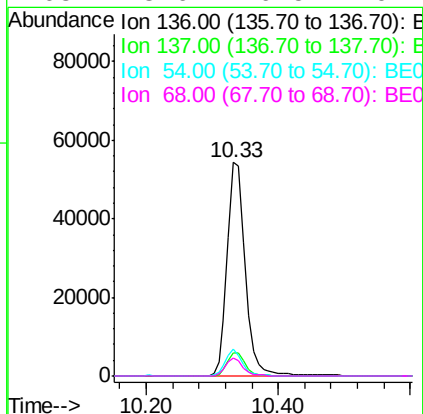



#7

Nitrobenzene-d5

Concen: 1.01 ng

RT: 8.72 min Scan# 1091

Delta R.T. -0.01 min

Lab File: BE090445.D


Acq: 12 Aug 2015 1:37

Instrument :

BNA_E

ClientSampleId :




SSTDCCC001



Tgt Ion:	82	Resp:	7054
Ion	Ratio	Lower	Upper
82	100		
128	29.1	25.0	37.6
54	60.2	48.8	73.2

Manual Integrations
APPROVED

MMDadoda
8/12/2015 3:55:47 PM

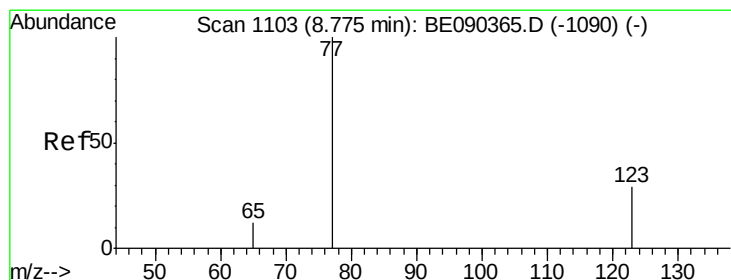

#8

Nitrobenzene

Concen: 1.00 ng




RT: 8.77 min Scan# 1101


Delta R.T. -0.01 min

Lab File: BE090445.D

Acq: 12 Aug 2015 1:37

Tgt Ion:	77	Resp:	7362
Ion	Ratio	Lower	Upper
77	100		
123	30.5	25.1	37.7
65	11.6	9.3	13.9





#9

Naphthalene

Concen: 1.01 ng

RT: 10.38 min Scan# 1377

Delta R.T. -0.01 min

Lab File: BE090445.D


Acq: 12 Aug 2015 1:37

Instrument :

BNA_E

ClientSampleId :




SSTDCCC001



Tgt Ion	Ratio	Lower	Upper
128	100		
129	11.3	9.8	14.6
127	13.0	10.6	16.0

Manual Integrations
APPROVED

MMDadoda
8/12/2015 3:55:47 PM

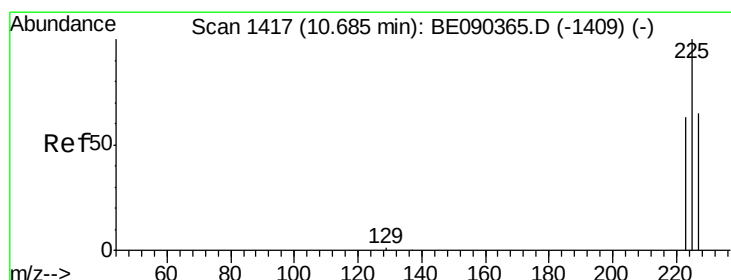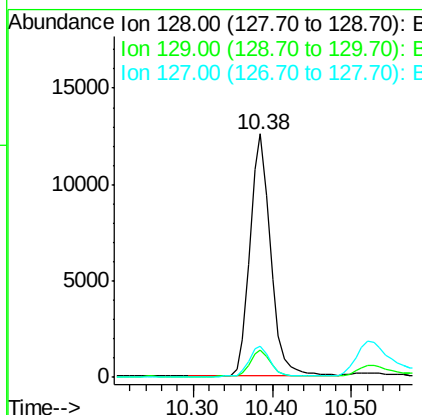

#10

Hexachlorobutadiene

Concen: 1.09 ng




RT: 10.68 min Scan# 1416


Delta R.T. -0.01 min

Lab File: BE090445.D

Acq: 12 Aug 2015 1:37

Tgt Ion	Ratio	Lower	Upper
225	100		
223	61.9	50.6	75.8
227	63.0	50.7	76.1



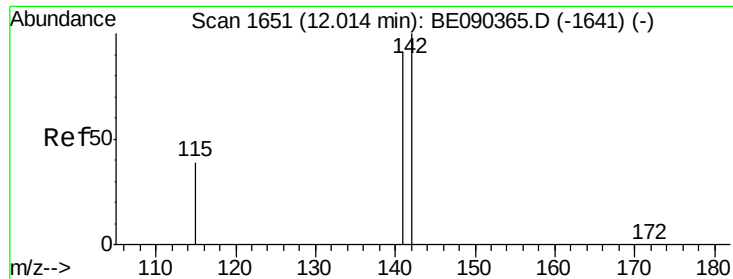





#11
2-Methylnaphthalene
Concen: 1.09 ng
RT: 12.00 min Scan# 1649
Delta R.T. -0.01 min
Lab File: BE090445.D
Acq: 12 Aug 2015 1:37

Instrument :
BNA_E
ClientSampleId :
SSTDCCC001

Tgt Ion	Ratio	Lower	Upper
142	100		
141	88.3	72.6	109.0
115	38.3	31.6	47.4




Manual Integrations
APPROVED


MMDadoda
8/12/2015 3:55:47 PM

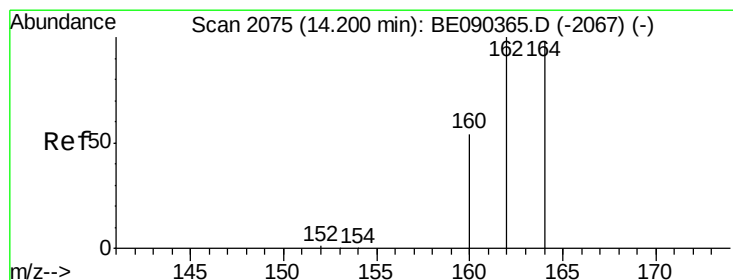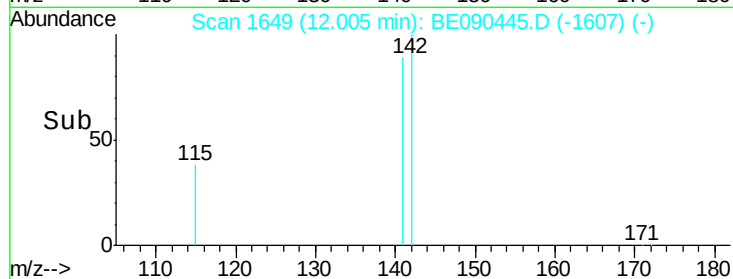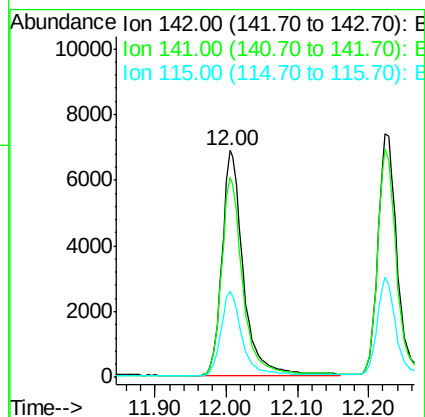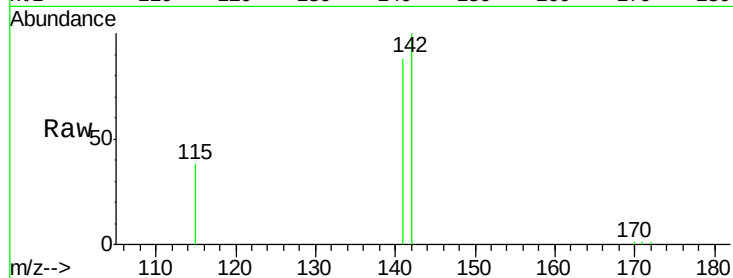

#12
Acenaphthene-d10
Concen: 5.00 ng
RT: 14.19 min Scan# 2074
Delta R.T. -0.01 min
Lab File: BE090445.D
Acq: 12 Aug 2015 1:37

Tgt Ion	Ratio	Lower	Upper
164	100		
162	105.2	81.8	122.8
160	52.2	44.2	66.4

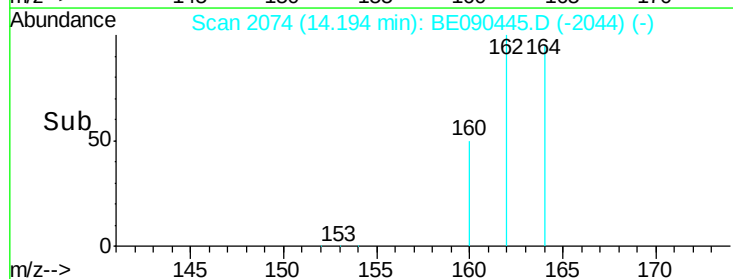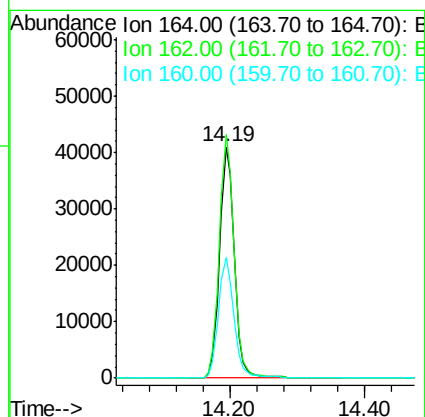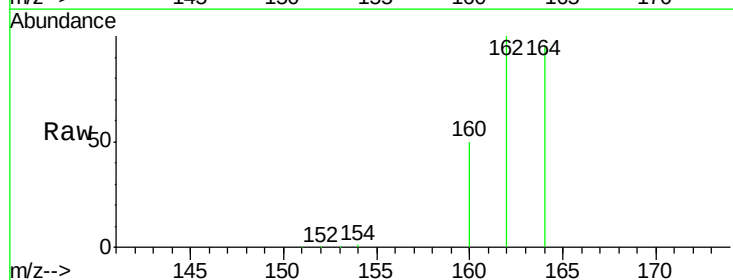

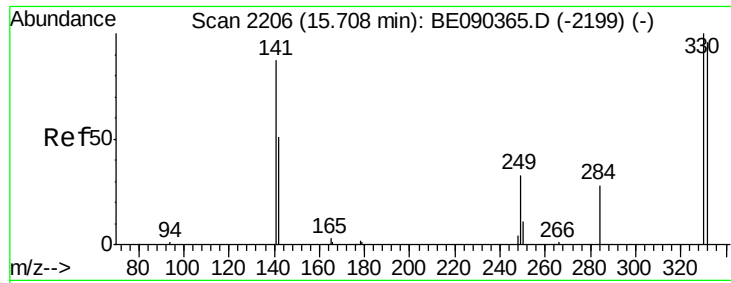





#13
 2,4,6-Tribromophenol
 Concen: 1.40 ng
 RT: 15.71 min Scan# 2206
 Delta R.T. 0.00 min
 Lab File: BE090445.D
 Acq: 12 Aug 2015 1:37

Instrument :
 BNA_E
 ClientSampleId :
 SSTDCCC001

Tgt Ion	Ratio	Resp	Lower	Upper
330	100	1510		
332	98.7	75.8	113.6	
141	173.2	114.4	171.6#	




Manual Integrations
 APPROVED


MMDadoda
 8/12/2015 3:55:47 PM

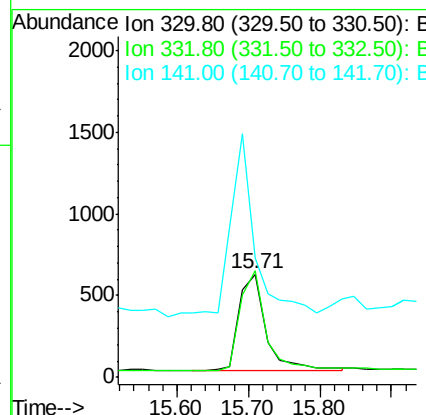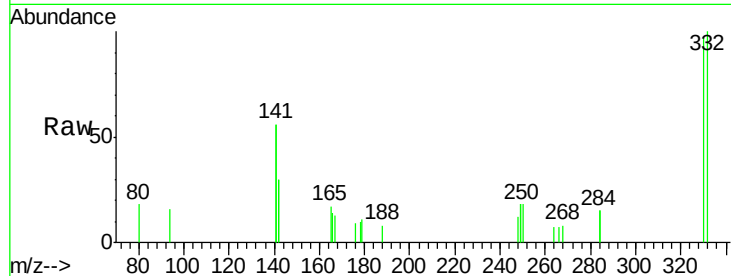

#14
 2-Fluorobiphenyl
 Concen: 1.03 ng
 RT: 12.82 min Scan# 1828
 Delta R.T. -0.00 min
 Lab File: BE090445.D
 Acq: 12 Aug 2015 1:37

Tgt Ion	Ratio	Resp	Lower	Upper
172	100	17445		
171	34.6	28.5	42.7	
170	24.8	19.8	29.8	

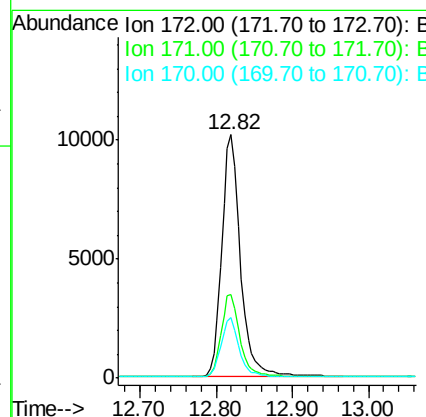

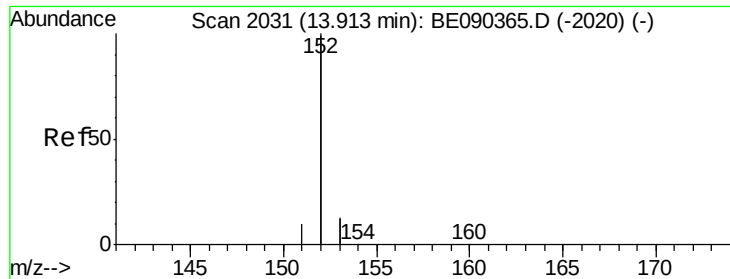





#15
Acenaphthylene
Concen: 1.04 ng
RT: 13.91 min Scan# 2031
Delta R.T. 0.00 min
Lab File: BE090445.D
Acq: 12 Aug 2015 1:37

Instrument :
BNA_E
ClientSampleId :
SSTDCCC001

Tgt Ion	Ratio	Lower	Upper
152	100		
151	4.8	3.8	5.8
153	12.9	10.3	15.5




Manual Integrations
APPROVED


MMDadoda
8/12/2015 3:55:47 PM

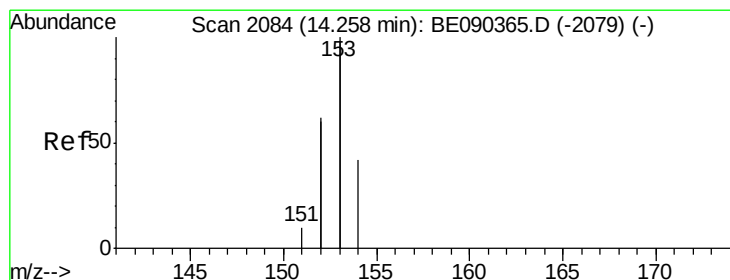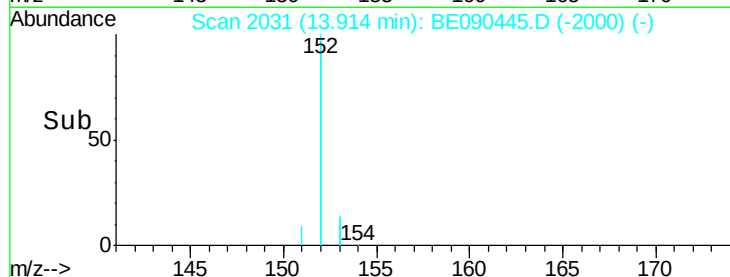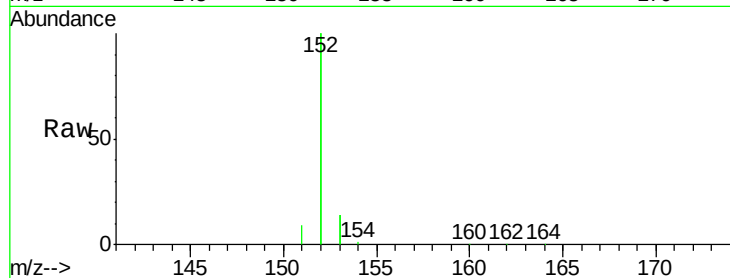

#16
Acenaphthene
Concen: 1.01 ng
RT: 14.26 min Scan# 2084
Delta R.T. 0.00 min
Lab File: BE090445.D
Acq: 12 Aug 2015 1:37

Tgt Ion	Ratio	Lower	Upper
154	100		
153	463.4	376.2	564.2
152	264.9	235.0	352.4

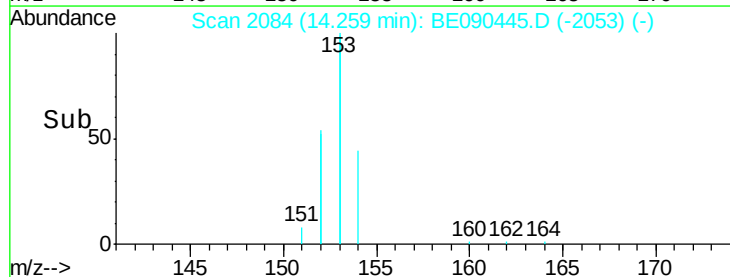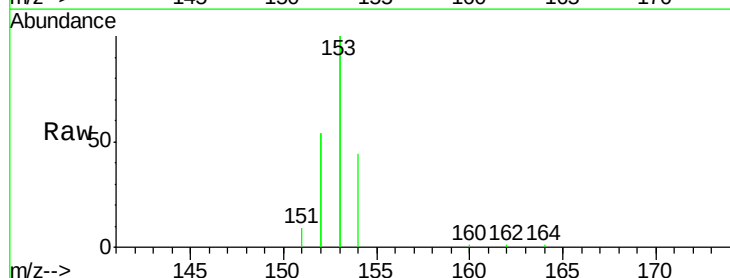







#17
Fluorene
 Concen: 1.02 ng
 RT: 15.26 min Scan# 2180
 Delta R.T. 0.00 min
 Lab File: BE090445.D
 Acq: 12 Aug 2015 1:37

Instrument :
 BNA_E
 ClientSampleId :
 SSTDCCC001

Tgt Ion	Ratio	Lower	Upper
166	100		
165	100.0	81.5	122.3
167	14.1	11.4	17.0




Manual Integrations
APPROVED


MMDadoda
 8/12/2015 3:55:47 PM

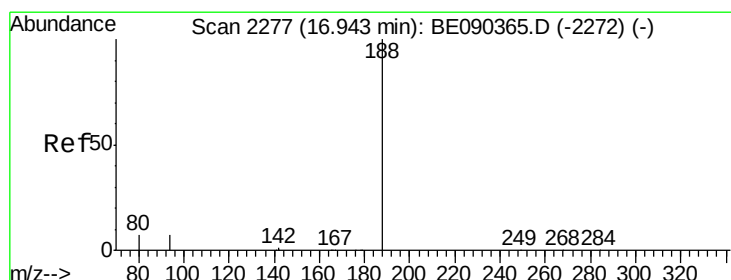

#18
Phenanthrene-d10
 Concen: 5.00 ng
 RT: 16.94 min Scan# 2277
 Delta R.T. 0.00 min
 Lab File: BE090445.D
 Acq: 12 Aug 2015 1:37

Tgt Ion	Ratio	Lower	Upper
188	100		
94	5.4	5.7	8.5#
80	5.7	5.8	8.8#









#19
4-Bromophenyl-phenylether
Concen: 0.99 ng
RT: 16.14 min Scan# 2231
Delta R.T. 0.00 min
Lab File: BE090445.D
Acq: 12 Aug 2015 1:37

Instrument :
BNA_E
ClientSampleId :
SSTDCCC001

Tgt Ion	Ratio	Lower	Upper
248	100		
250	99.5	79.0	118.6
141	332.9	239.5	359.3




Manual Integrations
APPROVED




MMDadoda
8/12/2015 3:55:47 PM

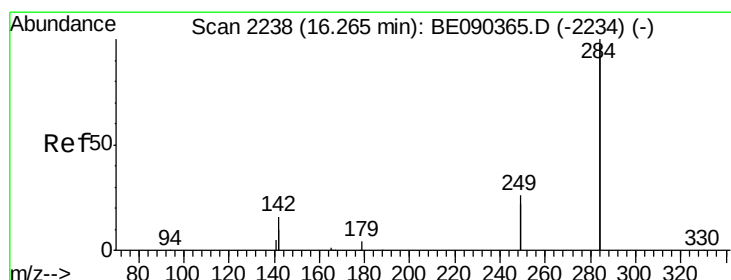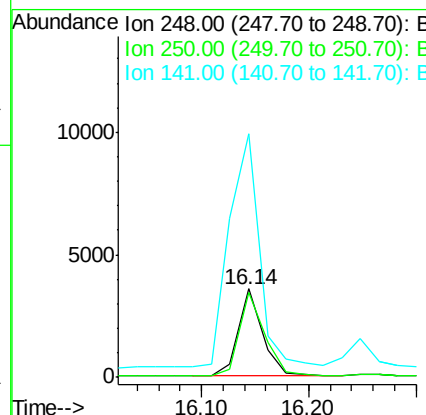

#20
Hexachlorobenzene
Concen: 0.94 ng
RT: 16.27 min Scan# 2238
Delta R.T. 0.00 min
Lab File: BE090445.D
Acq: 12 Aug 2015 1:37

Tgt Ion	Ratio	Lower	Upper
284	100		
142	37.4	30.1	45.1
249	30.5	25.7	38.5

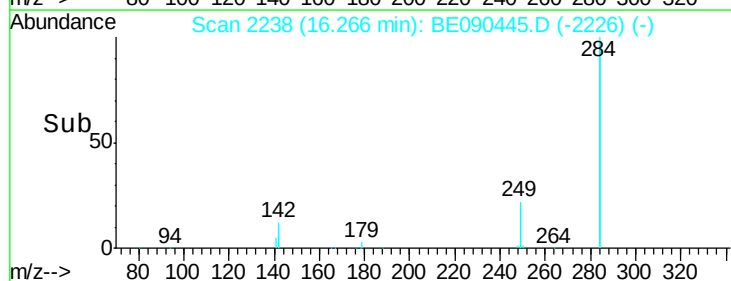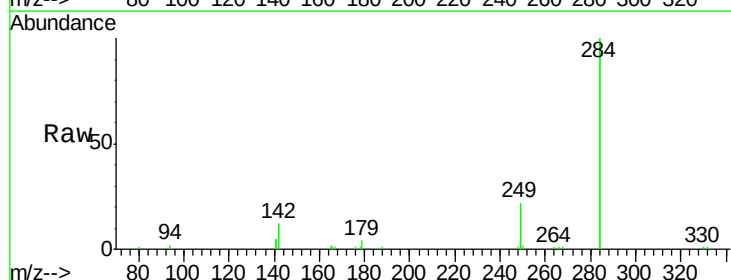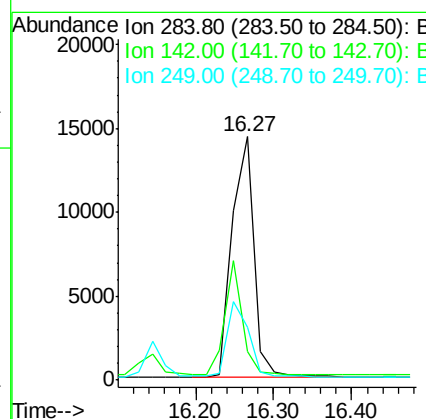

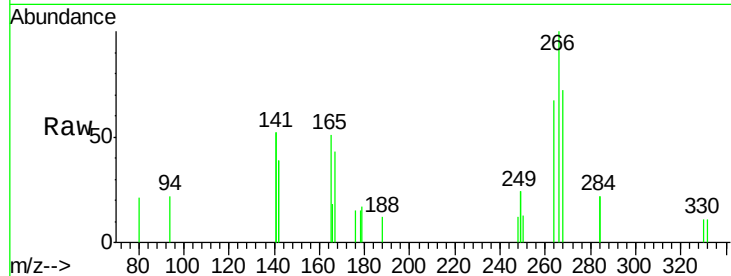





#21
 Pentachlorophenol
 Concen: 1.21 ng
 RT: 16.61 min Scan# 2258
 Delta R.T. 0.00 min
 Lab File: BE090445.D
 Acq: 12 Aug 2015 1:37

Tgt Ion	Ratio	Lower	Upper
266	100		
268	72.3	58.5	87.7
264	66.7	56.0	84.0

Instrument :
 BNA_E
 ClientSampleId :
 SSTDCCC001


Manual Integrations
 APPROVED


MMDadoda
 8/12/2015 3:55:47 PM



#22
 Phenanthrene
 Concen: 0.99 ng
 RT: 16.98 min Scan# 2279
 Delta R.T. 0.00 min
 Lab File: BE090445.D
 Acq: 12 Aug 2015 1:37

Tgt Ion	Ratio	Lower	Upper
178	100		
176	19.3	15.4	23.2
179	15.4	12.5	18.7

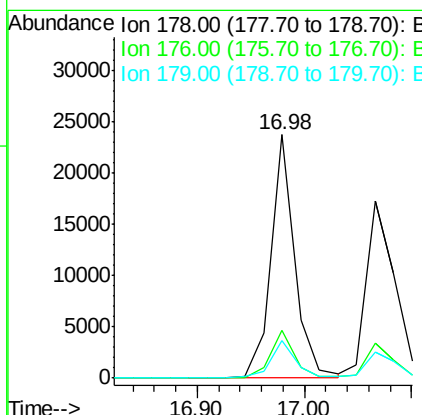







#23
 Anthracene
 Concen: 1.08 ng
 RT: 17.07 min Scan# 2284
 Delta R.T. -0.02 min
 Lab File: BE090445.D
 Acq: 12 Aug 2015 1:37

Instrument :
 BNA_E
 ClientSampleId :
 SSTDCCC001

Tgt Ion:	178	Resp:	32367
Ion Ratio	Lower	Upper	
178	100		
176	18.6	14.9	22.3
179	15.0	12.2	18.4




Manual Integrations
 APPROVED


MMDadoda
 8/12/2015 3:55:47 PM

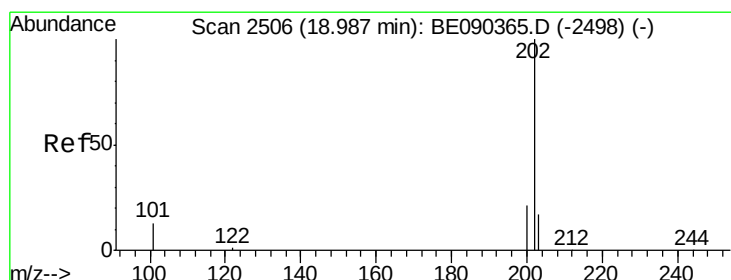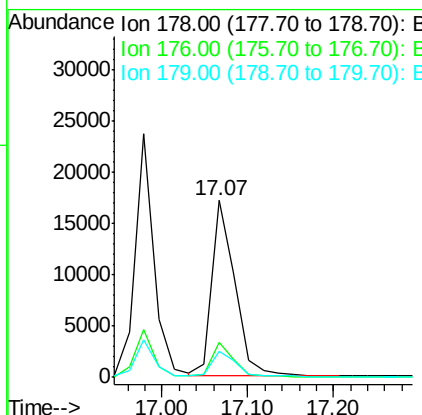

#24
 Fluoranthene
 Concen: 1.03 ng
 RT: 18.98 min Scan# 2505
 Delta R.T. -0.01 min
 Lab File: BE090445.D
 Acq: 12 Aug 2015 1:37

Tgt Ion:	202	Resp:	37226
Ion Ratio	Lower	Upper	
202	100		
101	13.3	10.3	15.5
203	17.3	13.7	20.5

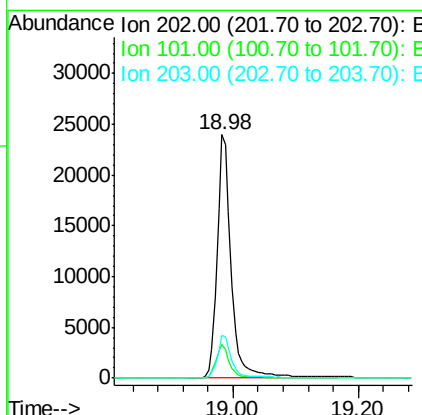



#25

Chrysene-d12

Concen: 5.00 ng

RT: 21.09 min Scan# 2863

Delta R.T. -0.01 min

Lab File: BE090445.D


Acq: 12 Aug 2015 1:37

Instrument :

BNA_E

ClientSampleId :




SSTDCCC001

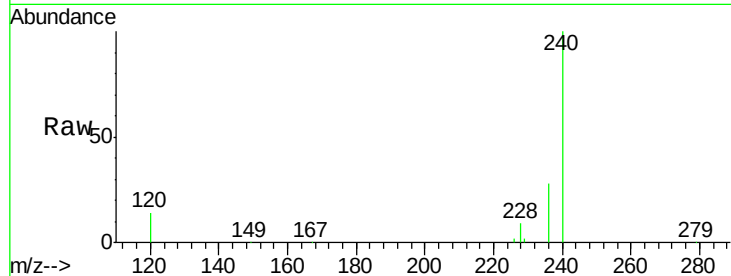

Tgt Ion:	240	Resp:	163863
Ion Ratio	Lower	Upper	
240	100		
120	13.5	8.3	12.5#
236	28.0	21.0	31.4

Manual Integrations
APPROVED

MMDadoda
8/12/2015 3:55:47 PM

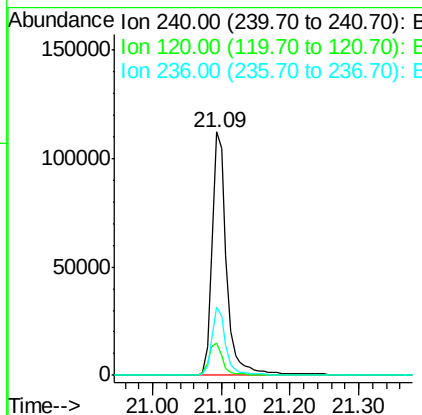

#26

Pyrene

Concen: 1.10 ng




RT: 19.35 min Scan# 2574


Delta R.T. 0.00 min

Lab File: BE090445.D

Acq: 12 Aug 2015 1:37

Tgt Ion:	202	Resp:	38982
Ion Ratio	Lower	Upper	
202	100		
200	20.9	16.7	25.1
203	17.3	13.8	20.8

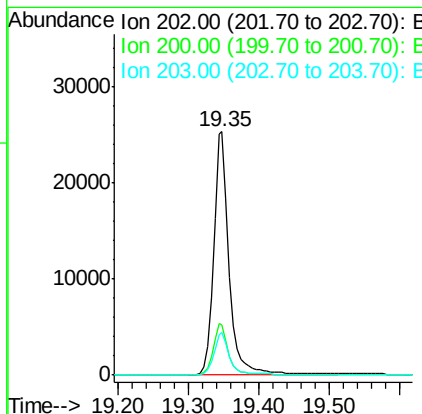

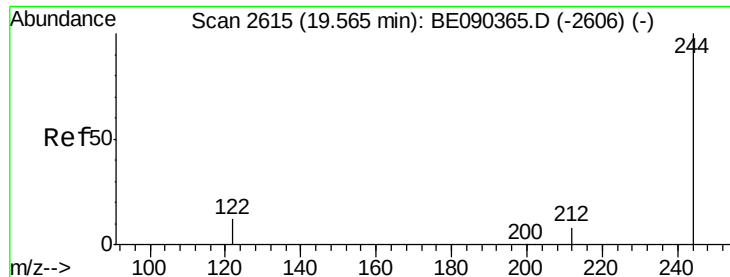

#27

Terphenyl-d14

Concen: 1.10 ng

RT: 19.56 min Scan# 2614

Delta R.T. -0.01 min

Lab File: BE090445.D


Acq: 12 Aug 2015 1:37

Instrument :

BNA_E

ClientSampleId :




SSTDCCC001

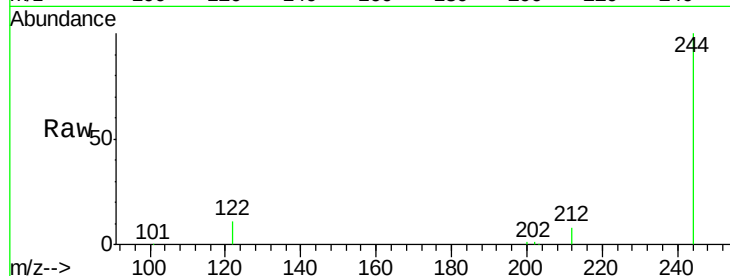

Tgt Ion:	244	Resp:	26540
Ion Ratio	Lower	Upper	
244	100		
212	8.1	6.6	9.8
122	11.4	10.2	15.4

Manual Integrations
APPROVED

MMDadoda
8/12/2015 3:55:47 PM

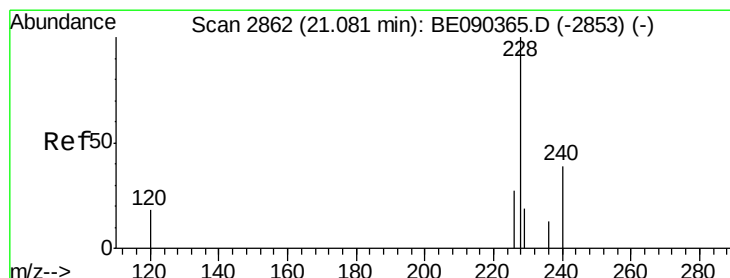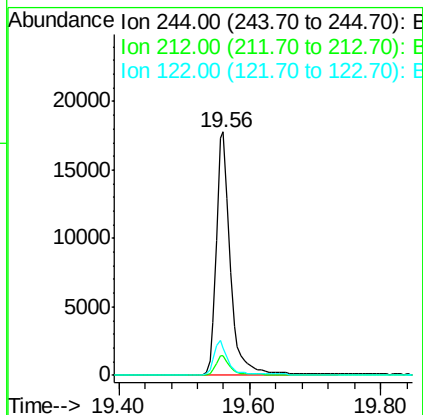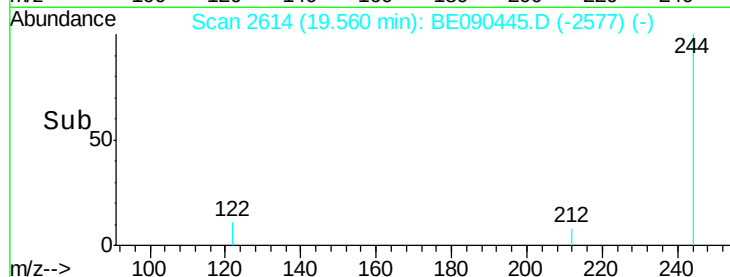

#28

Benzo(a)anthracene

Concen: 1.05 ng




RT: 21.08 min Scan# 2861


Delta R.T. -0.00 min

Lab File: BE090445.D

Acq: 12 Aug 2015 1:37

Tgt Ion:	228	Resp:	38002
Ion Ratio	Lower	Upper	
228	100		
226	27.3	21.9	32.9
229	19.4	15.4	23.0

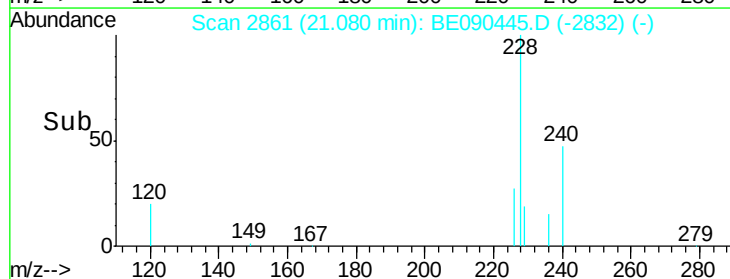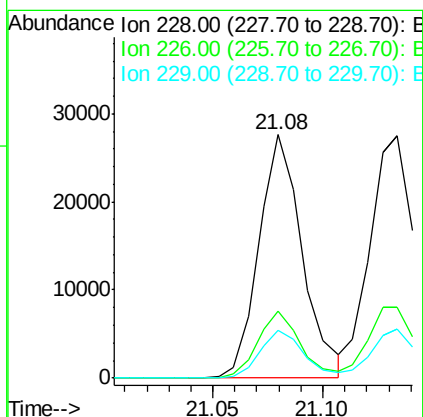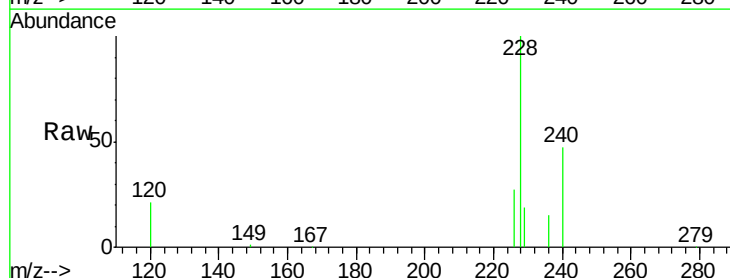



#29

Chrysene

Concen: 1.01 ng m

RT: 21.13 min Scan# 2869

Delta R.T. -0.00 min

Lab File: BE090445.D

Acq: 12 Aug 2015 1:37

Instrument :

BNA_E





ClientSampleId :

SSTDCCC001

Tgt Ion:	228	Resp:	44493
Ion Ratio	Lower	Upper	
228	100		
226	29.0	23.1	34.7
229	20.2	15.8	23.8

Manual Integrations
APPROVED

MMDadoda
8/12/2015 3:55:47 PM

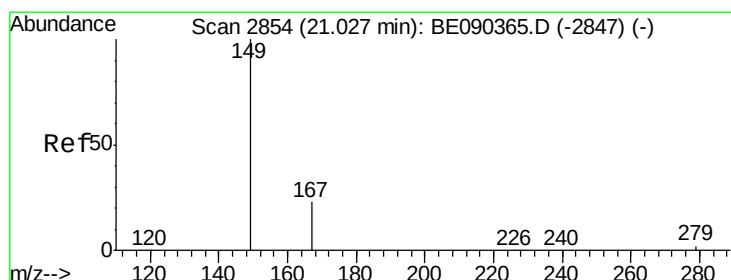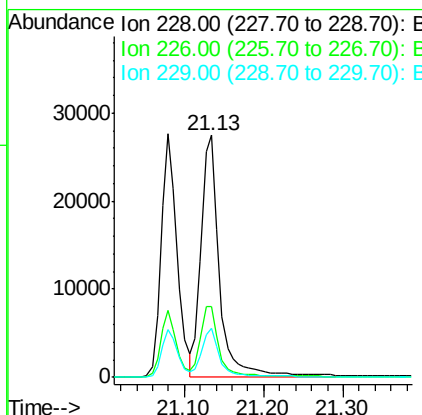

#30

Bis(2-ethylhexyl)phthalate

Concen: 1.11 ng




RT: 21.03 min Scan# 2853


Delta R.T. -0.00 min

Lab File: BE090445.D

Acq: 12 Aug 2015 1:37

Tgt Ion:	149	Resp:	9482
Ion Ratio	Lower	Upper	
149	100		
167	25.5	19.8	29.8
279	3.1	2.4	3.6



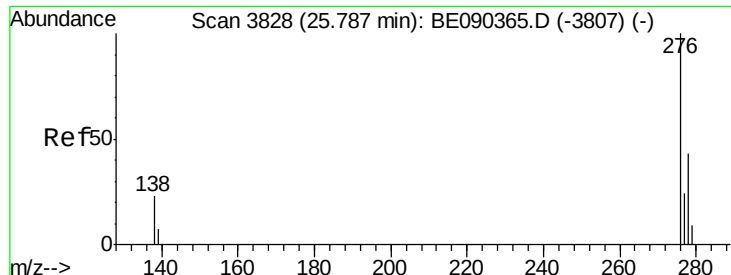





#31
 Indeno(1,2,3-cd)pyrene
 Concen: 1.04 ng
 RT: 25.79 min Scan# 3828
 Delta R.T. -0.00 min
 Lab File: BE090445.D
 Acq: 12 Aug 2015 1:37

Instrument :
 BNA_E
 ClientSampleId :
 SSTDCCC001

Tgt Ion	Ratio	Resp	Lower	Upper
276	100	32953		
138	26.0		18.8	28.2
277	24.1		18.2	27.4




Manual Integrations
 APPROVED


MMDadoda
 8/12/2015 3:55:47 PM

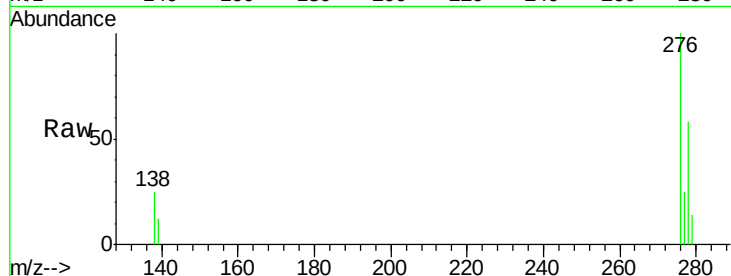

#32
 Perylene-d12
 Concen: 5.00 ng
 RT: 23.40 min Scan# 3308
 Delta R.T. 0.00 min
 Lab File: BE090445.D
 Acq: 12 Aug 2015 1:37

Tgt Ion	Ratio	Resp	Lower	Upper
264	100	144622		
260	24.5		20.1	30.1
265	22.0		17.2	25.8



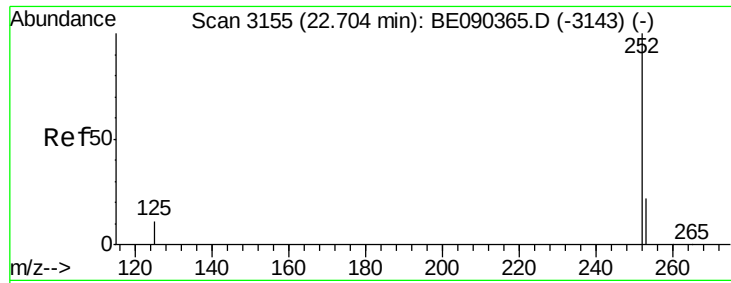

#33

Benzo(b)fluoranthene

Concen: 1.07 ng

RT: 22.70 min Scan# 3153

Delta R.T. -0.01 min

Lab File: BE090445.D


Acq: 12 Aug 2015 1:37

Instrument :

BNA_E

ClientSampleId :




SSTDCCC001



Tgt Ion	Ratio	Lower	Upper
252	100		
253	22.5	18.1	27.1
125	11.5	9.4	14.2

Manual Integrations
APPROVED

MMDadoda
8/12/2015 3:55:47 PM

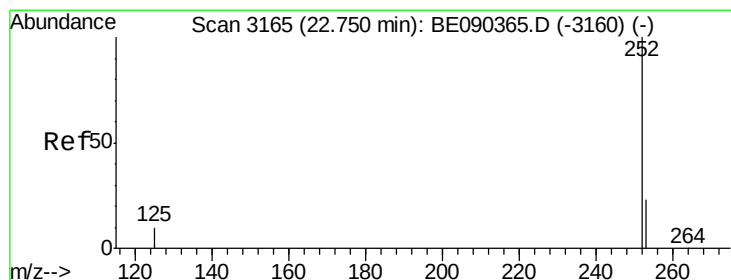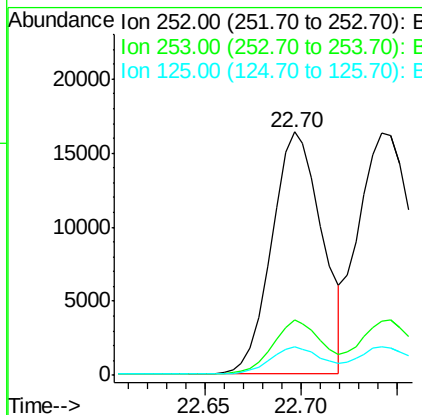

#34

Benzo(k)fluoranthene

Concen: 0.95 ng m




RT: 22.74 min Scan# 3163


Delta R.T. -0.01 min

Lab File: BE090445.D

Acq: 12 Aug 2015 1:37

Tgt Ion	Ratio	Lower	Upper
252	100		
253	22.3	18.1	27.1
125	11.7	9.1	13.7

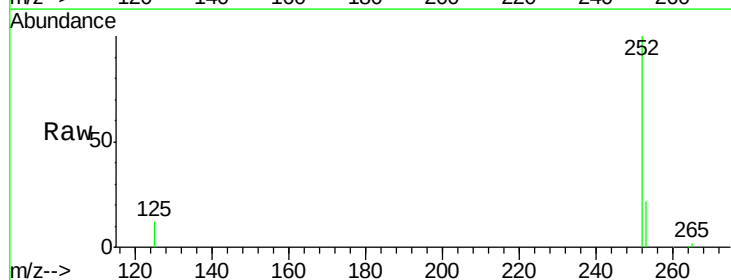







#35
Benzo(a)pyrene
Concen: 1.04 ng
RT: 23.29 min Scan# 3284
Delta R.T. -0.00 min
Lab File: BE090445.D
Acq: 12 Aug 2015 1:37

Instrument :
BNA_E
ClientSampleId :
SSTDCCC001

Tgt Ion	Ratio	Lower	Upper
252	100		
253	22.4	17.6	26.4
125	13.0	9.8	14.6




Manual Integrations
APPROVED


MMDadoda
8/12/2015 3:55:47 PM

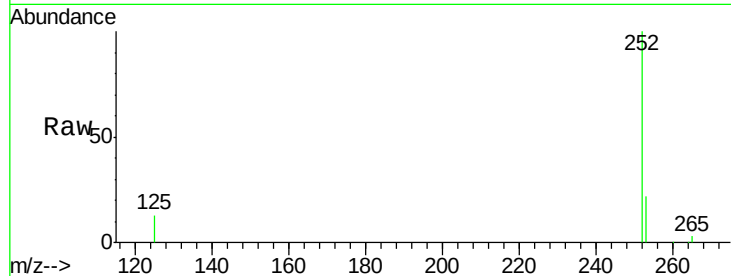

#36
Dibenzo(a,h)anthracene
Concen: 1.06 ng
RT: 25.80 min Scan# 3832
Delta R.T. -0.01 min
Lab File: BE090445.D
Acq: 12 Aug 2015 1:37


Tgt Ion	Ratio	Lower	Upper
278	100		
139	17.7	14.2	21.4
279	24.0	20.1	30.1





#37
 Benzo(g,h,i)perylene
 Concen: 1.06 ng
 RT: 26.51 min Scan# 3987
 Delta R.T. -0.01 min
 Lab File: BE090445.D
 Acq: 12 Aug 2015 1:37

Instrument :
 BNA_E
 ClientSampleId :
 SSTDCCC001



Tgt Ion:	276	Resp:	28321
Ion Ratio	Lower	Upper	
276	100		
277	24.4	20.1	30.1
138	23.5	18.1	27.1

Manual Integrations
 APPROVED

MMDadoda
 8/12/2015 3:55:47 PM

