


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE081115\
 Data File : BE090428.D
 Acq On : 11 Aug 2015 15:04
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE080515.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 06 12:28:08 2015

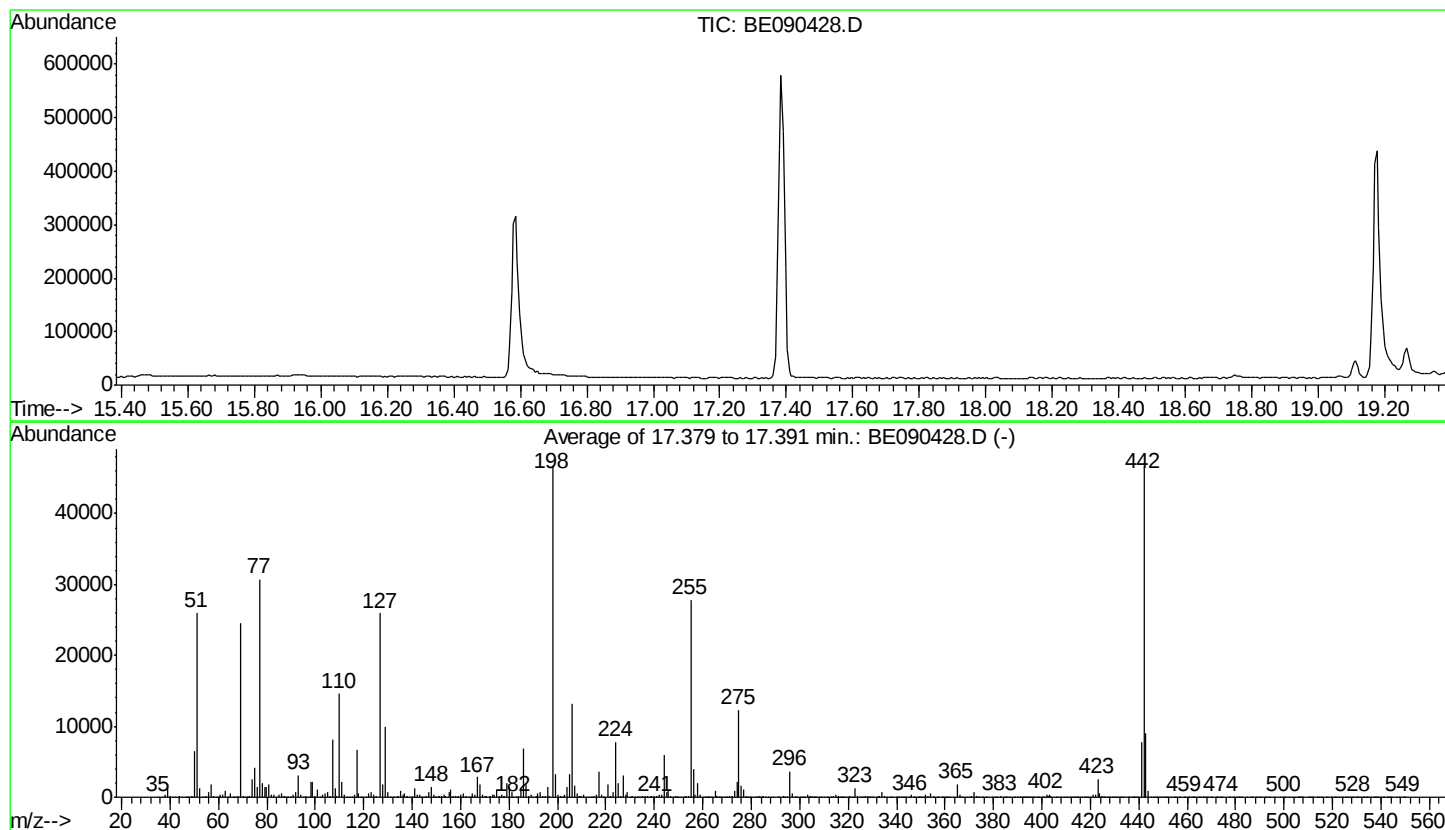

AutoFind: Scans 2517, 2518, 2519; Background Corrected with Scan 2511

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.6	26012	PASS
68	69	0.00	2	1.1	272	PASS
69	198	0.00	100	52.7	24645	PASS
70	69	0.00	2	0.7	181	PASS
127	198	10	80	55.6	25986	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	46769	PASS
199	198	5	9	6.9	3237	PASS
275	198	10	60	26.4	12340	PASS
365	198	1	100	3.9	1808	PASS
441	442	0.01	24	16.7	7786	PASS
442	198	50	100	99.8	46657	PASS
443	442	15	24	19.3	8988	PASS