


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE081115\
Data File : BE090444.D
Acq On : 12 Aug 2015 00:49
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE080515.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Aug 06 12:28:08 2015

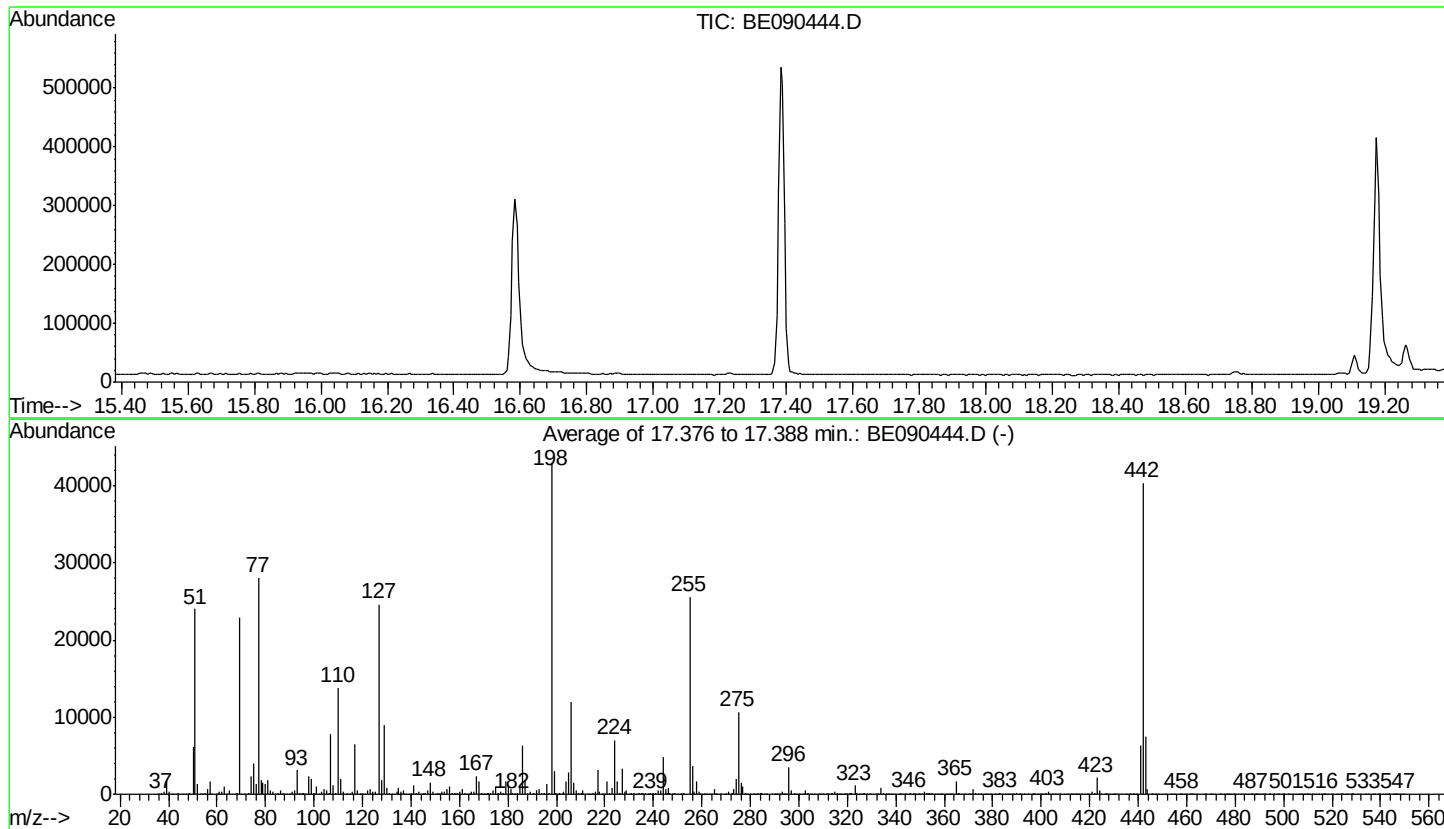

AutoFind: Scans 2517, 2518, 2519; Background Corrected with Scan 2510

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.9	24025	PASS
68	69	0.00	2	0.9	205	PASS
69	198	0.00	100	53.2	22861	PASS
70	69	0.00	2	0.3	79	PASS
127	198	10	80	57.2	24600	PASS
197	198	0.00	2	0.3	139	PASS
198	198	100	100	100.0	42993	PASS
199	198	5	9	6.9	2983	PASS
275	198	10	60	24.8	10666	PASS
365	198	1	100	3.9	1675	PASS
441	442	0.01	24	15.7	6356	PASS
442	198	50	100	94.0	40408	PASS
443	442	15	24	18.4	7422	PASS