


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE081116\
Data File : BE092262.D
Acq On : 11 Aug 2016 12:10
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE080916.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Aug 10 11:12:32 2016

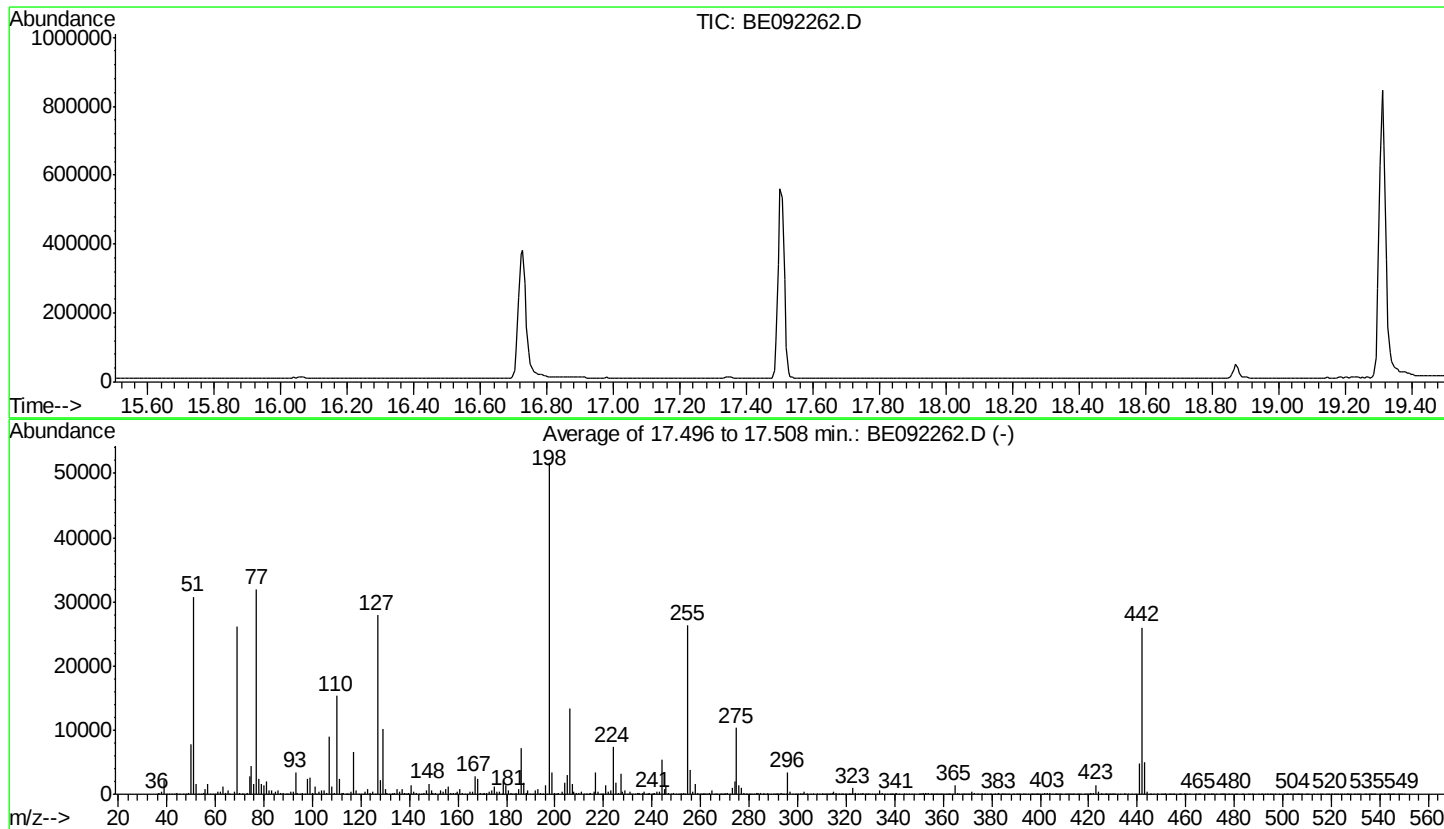

AutoFind: Scans 2537, 2538, 2539; Background Corrected with Scan 2530

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	59.5	30759	PASS
68	69	0.00	2	1.9	504	PASS
69	198	0.00	100	50.5	26130	PASS
70	69	0.00	2	0.5	121	PASS
127	198	10	80	53.9	27889	PASS
197	198	0.00	2	0.1	60	PASS
198	198	100	100	100.0	51698	PASS
199	198	5	9	6.5	3348	PASS
275	198	10	60	19.9	10294	PASS
365	198	1	100	2.6	1334	PASS
441	442	0.01	24	18.3	4771	PASS
442	198	50	100	50.3	26016	PASS
443	442	15	24	19.6	5093	PASS