

Data Path : Z:\HPCHEM1\BNA E\DATA\BE081117\
 Data File : BE093777.D
 Acq On : 11 Aug 2017 19:37
 Operator : SJ/JU
 Sample : PB101387BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SBLK87

Quant Time: Aug 12 02:02:41 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Aug 12 02:01:53 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.92	152	2505	0.40	ng/ul	0.00
2) Naphthalene-d8	10.70	136	13502	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.52	164	8497	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.26
16) Chrysene-d12	21.41	240	17083	0.40	ng/ul	0.00
20) Perylene-d12	23.76	264	1255430	0.40	ng/ul	-0.15
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.29	152	6283	0.29	ng/ul	0.00
14) Fluoranthene-d10	19.27	212	15039	0.00	ng/ul	0.00
Target Compounds						
9) Fluorene	15.51	166	1882	0.053	ng/ul#	20
17) Pyrene	19.64	202	2002	0.040	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE081117\
Data File : BE093777.D
Acq On : 11 Aug 2017 19:37
Operator : SJ/JU
Sample : PB101387BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK87

Quant Time: Aug 12 02:02:41 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 12 02:01:53 2017
Response via : Initial Calibration

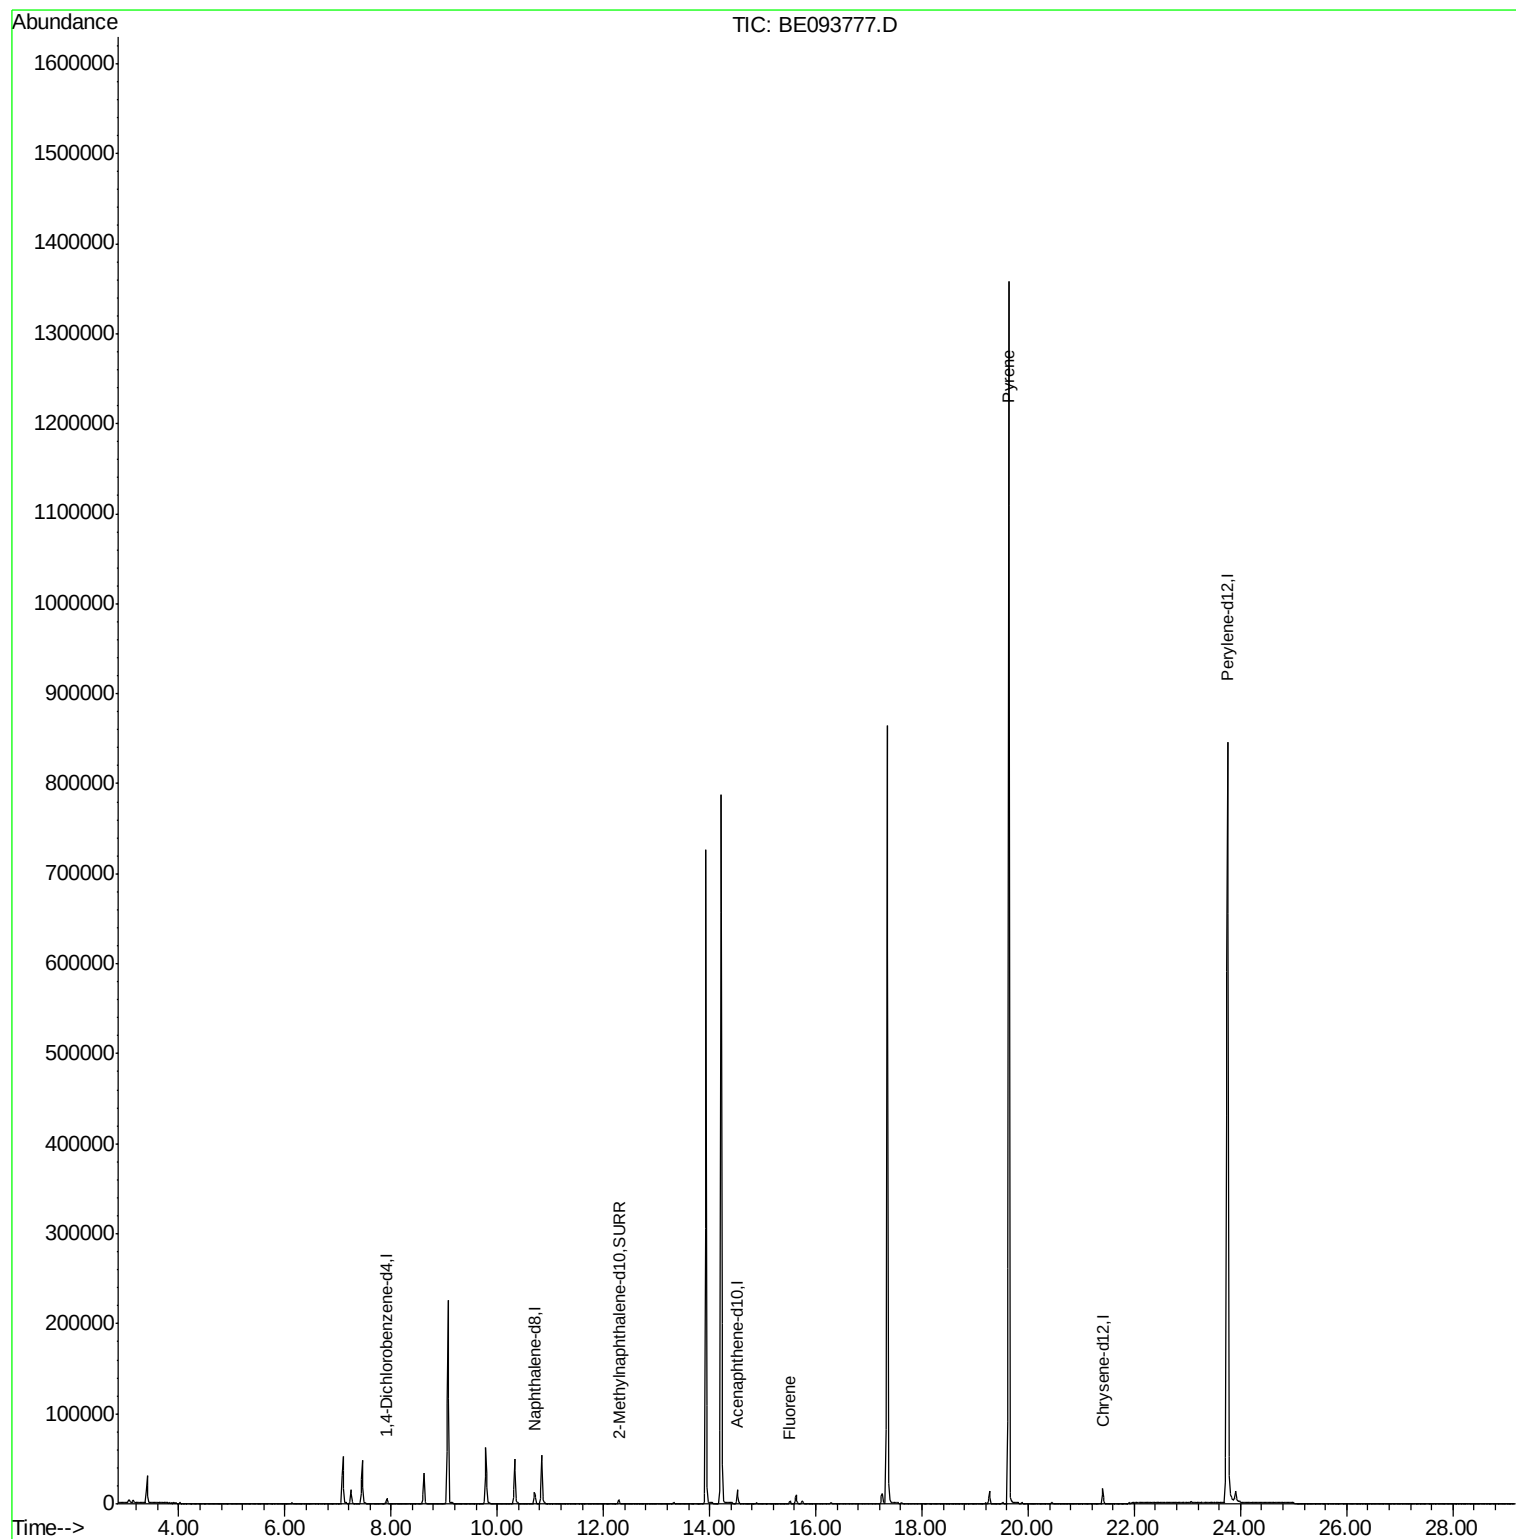

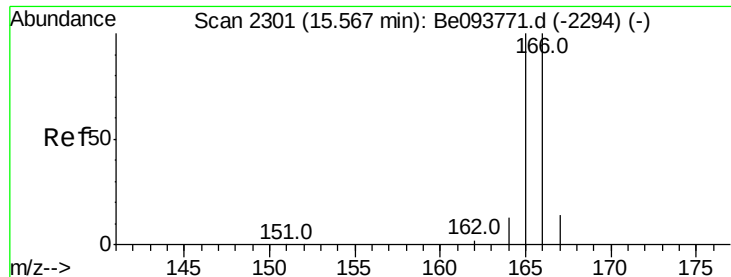

#9

Fluorene

Concen: 0.053 ng/ul

RT: 15.51 min Scan# 2292

Delta R.T. -0.05 min

Lab File: BE093777.D

Acq: 11 Aug 2017 19:37

Instrument :

BNA_E

ClientSampleId :

SBLK87


Tot Ion:166 Resp: 1882

Ion Ratio Lower Upper

166 100

165 7.5 73.4 110.2#


167 34.6 14.6 22.0#

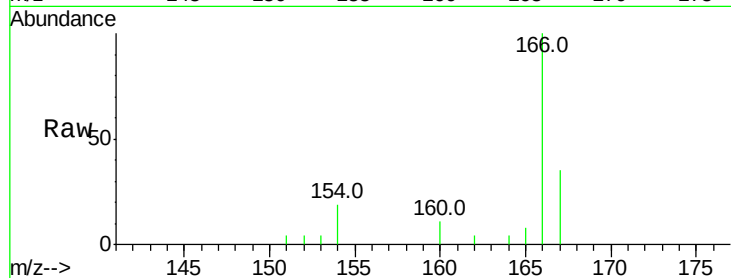



Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

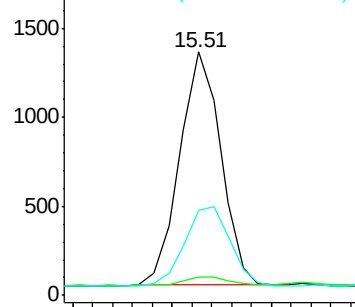

Time--> 15.45 15.50 15.55

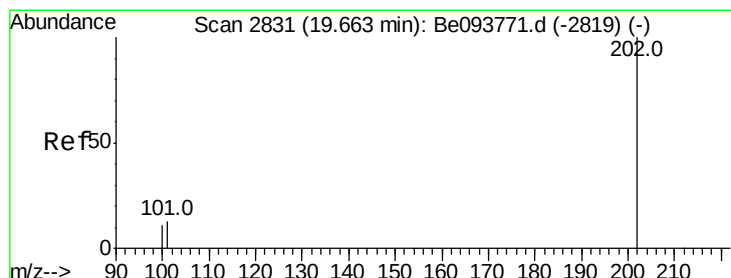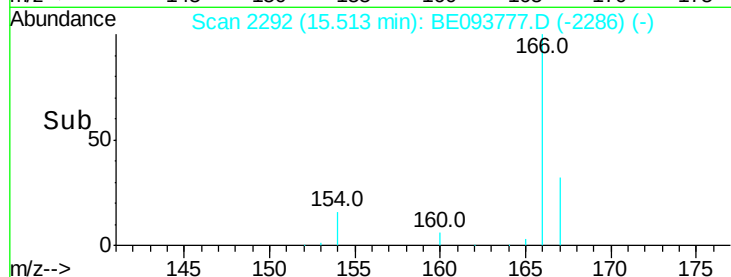

#17

Pyrene

Concen: 0.040 ng/ul

RT: 19.64 min Scan# 2824

Delta R.T. -0.03 min

Lab File: BE093777.D

Acq: 11 Aug 2017 19:37


Tgt Ion:202 Resp: 2002

Ion Ratio Lower Upper

202 100

101 181.2 18.2 27.4#


100 998.8 15.6 23.4#

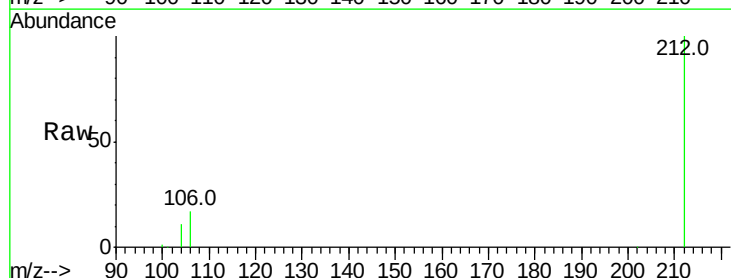

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): BE

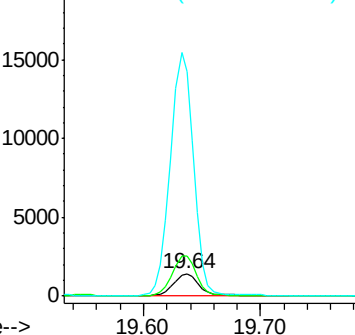

Time--> 19.60 19.65 19.70

