


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE081215\
 Data File : BE090461.D
 Acq On : 12 Aug 2015 11:15
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE080515.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 06 12:28:08 2015

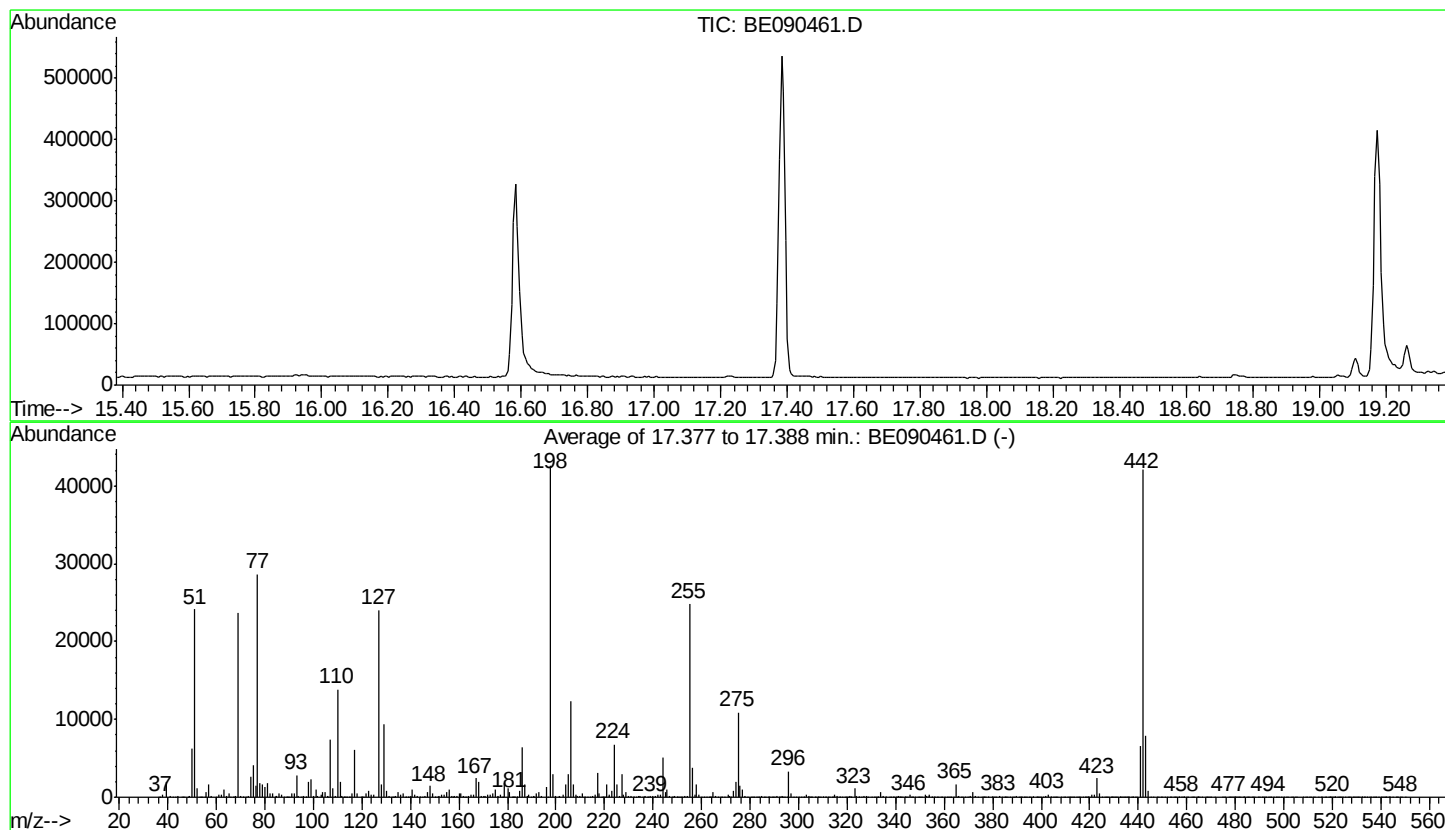

AutoFind: Scans 2517, 2518, 2519; Background Corrected with Scan 2508

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	56.7	24163	PASS
68	69	0.00	2	0.9	221	PASS
69	198	0.00	100	55.4	23600	PASS
70	69	0.00	2	0.8	181	PASS
127	198	10	80	56.4	24005	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	42581	PASS
199	198	5	9	6.9	2957	PASS
275	198	10	60	25.6	10903	PASS
365	198	1	100	3.9	1655	PASS
441	442	0.01	24	15.7	6617	PASS
442	198	50	100	98.7	42019	PASS
443	442	15	24	18.8	7913	PASS