


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE081215\
 Data File : BE090479.D
 Acq On : 12 Aug 2015 22:21
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE080515.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 06 12:28:08 2015

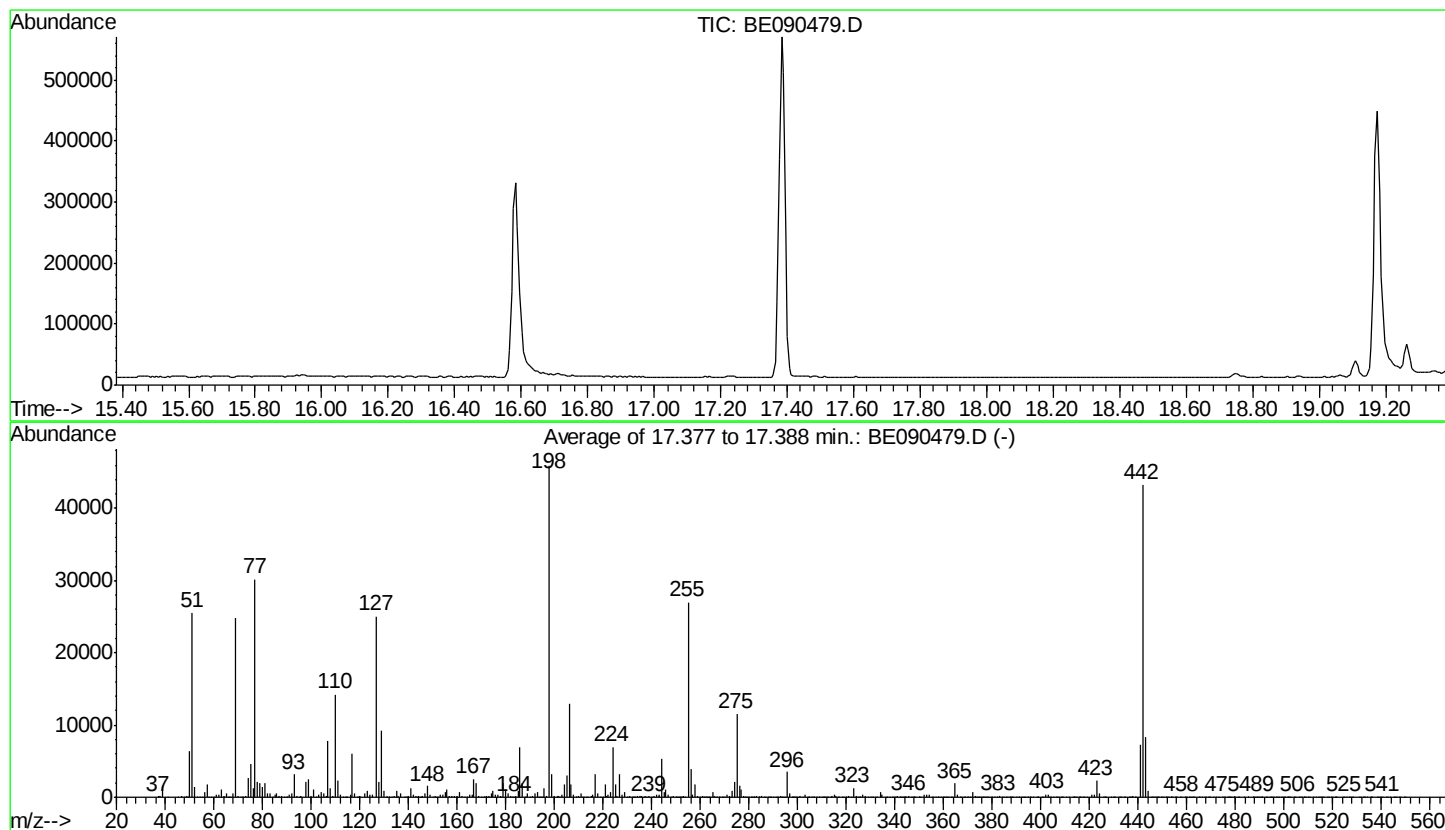

AutoFind: Scans 2517, 2518, 2519; Background Corrected with Scan 2510

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.6	25539	PASS
68	69	0.00	2	1.8	455	PASS
69	198	0.00	100	54.2	24872	PASS
70	69	0.00	2	0.5	131	PASS
127	198	10	80	54.6	25074	PASS
197	198	0.00	2	0.3	122	PASS
198	198	100	100	100.0	45918	PASS
199	198	5	9	7.0	3226	PASS
275	198	10	60	25.1	11543	PASS
365	198	1	100	4.1	1899	PASS
441	442	0.01	24	17.0	7336	PASS
442	198	50	100	94.2	43252	PASS
443	442	15	24	19.3	8361	PASS