


Data Path : Z:\HPCHEM1\BNA E\DATA\BE081415\
 Data File : BE090513.D
 Acq On : 14 Aug 2015 9:22
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE081415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 14 16:52:42 2015

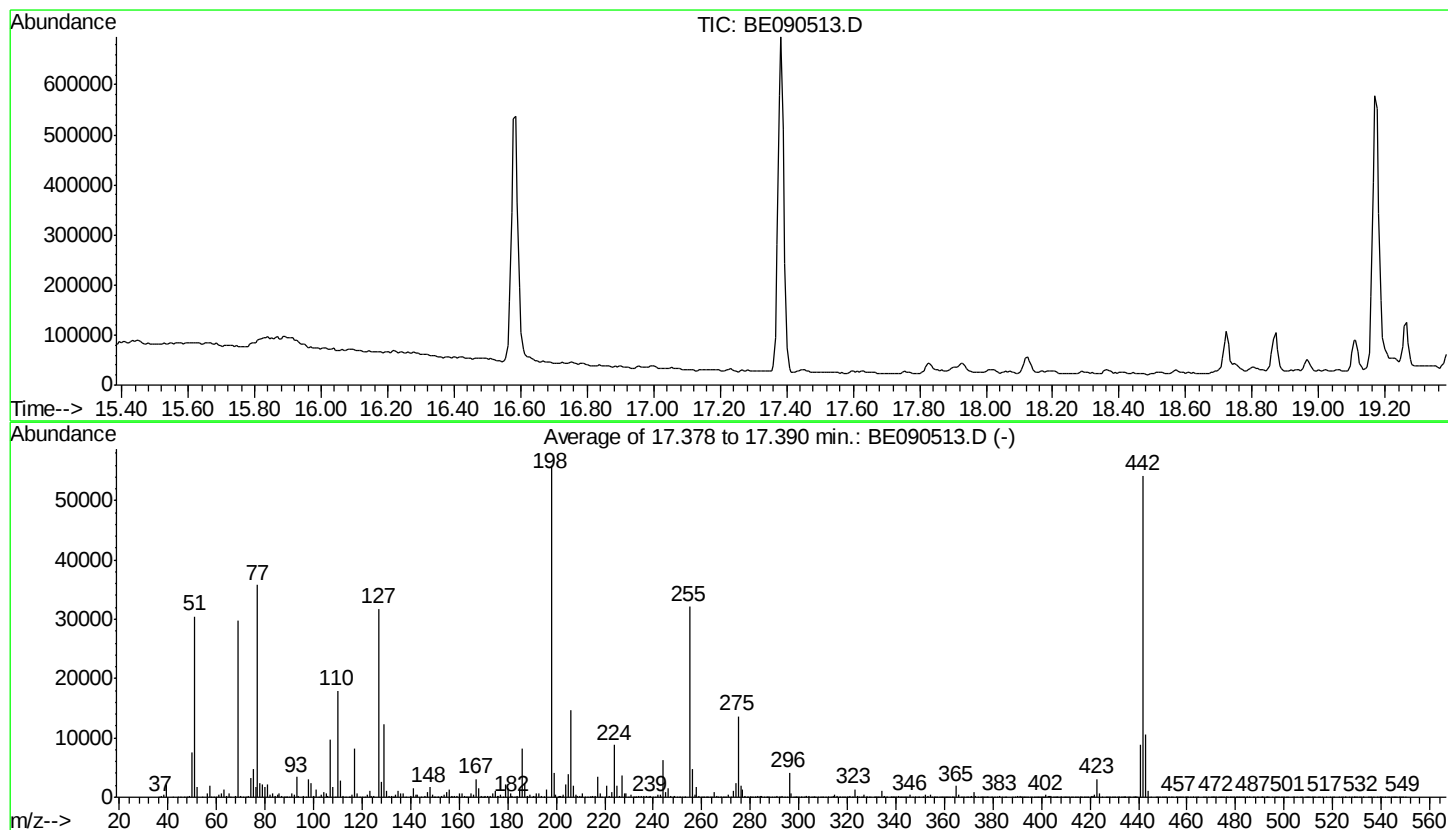

AutoFind: Scans 2517, 2518, 2519; Background Corrected with Scan 2511

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.4	30440	PASS
68	69	0.00	2	0.9	267	PASS
69	198	0.00	100	53.4	29863	PASS
70	69	0.00	2	0.8	242	PASS
127	198	10	80	56.9	31786	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	55906	PASS
199	198	5	9	7.3	4059	PASS
275	198	10	60	24.4	13618	PASS
365	198	1	100	3.4	1898	PASS
441	442	0.01	24	16.2	8785	PASS
442	198	50	100	97.0	54221	PASS
443	442	15	24	19.7	10663	PASS