


```
Data Path : Z:\HPCHEM1\BNA E\Data\BE081417\  
Data File : BE093797.D  
Acq On    : 14 Aug 2017 21:21  
Operator   : SJ/JU  
Sample     : I4529-11  
Misc      :  
ALS Vial   : 15 Sample Multiplier: 1
```

Instrument :
BNA_E
ClientSampleId :
C0AA5

Manual Integrations

Sohil
8/21/2017 1:43:32 PM

Quant Time: Aug 15 19:19:06 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 15 10:51:12 2017
Response via : Initial Calibration

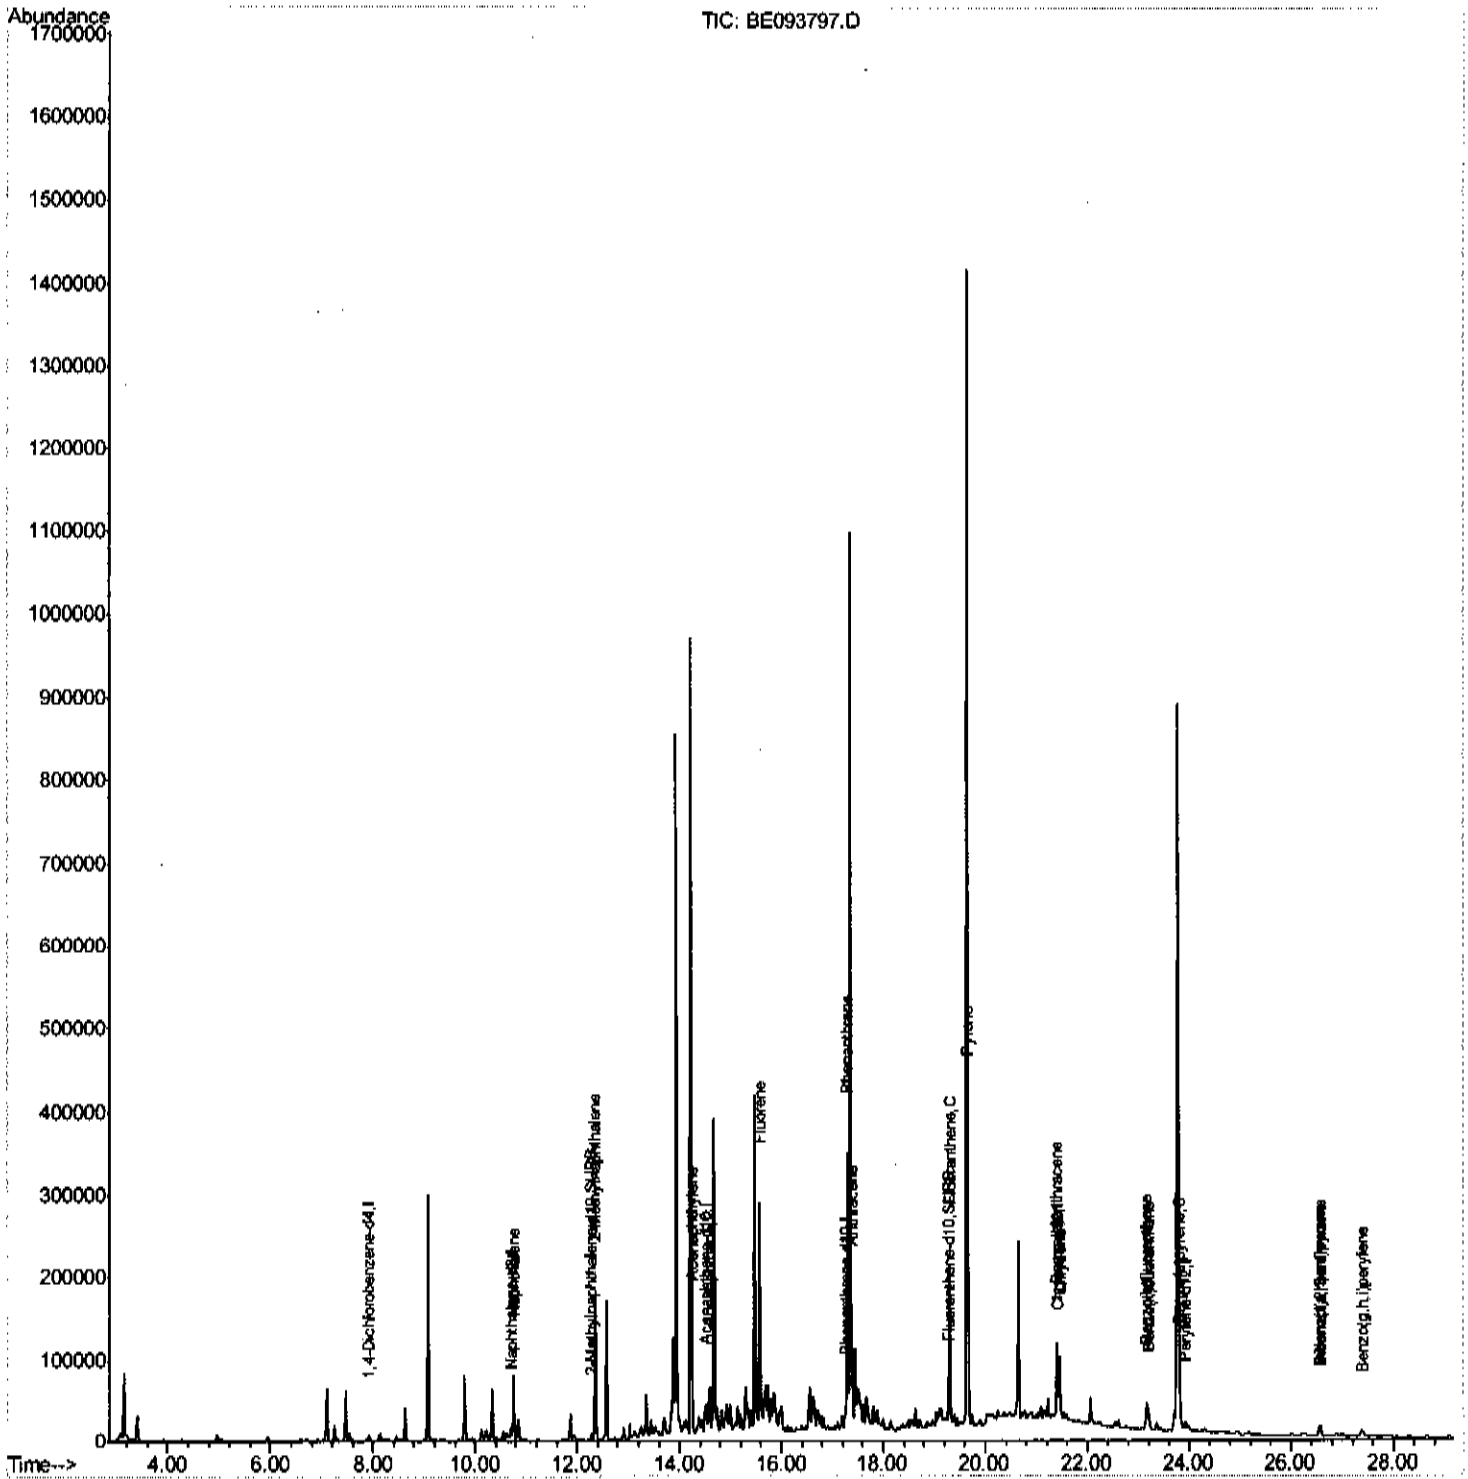

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\Data\BE081417\
Data File : BE093797.D
Acq On : 14 Aug 2017 21:21
Operator : SJ/JU
Sample : I4529-11
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AA5

Manual Integrations
APPROVED

Sohil
8/21/2017 1:43:32 PM

Quant Time: Aug 18 08:29:50 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 17 19:06:13 2017
Response via : Initial Calibration

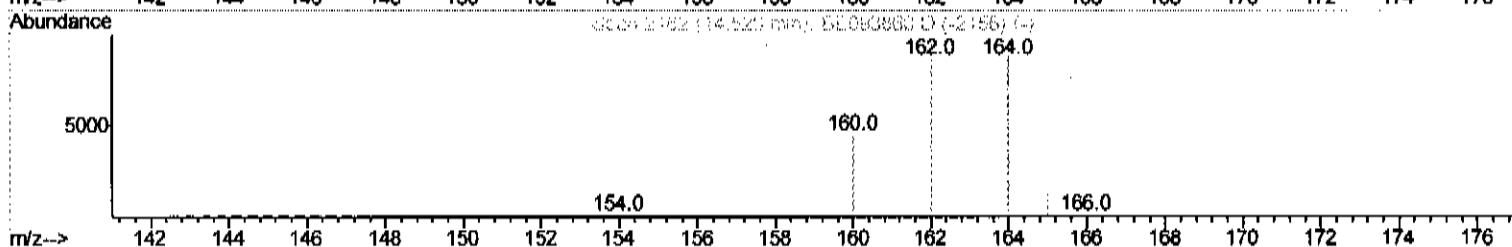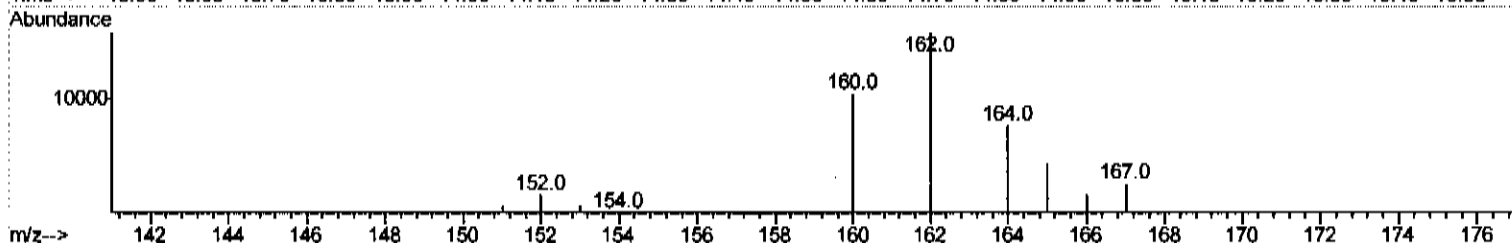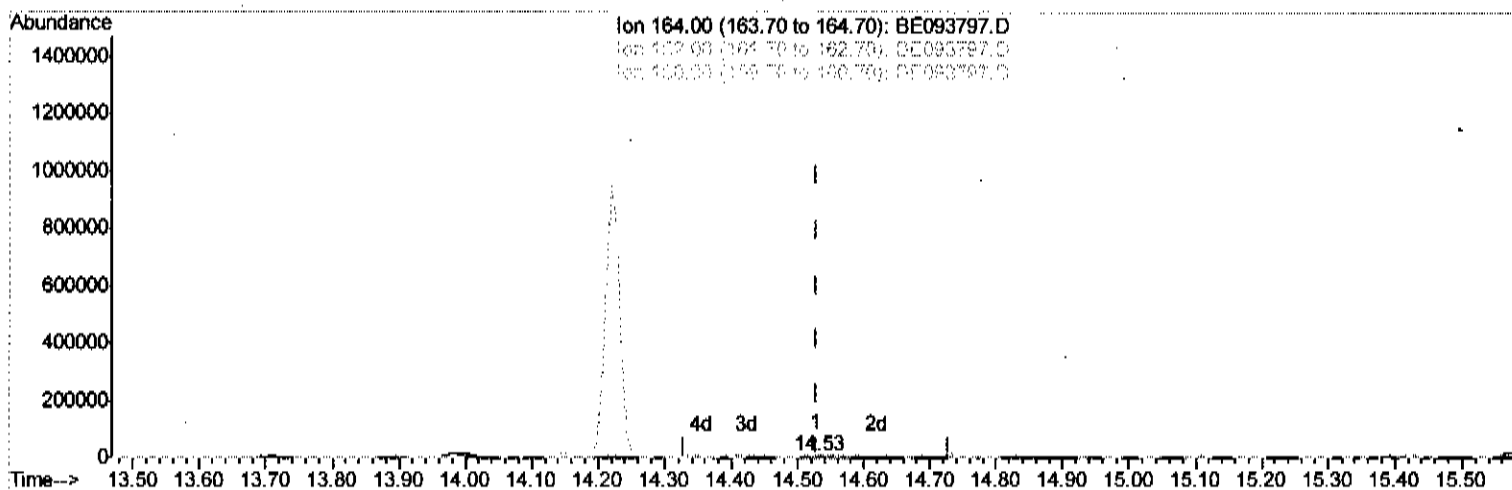

TIC: BE093797.D

(6) Acenaphthene-d10 (I)

14.529min (-0.000) 0.40ng/ul

response 13515

Ion	Exp%	Act%
164.00	100	100
162.00	98.60	202.31#
160.00	48.80	134.29#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\Data\BE081417\
 Data File : BE093797.D
 Acq On : 14 Aug 2017 21:21
 Operator : SJ/JU
 Sample : I4529-11
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 C0AA5

Manual Integrations
 APPROVED

Sohil
 8/21/2017 1:43:32 PM

Quant Time: Aug 15 19:19:06 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 15 10:51:12 2017
 Response via : Initial Calibration

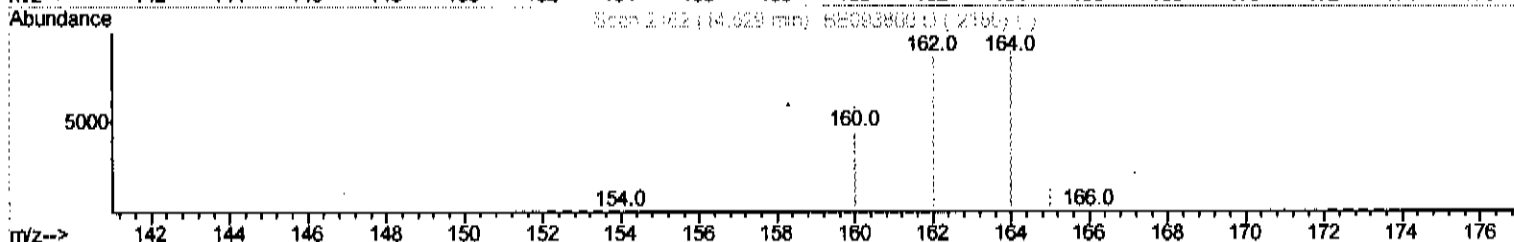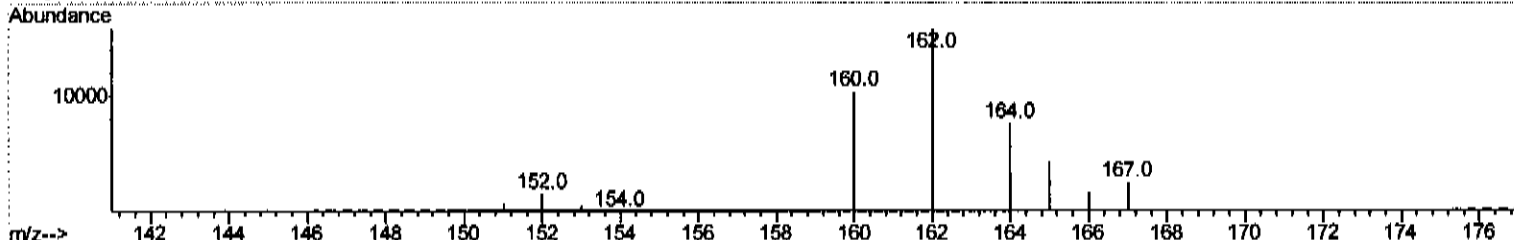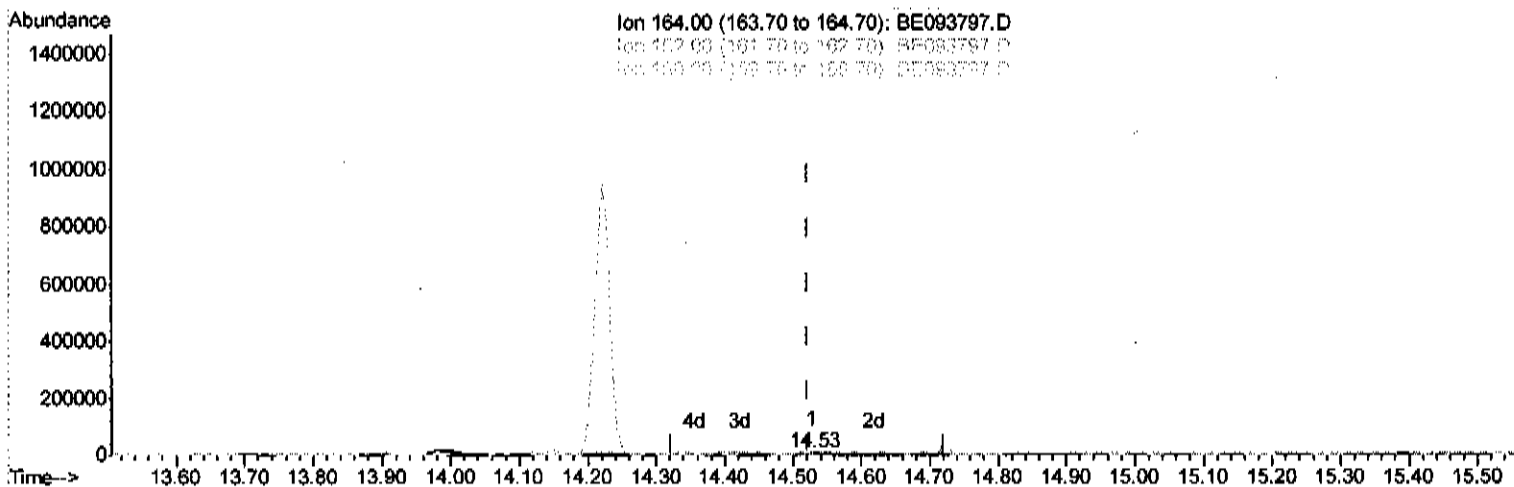

TIC: BE093797.D

(6) Acenaphthene-d10 (I)

14.529min (+0.007) 0.40ng/ul m

response 10738

Ion	Exp%	Act%
164.00	100	100
162.00	98.60	202.31#
160.00	48.80	134.29#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\Data\BE081417\
 Data File : BE093797.D
 Acq On : 14 Aug 2017 21:21
 Operator : SJ/JU
 Sample : I4529-11
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AA5

Manual Integrations
 APPROVED

Sohil
 8/21/2017 1:43:32 PM

Quant Time: Aug 18 08:29:50 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 17 19:06:13 2017
 Response via : Initial Calibration

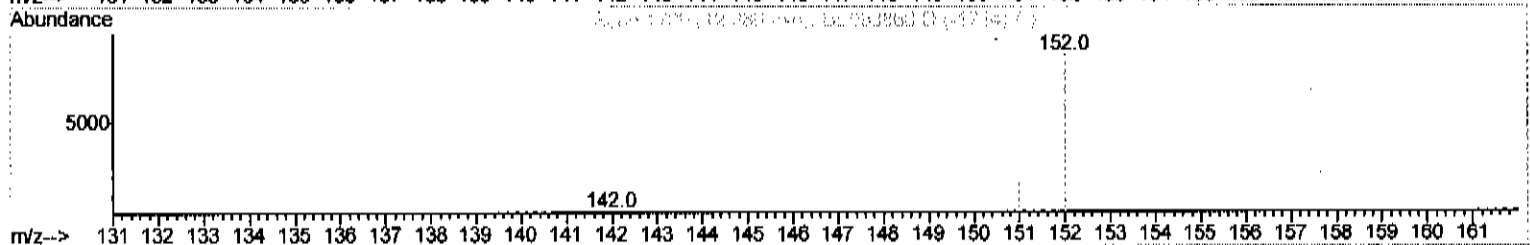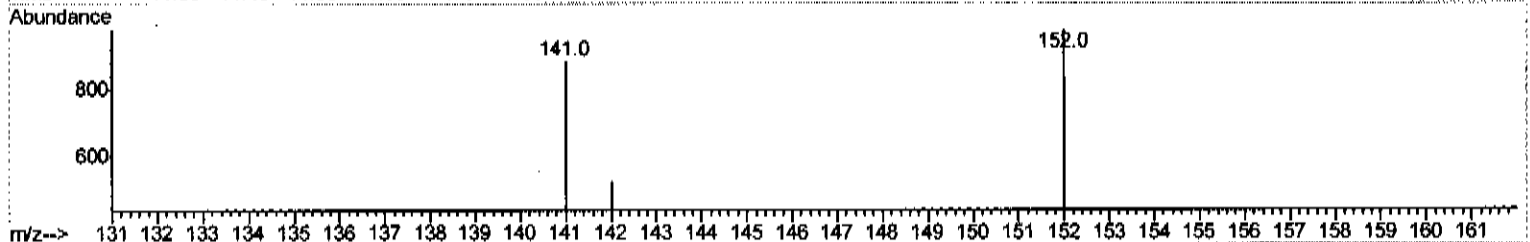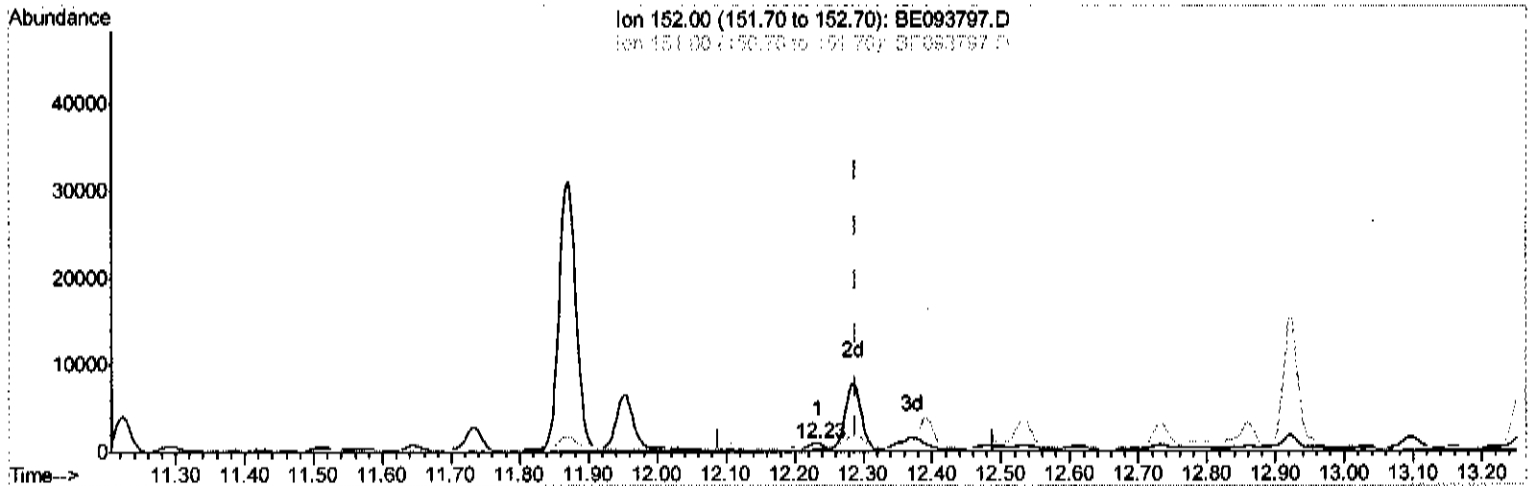

TIC: BE093797.D

(4) 2-Methylnaphthalene-d10 (SURR)

12.234min (-0.055) 0.05ng/ul

response 1141

Ion	Exp%	Act%
152.00	100	100
151.00	19.30	21.65
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\Data\BE081417\
 Data File : BE093797.D
 Acq On : 14 Aug 2017 21:21
 Operator : SJ/JU
 Sample : I4529-11
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 C0AA5

Manual Integrations
 APPROVED

Sohil
 8/21/2017 1:43:32 PM

Quant Time: Aug 15 19:19:06 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 15 10:51:12 2017
 Response via : Initial Calibration

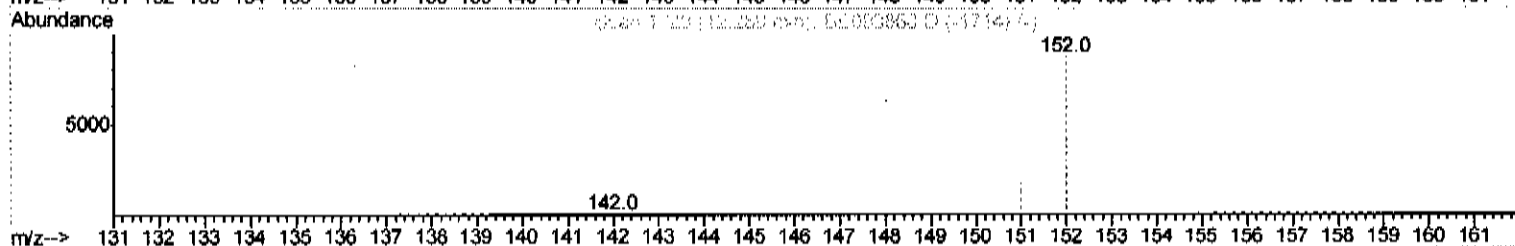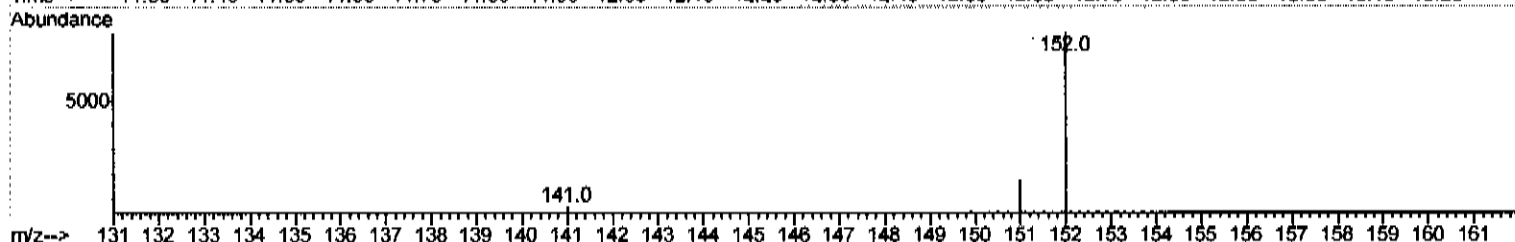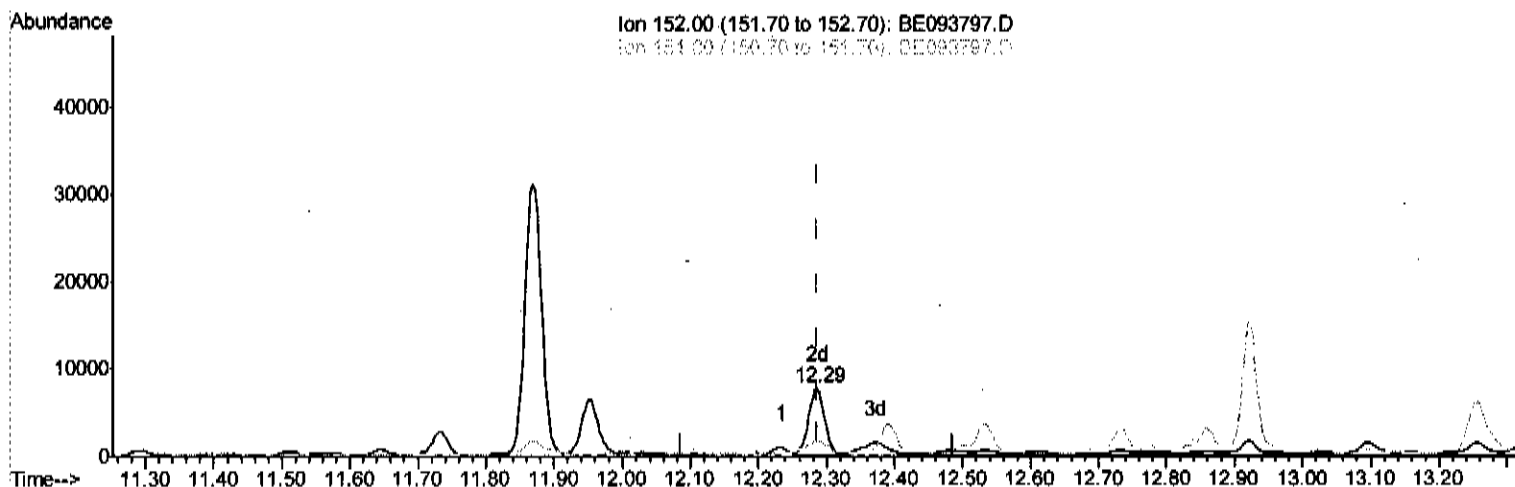

TIC: BE093797.D

(4) 2-Methylnaphthalene-d10 (SURR)

12.286min (-0.000) 0.48ng/ul m

response 12175

Ion	Exp%	Act%
152.00	100	100
151.00	19.30	2.03#
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\Data\BE081417\
 Data File : BE093797.D
 Acq On : 14 Aug 2017 21:21
 Operator : SJ/JU
 Sample : I4529-11
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AA5

Manual Integrations
 APPROVED

Sohil
 8/21/2017 1:43:32 PM

Quant Time: Aug 18 08:29:50 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 17 19:06:13 2017
 Response via : Initial Calibration

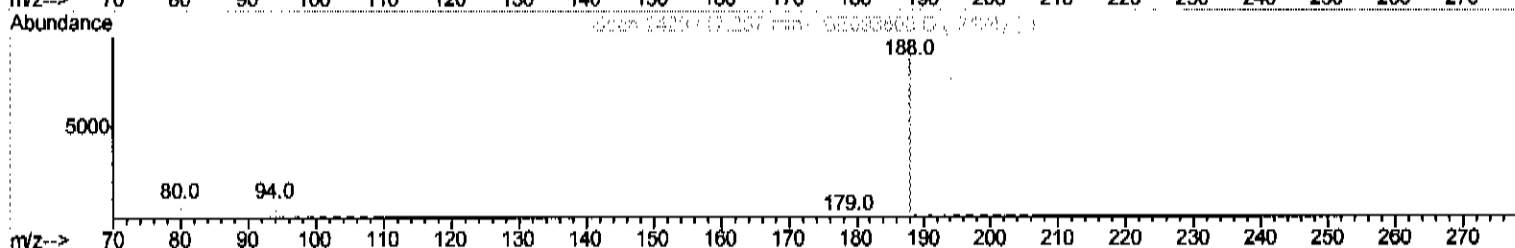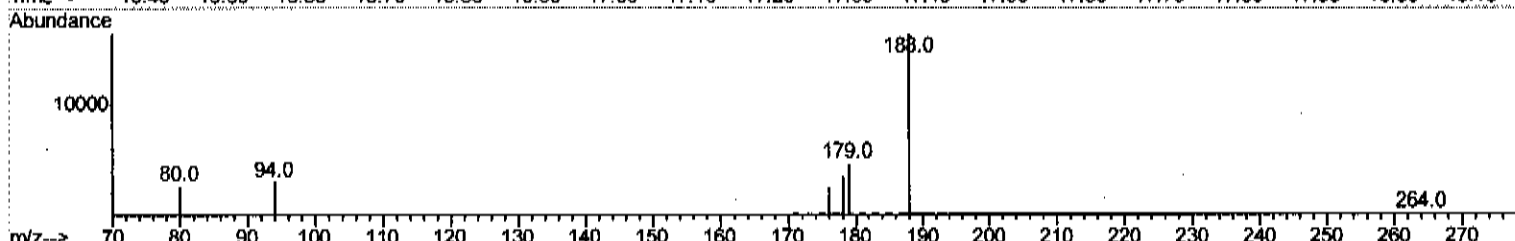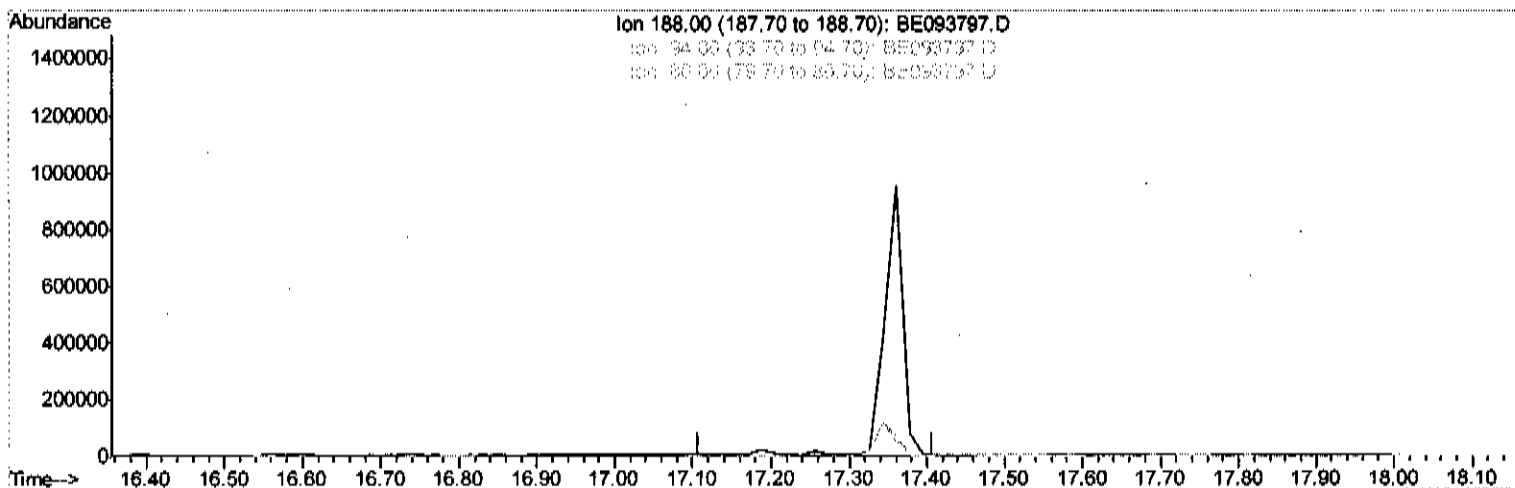

TIC: BE093797.D

(10) Phenanthrene-d10 (I)

17.257min (-17.257) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.00	0.00#
80.00	11.80	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\Data\BE081417\
 Data File : BE093797.D
 Acq On : 14 Aug 2017 21:21
 Operator : SJ/JU
 Sample : I4529-11
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AA5

Manual Integrations
 APPROVED

Sohil
 8/21/2017 1:43:32 PM

Quant Time: Aug 15 19:19:06 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 15 10:51:12 2017
 Response via : Initial Calibration

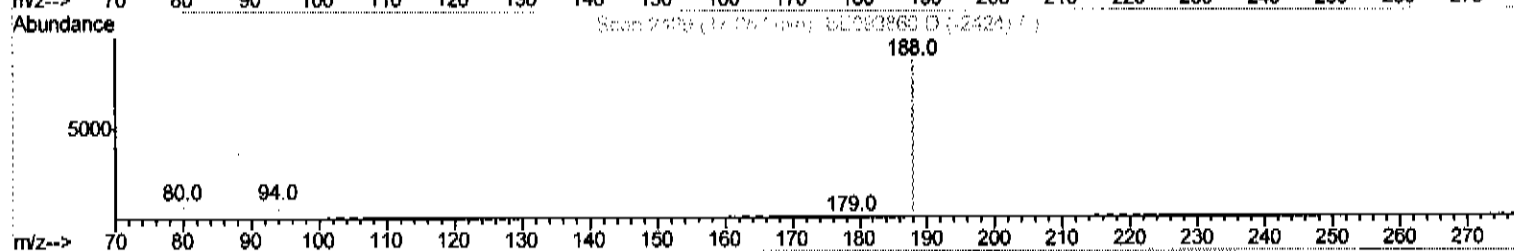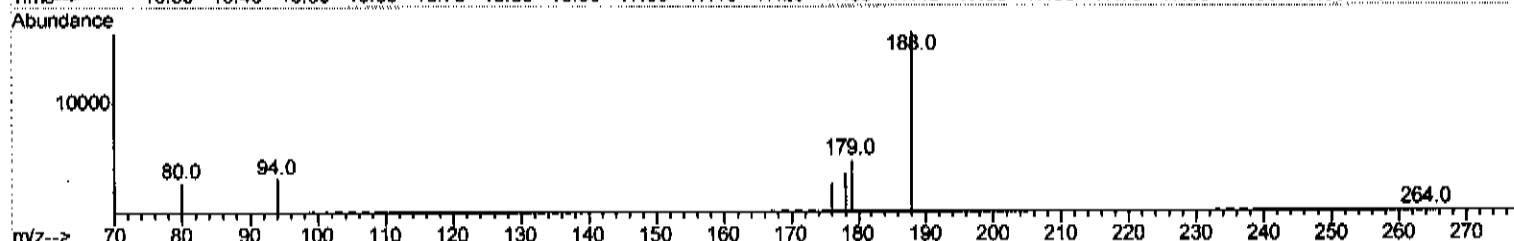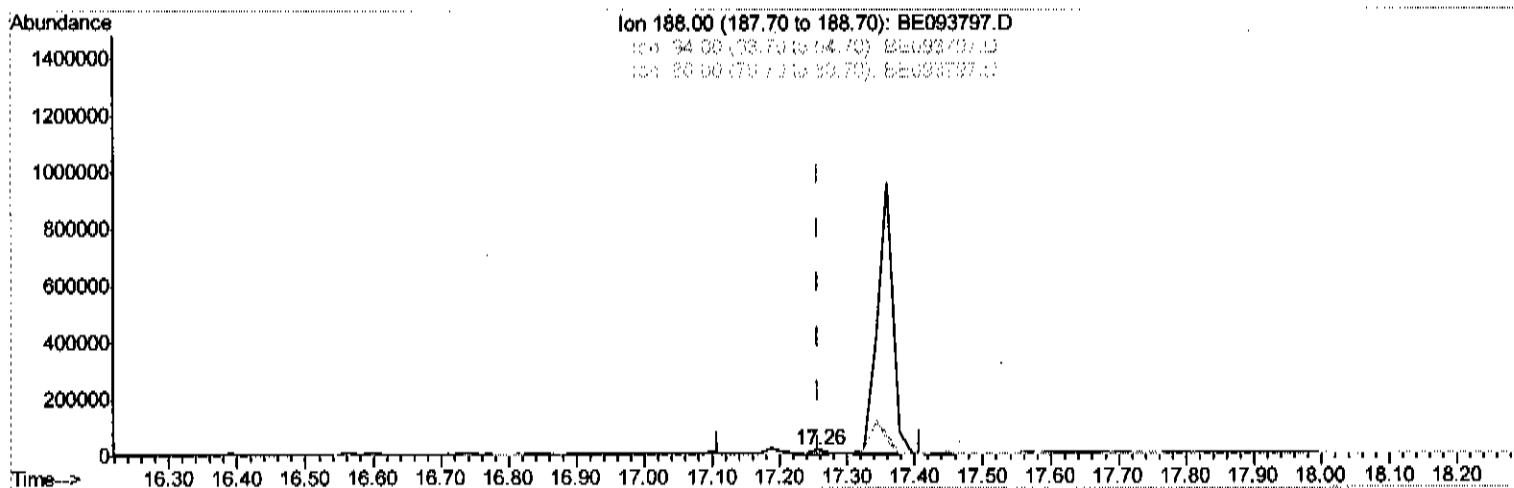

TIC: BE093797.D

(10) Phenanthrene-d10 (I)

17.256min (-0.001) 0.40ng/ul m *plus 8/18/17*

response 22290

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	18.68#
80.00	11.80	16.45#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\Data\BE081417\
Data File : BE093797.D
Acq On : 14 Aug 2017 21:21
Operator : SJ/JU
Sample : I4529-11
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
C0AA5

Manual Integrations
APPROVED

Sohil
8/21/2017 1:43:32 PM

Quant Time: Aug 18 08:29:50 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 17 19:06:13 2017
Response via : Initial Calibration

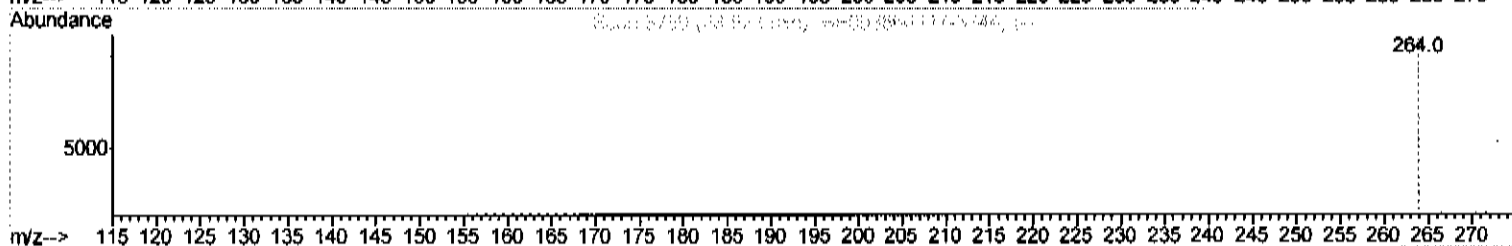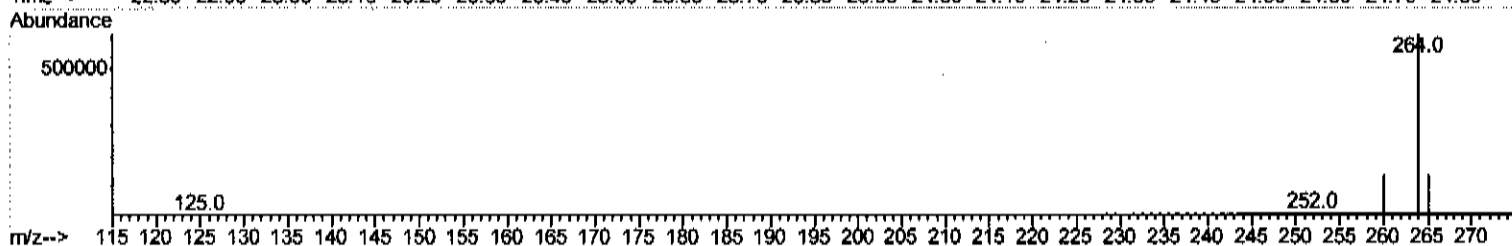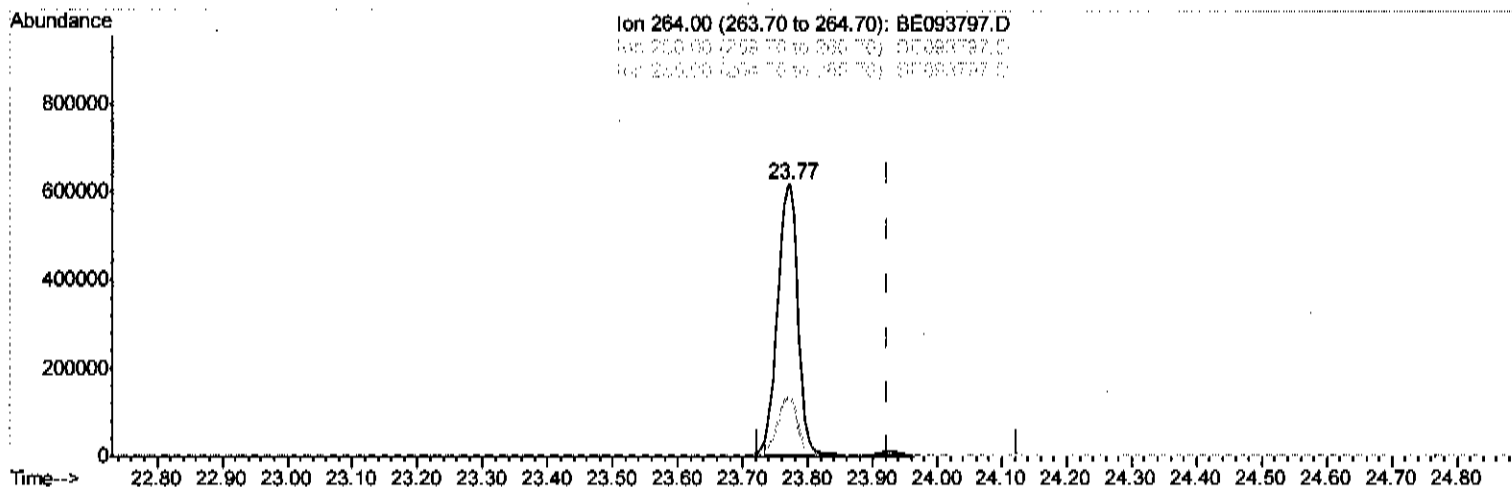

TIC: BE093797.D

(20) Perylene-d12 (I)

23.774min (-0.149) 0.40ng/ul

response 1325290

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.55#
265.00	103.50	21.77#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\Data\BE081417\
 Data File : BE093797.D
 Acq On : 14 Aug 2017 21:21
 Operator : SJ/JU
 Sample : I4529-11
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AA5

Manual Integrations
 APPROVED

Sohil
 8/21/2017 1:43:32 PM

Quant Time: Aug 15 19:19:06 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 15 10:51:12 2017
 Response via : Initial Calibration

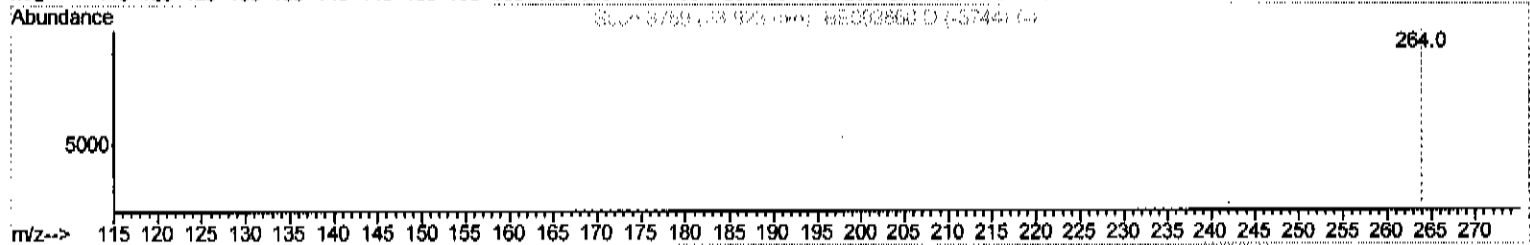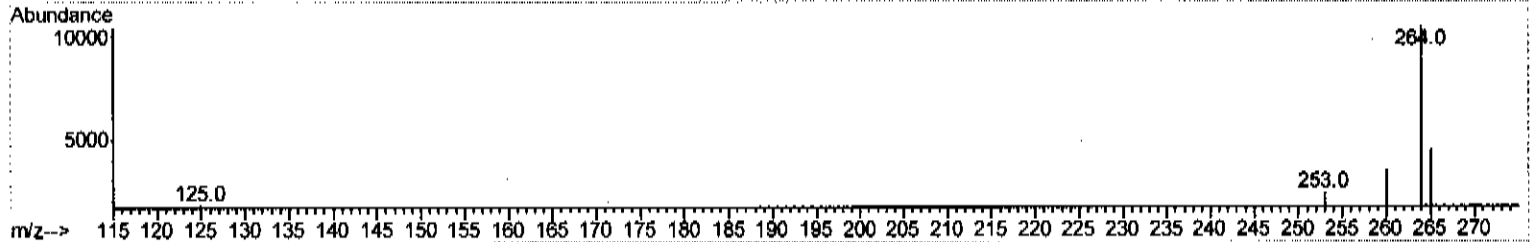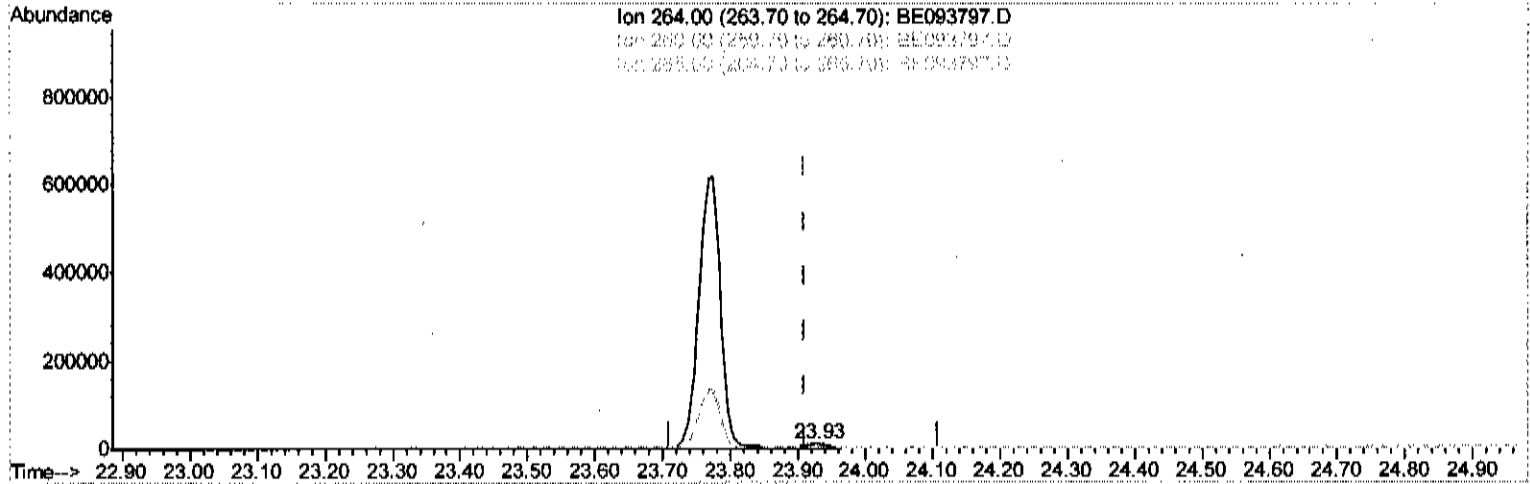

TIC: BE093797.D

(20) Perylene-d12 (I)

23.929min (+0.019) 0.40ng/ul m *SJ*

response 16340

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	33.00
265.00	103.50	42.62*
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\Data\BE081417\
Data File : BE093797.D
Acq On : 14 Aug 2017 21:21
Operator : SJ/JU
Sample : I4529-11
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AA5

Manual Integrations
APPROVED

Sohil
8/21/2017 1:43:32 PM

Quant Time: Aug 18 08:29:50 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 17 19:06:13 2017
Response via : Initial Calibration

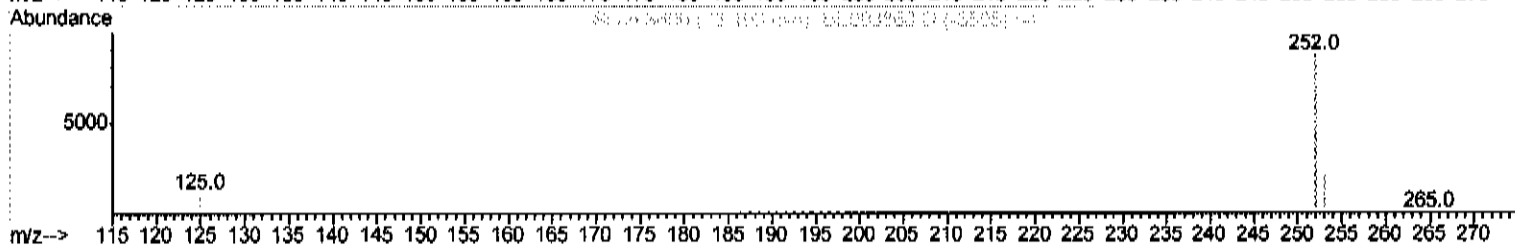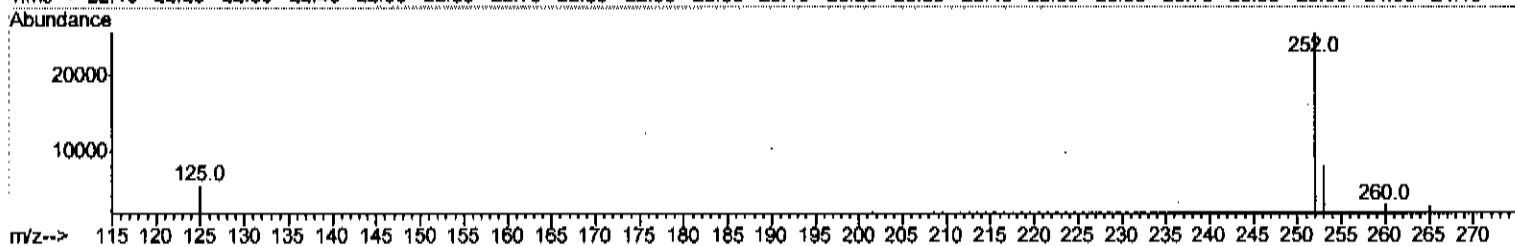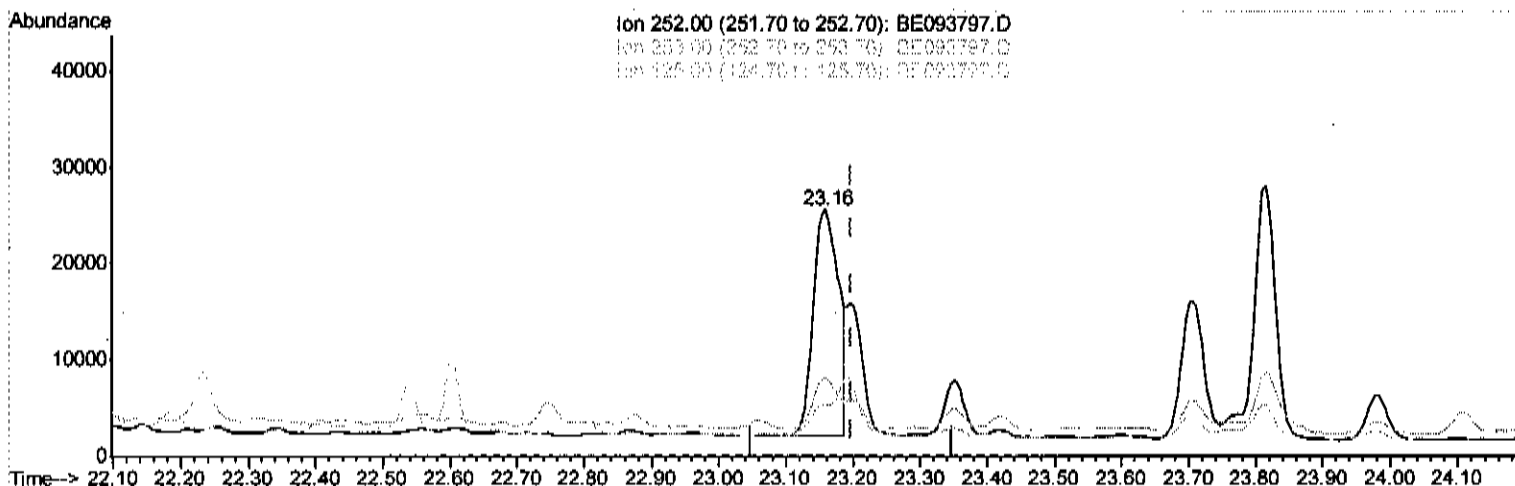

TIC: BE093797.D

(22) Benzo(k)fluoranthene

23.159min (-0.040) 0.02ng/ul

response 61462

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	31.62
125.00	17.10	21.04#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\Data\BE081417\
Data File : BE093797.D
Acq On : 14 Aug 2017 21:21
Operator : SJ/JU
Sample : I4529-11
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AA5

Manual Integrations
APPROVED

Sohil
8/21/2017 1:43:32 PM

Quant Time: Aug 15 19:19:06 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 15 10:51:12 2017
Response via : Initial Calibration

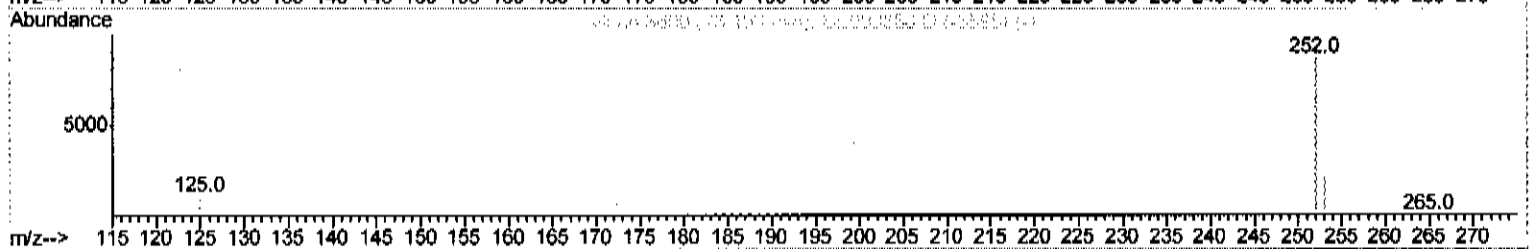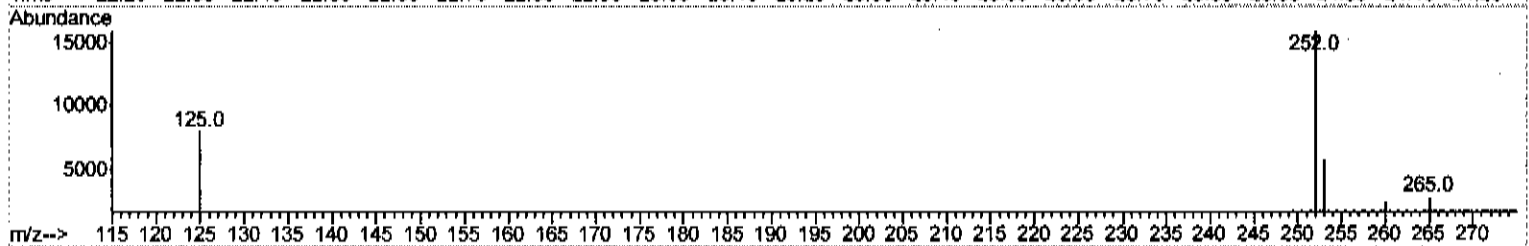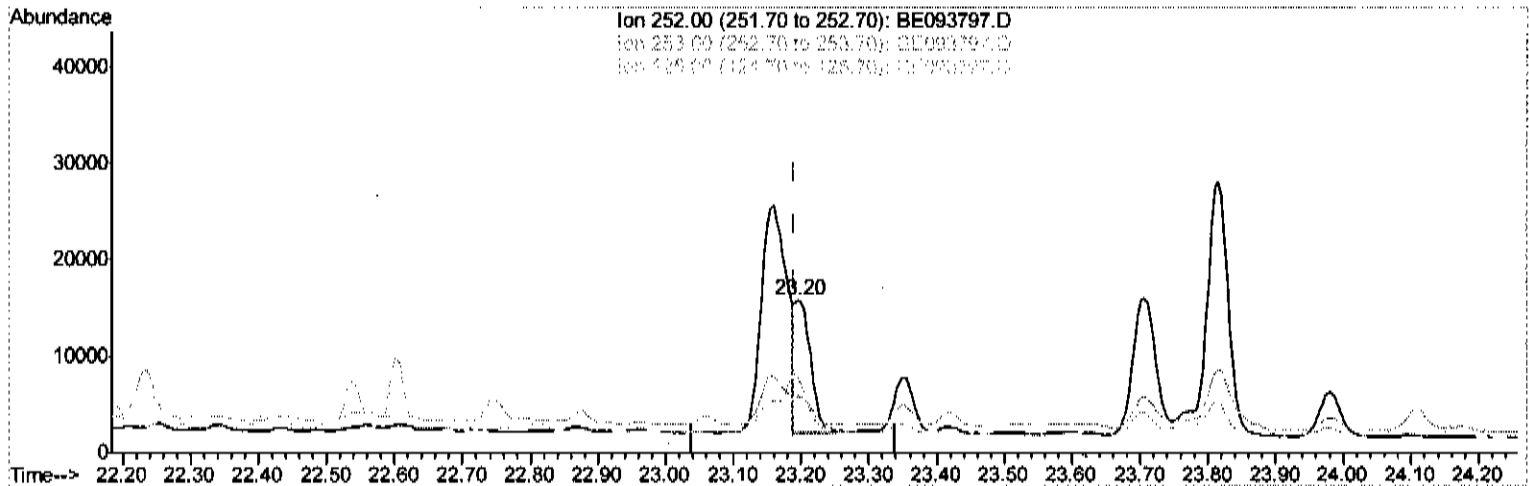

TIC: BE093797.D

(22) Benzo(k)fluoranthene

23.195min (+0.006) 0.46ng/ul m

response 23040

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	37.14#
125.00	17.10	50.45#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\Data\BE081417\
Data File : BE093797.D
Acq On : 14 Aug 2017 21:21
Operator : SJ/JU
Sample : I4529-11
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AA5

Manual Integrations
APPROVED

Sohil
8/21/2017 1:43:32 PM

Quant Time: Aug 18 08:29:50 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 17 19:06:13 2017
Response via : Initial Calibration

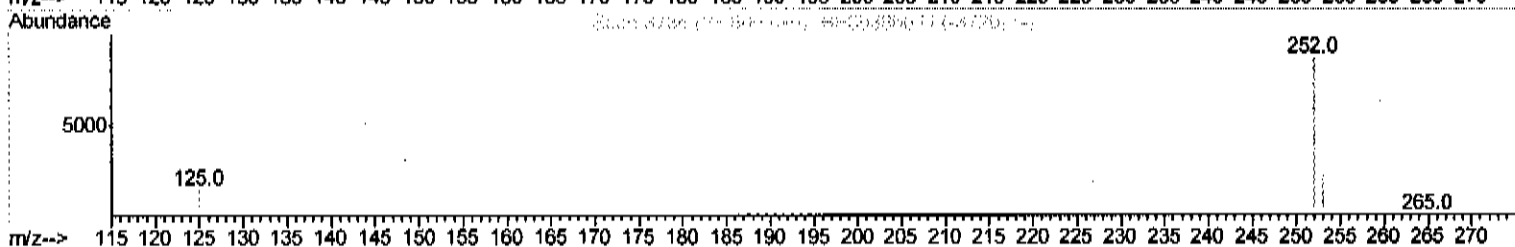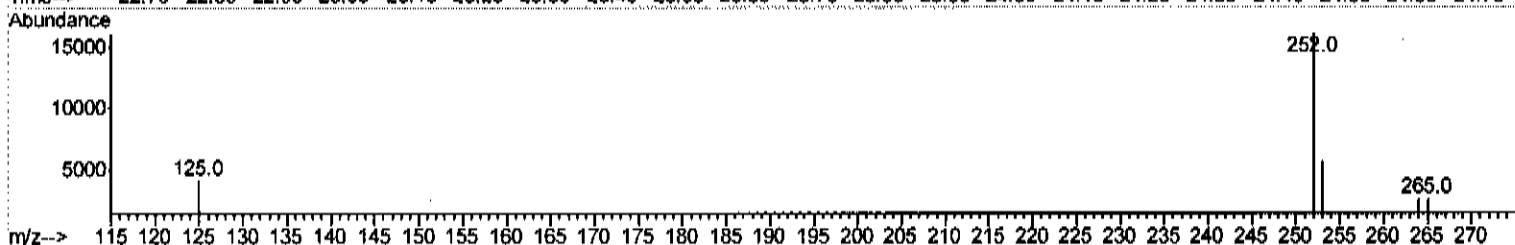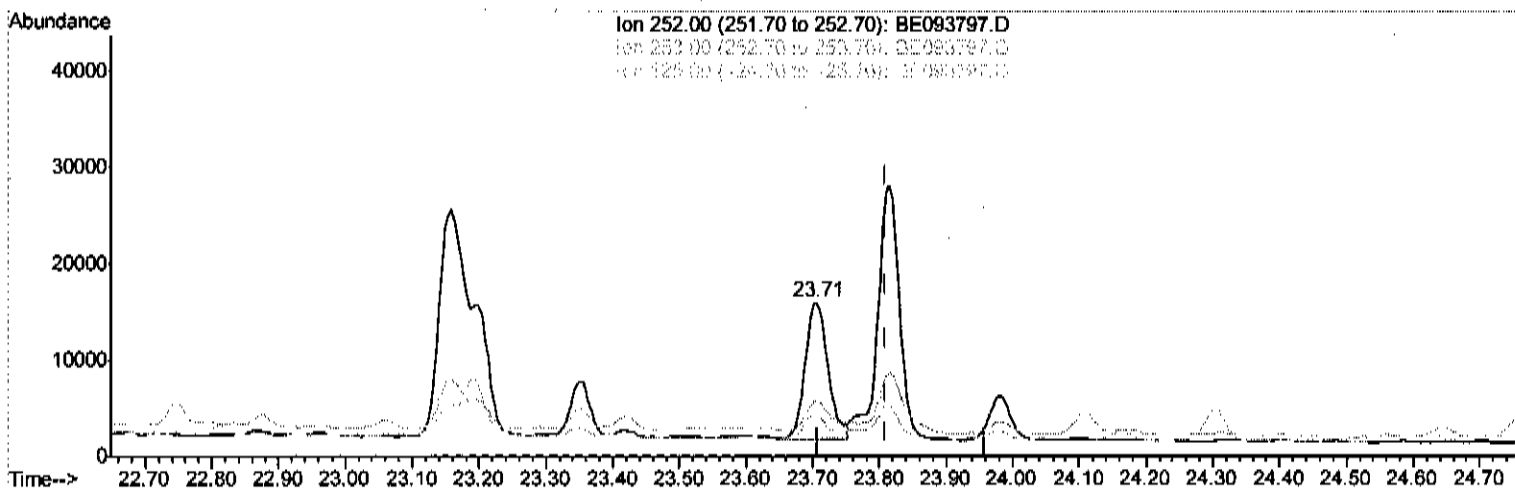

TIC: BE093797.D

(23) Benzo(a)pyrene (C)

23.705min (-0.104) 0.01ng/ul

response 34080

Ion	Exp%	Act%
252.00	100	100
253.00	35.60	35.66
125.00	22.60	26.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\Data\BE081417\
Data File : BE093797.D
Acq On : 14 Aug 2017 21:21
Operator : SJ/JU
Sample : I4529-11
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
C0AA5

Manual Integrations
APPROVED

Sohil
8/21/2017 1:43:32 PM

Quant Time: Aug 15 19:19:06 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 15 10:51:12 2017
Response via : Initial Calibration

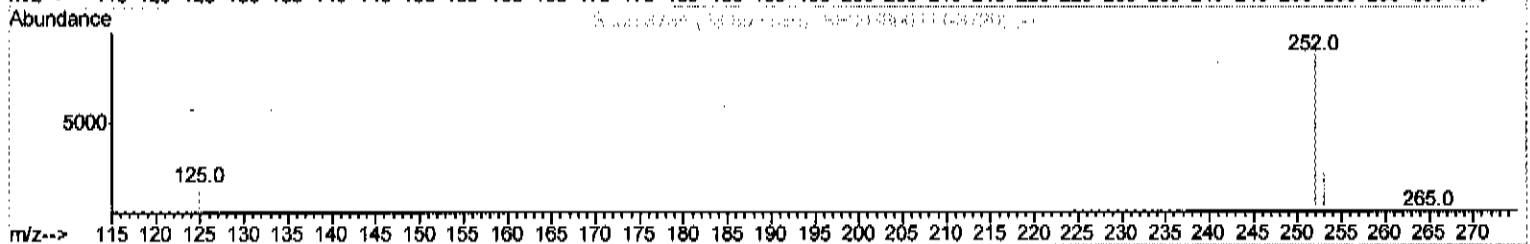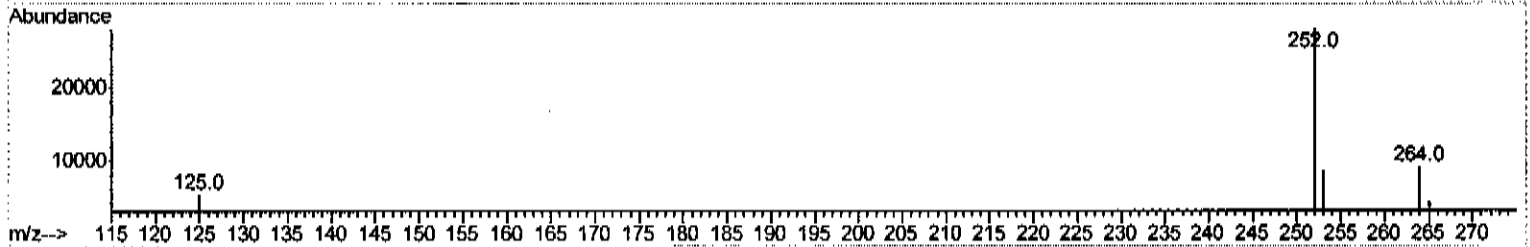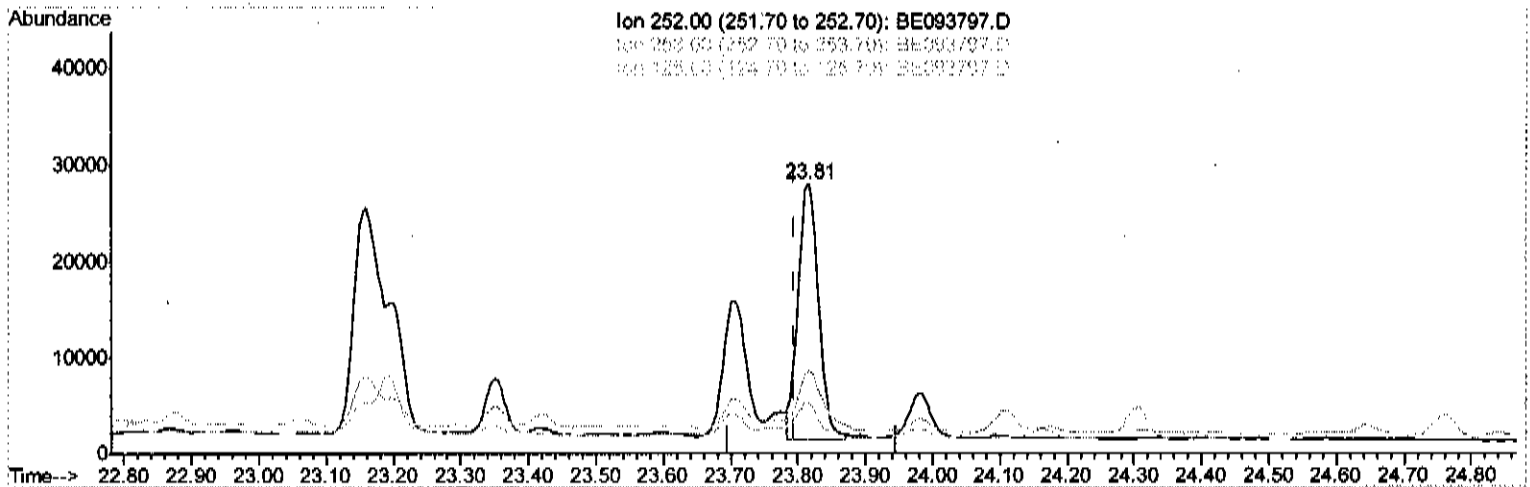

TIC: BE093797.D

(23) Benzo(a)pyrene (C)

23.815min (+0.019) 1.17ng/ul m

response 56229

Ion	Exp%	Act%
252.00	100	100
253.00	35.60	31.08
125.00	22.60	18.56
0.00	0.00	0.00

Quantitation Report (Qcudit)




Data Path : Z:\HPCHEM1\BNA E\Data\BE081417\
 Data File : BE093797.D
 Acq On : 14 Aug 2017 21:21
 Operator : SJ/JU
 Sample : I4529-11
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AA5

Manual Integrations
 APPROVED

Sohil
 8/21/2017 1:43:32 PM

Quant Time: Aug 18 08:29:50 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 17 19:06:13 2017
 Response via : Initial Calibration

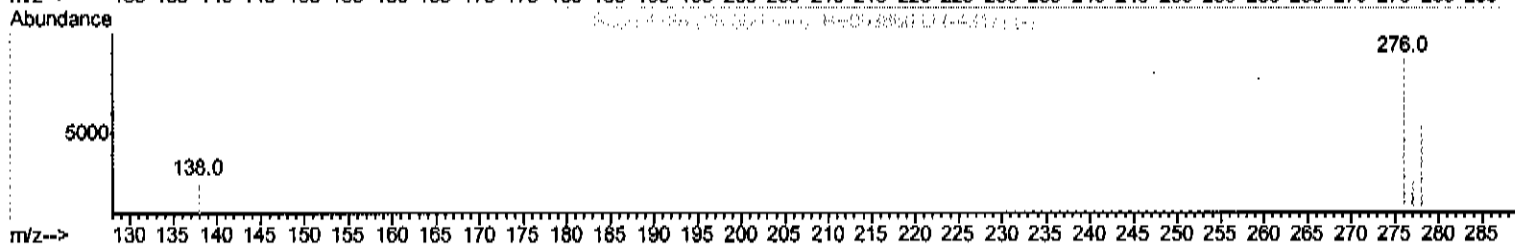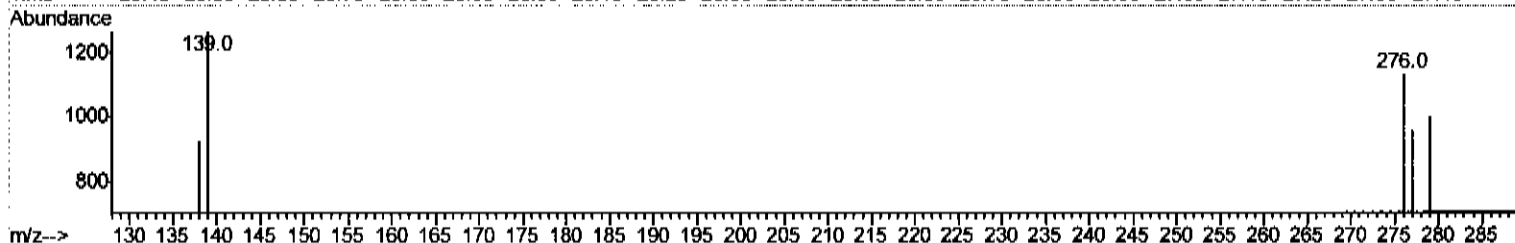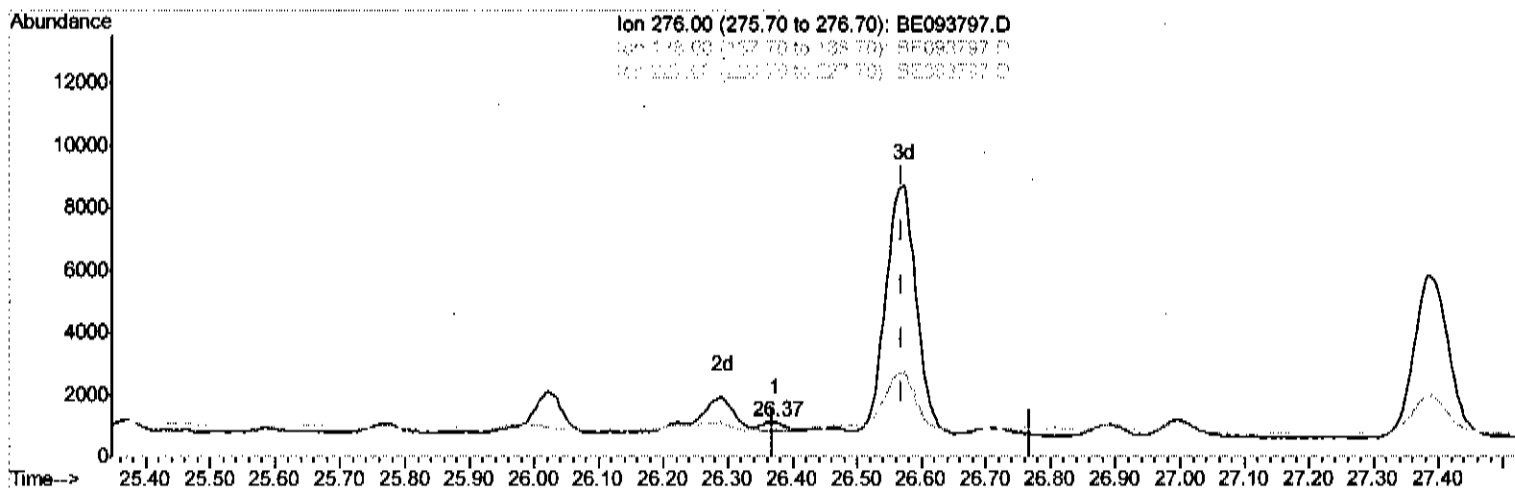

TIC: BE093797.D

(24) Indeno(1,2,3-cd)pyrene

26.373min (-0.196) 0.00ng/ul

response 685

Ion	Exp%	Act%
276.00	100	100
138.00	35.00	0.00#
227.00	10.00	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\Data\BE081417\
Data File : BE093797.D
Acq On : 14 Aug 2017 21:21
Operator : SJ/JU
Sample : I4529-11
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
C0AA5

Manual Integrations
APPROVED

Sohil
8/21/2017 1:43:32 PM

Quant Time: Aug 15 19:19:06 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 15 10:51:12 2017
Response via : Initial Calibration

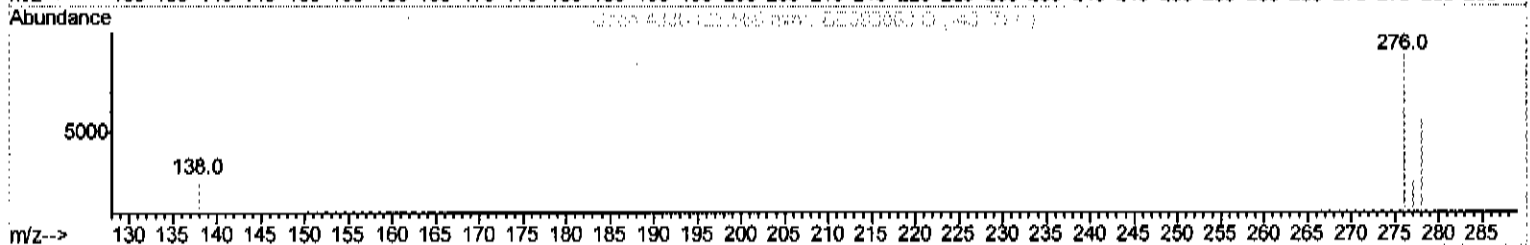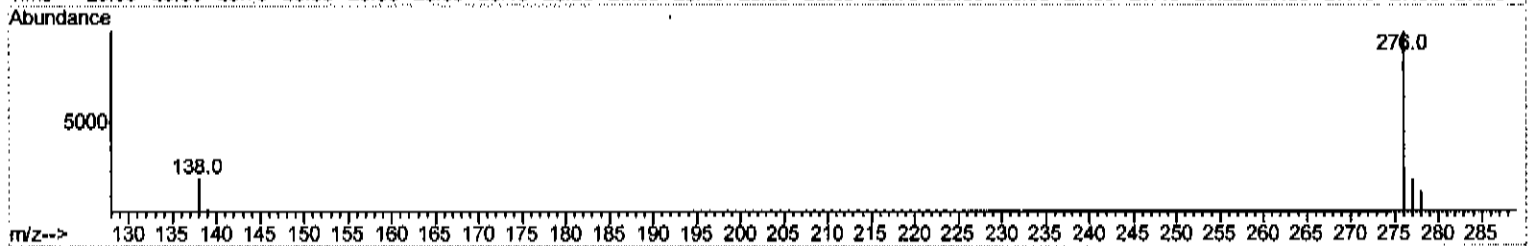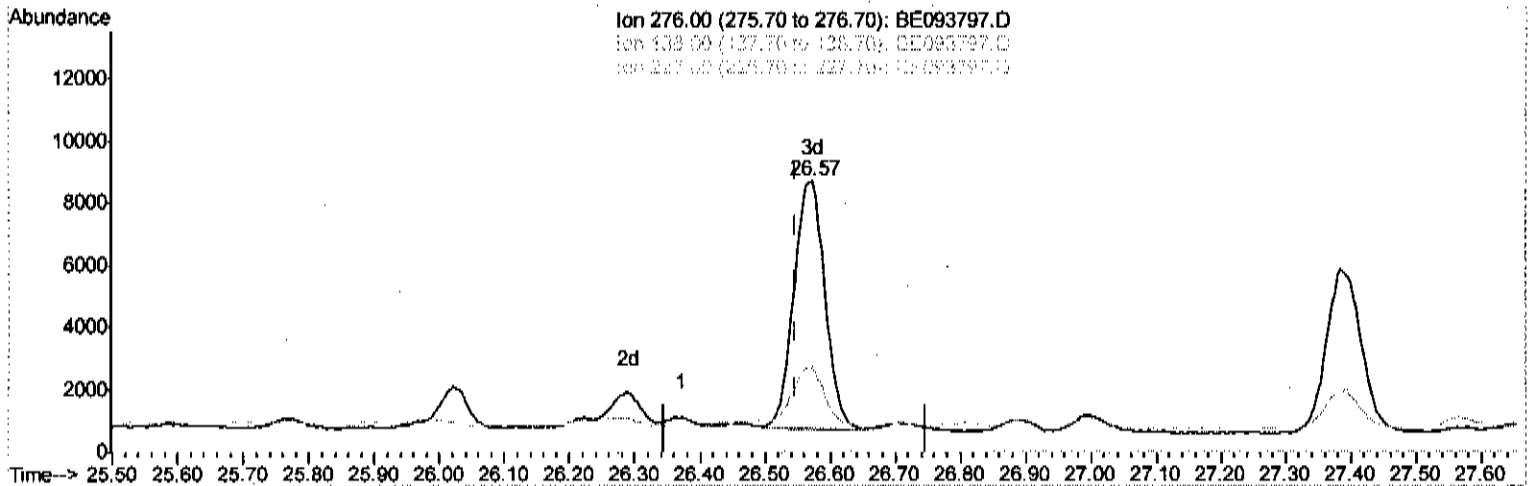

TIC: BE093797.D

(24) Indeno(1,2,3-cd)pyrene

26.573min (+0.027) 0.50ng/ul m

response 26509

Ion	Exp%	Act%
276.00	100	100
138.00	35.00	0.00#
227.00	10.00	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\Data\BE081417\
 Data File : BE093797.D
 Acq On : 14 Aug 2017 21:21
 Operator : SJ/JU
 Sample : I4529-11
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 C0AA5

Manual Integrations
 APPROVED

Sohil
 8/21/2017 1:43:32 PM

Quant Time: Aug 18 08:29:50 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 17 19:06:13 2017
 Response via : Initial Calibration

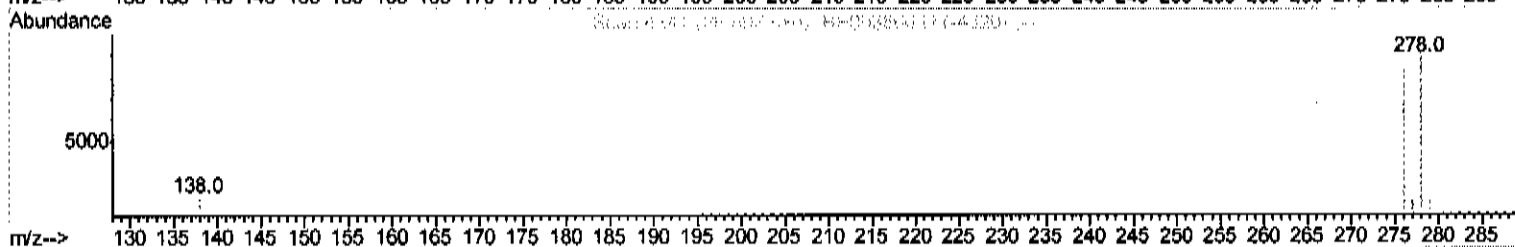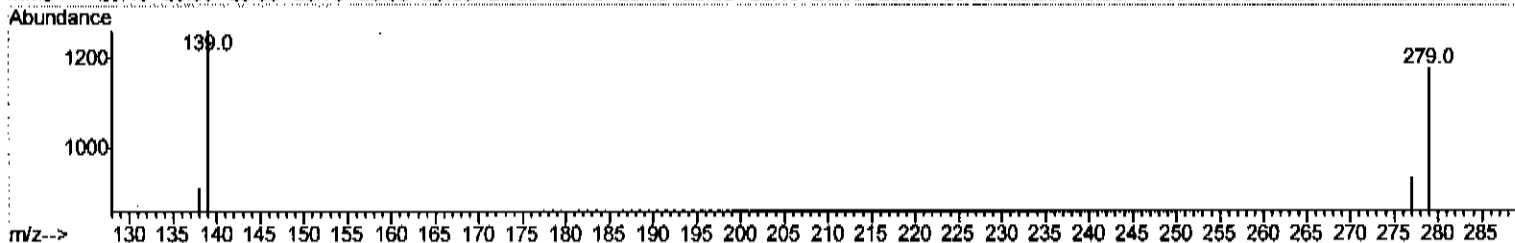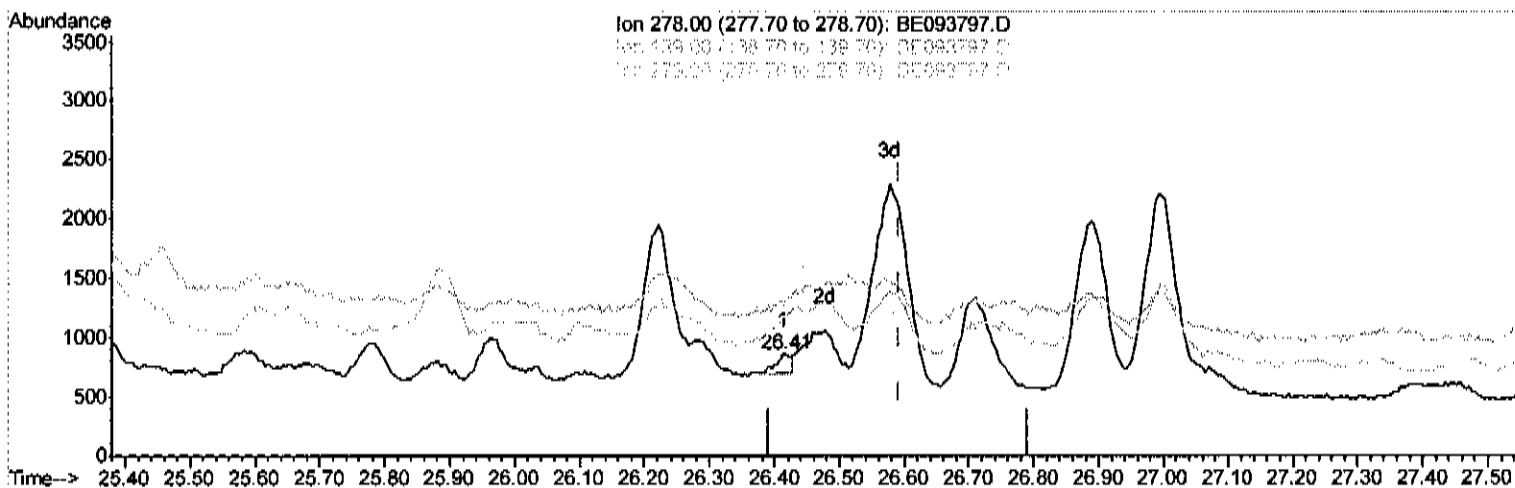

TIC: BE093797.D

(25) Dibenzo(a,h)anthracene

26.414min (-0.178) 0.00ng/ul

response 272

Ion	Exp%	Act%
278.00	100	100
139.00	21.70	146.40#
279.00	32.40	136.40#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\Data\BE081417\
 Data File : BE093797.D
 Acq On : 14 Aug 2017 21:21
 Operator : SJ/JU
 Sample : I4529-11
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AA5

Manual Integrations
 APPROVED

Sohil
 8/21/2017 1:43:32 PM

Quant Time: Aug 15 19:19:06 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 15 10:51:12 2017
 Response via : Initial Calibration

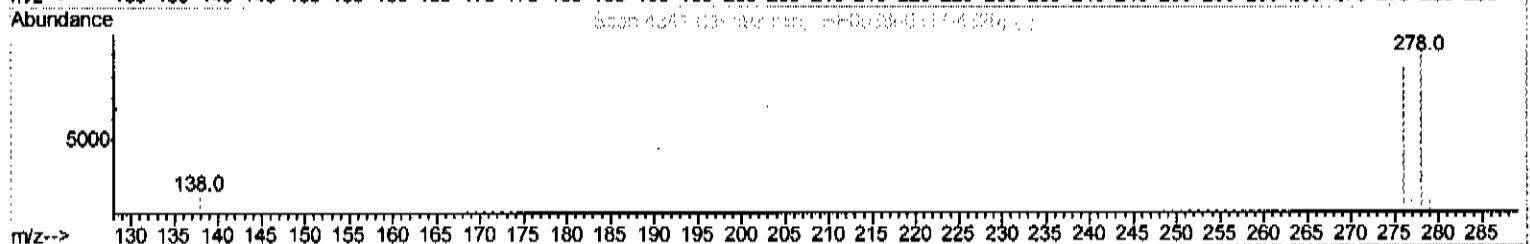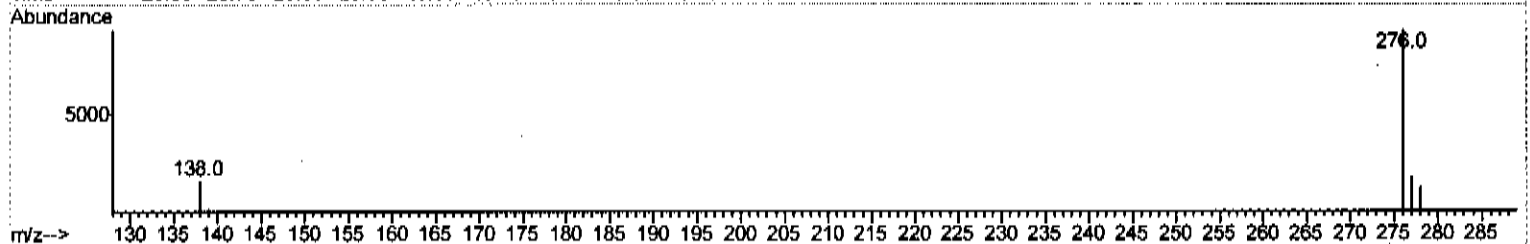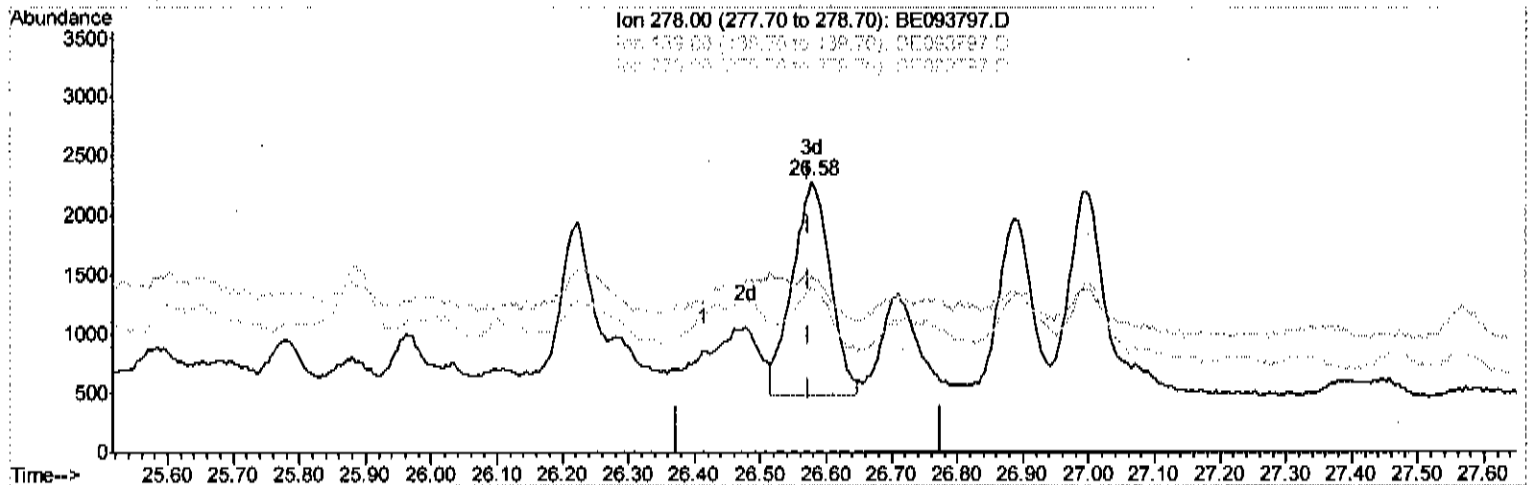

TIC: BE093797.D

(25) Dibenzo(a,h)anthracene

26.578min (+0.004) 0.16ng/ul m

response 7198

Ion	Exp%	Act%
278.00	100	100
139.00	21.70	65.17#
279.00	32.40	60.85#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\Data\BE081417\
 Data File : BE093797.D
 Acq On : 14 Aug 2017 21:21
 Operator : SJ/JU
 Sample : I4529-11
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 C0AA5

Manual Integrations
 APPROVED

Sohil
 8/21/2017 1:43:32 PM

Quant Time: Aug 18 08:29:50 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 17 19:06:13 2017
 Response via : Initial Calibration

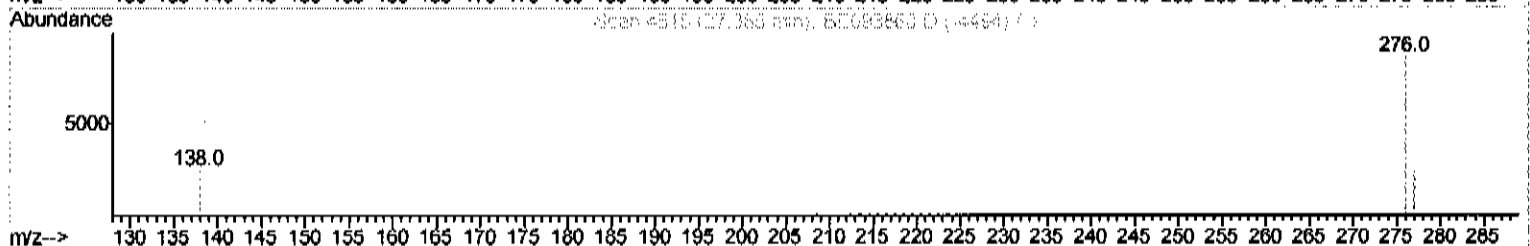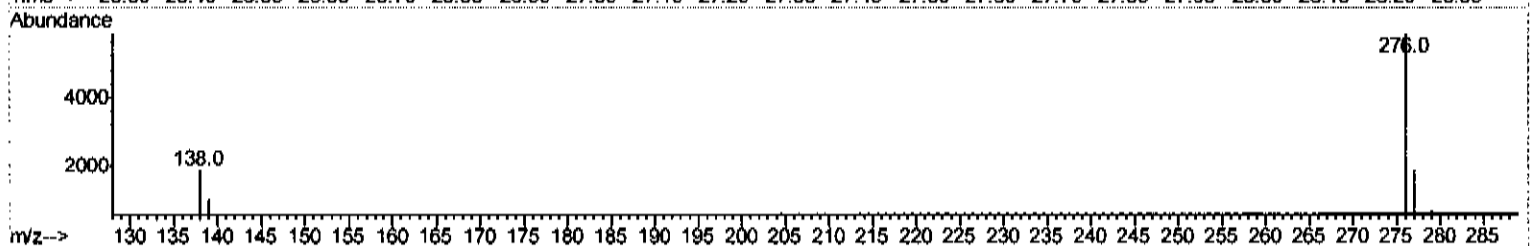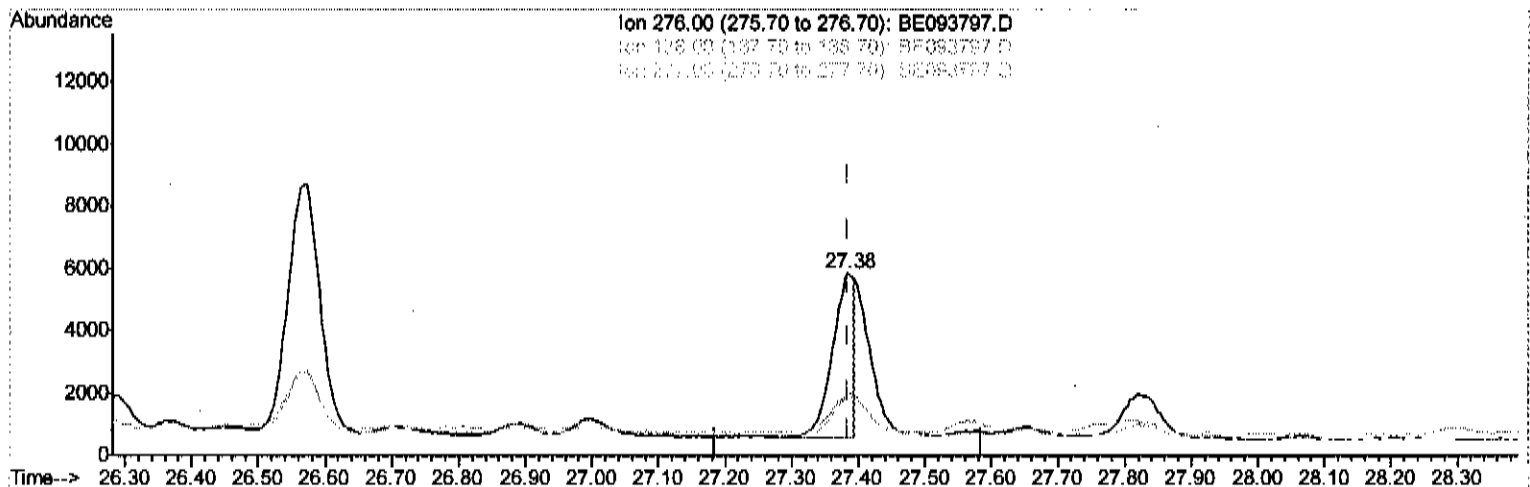

TIC: BE093797.D

(26) Benzo(g,h,i)perylene

27.384min (-0.000) 0.00ng/ul

response 11773

Ion	Exp%	Act%
276.00	100	100
138.00	27.30	32.41
277.00	25.60	32.65#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\Data\BE081417\
Data File : BE093797.D
Acq On : 14 Aug 2017 21:21
Operator : SJ/JU
Sample : I4529-11
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AA5

Manual Integrations
APPROVED

Sohil
8/21/2017 1:43:32 PM

Quant Time: Aug 15 19:19:06 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 15 10:51:12 2017
Response via : Initial Calibration

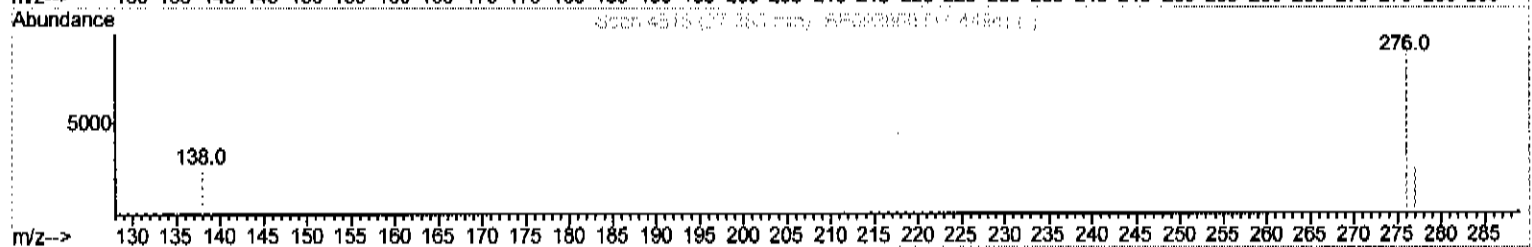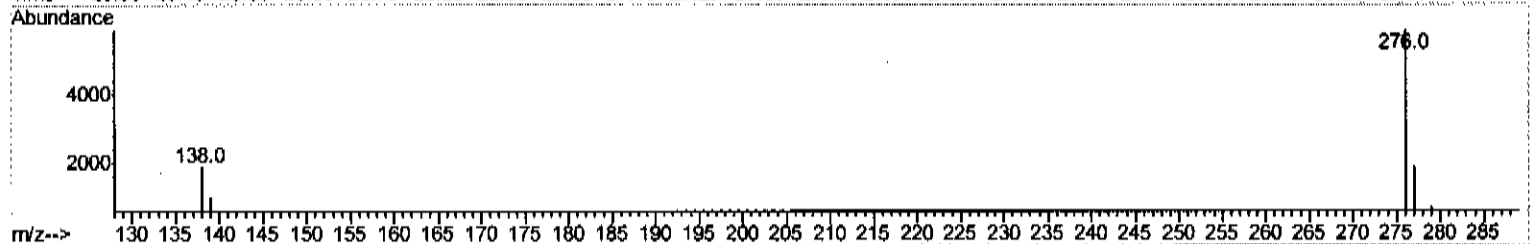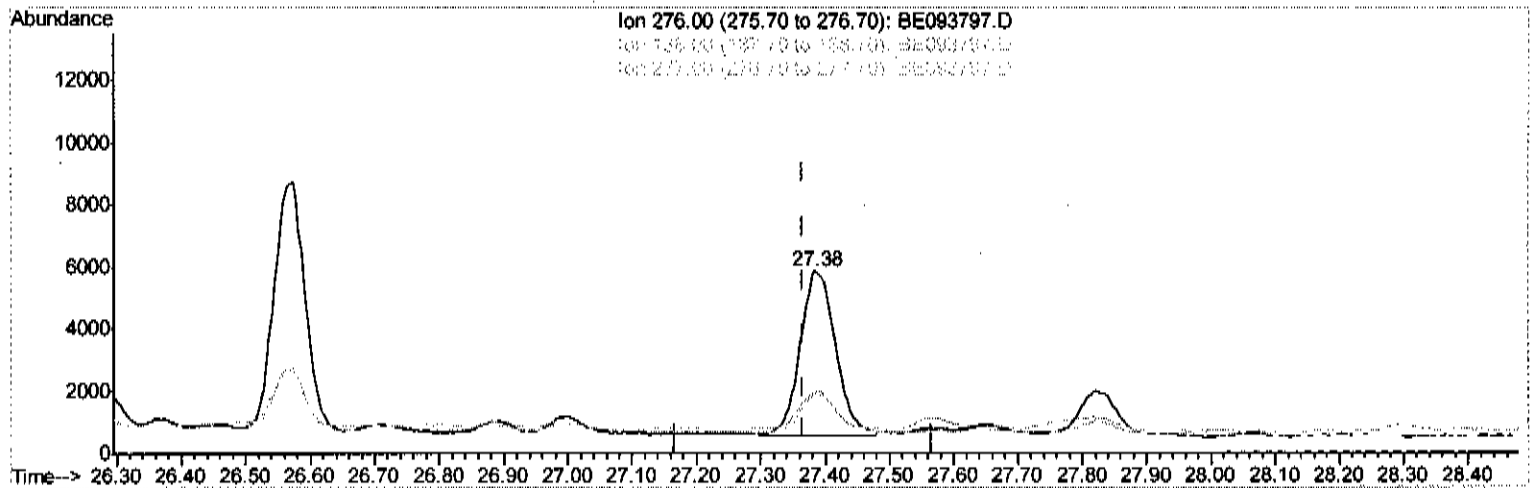

TIC: BE093797.D

(26) Benzo(g,h,i)perylene

27.384min (+0.018) 0.45ng/ul m

response 20028

Ion	Exp%	Act%
276.00	100	100
138.00	27.30	32.41
277.00	25.60	32.65#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\Data\BE081417\
 Data File : BE093797.D
 Acq On : 14 Aug 2017 21:21
 Operator : SJ/JU
 Sample : I4529-11
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AA5

Manual Integrations
 APPROVED

Sohil
 8/21/2017 1:43:32 PM

Quant Time: Aug 15 19:19:06 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 15 10:51:12 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.92	152	3144	0.40	ng/ul	0.00
2) Naphthalene-d8	10.71	136	15625	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.53	164	10738m	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.26	188	22290m	0.40	ng/ul	0.00
16) Chrysene-d12	21.42	240	19056	0.40	ng/ul	0.01
20) Perylene-d12	23.93	264	16340m	0.40	ng/ul	0.02

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.29	152	12175m	0.48	ng/ul	0.00
14) Fluoranthene-d10	19.28	212	26635	0.38	ng/ul	0.00

Target Compounds

						Ovalue
3) Naphthalene	10.75	128	116313	3.060	ng/ul#	93
5) 2-Methylnaphthalene	12.36	142	144399	5.208	ng/ul	99
7) Acenaphthylene	14.25	152	23992	0.534	ng/ul#	70
8) Acenaphthene	14.59	153	33723	0.954	ng/ul	96
9) Fluorene	15.57	166	173280	3.879	ng/ul	94
12) Phenanthrene	17.29	178	403326	6.644	ng/ul#	88
13) Anthracene	17.38	178	94836	1.604	ng/ul#	90
15) Fluoranthene	19.31	202	213241	2.809	ng/ul	83
17) Pyrene	19.67	202	255082	4.586	ng/ul#	85
18) Benzo(a)anthracene	21.40	228	78291	1.417	ng/ul#	80
19) Chrysene	21.45	228	81467	1.537	ng/ul#	82
21) Benzo(b)fluoranthene	23.16	252	61462	1.216	ng/ul	97
22) Benzo(k)fluoranthene	23.20	252	23040m	0.462	ng/ul	} 8/18/17
23) Benzo(a)pyrene	23.81	252	56229m	1.170	ng/ul	
24) Indeno(1,2,3-cd)pyrene	26.57	276	26509m	0.499	ng/ul	
25) Dibenzo(a,h)anthracene	26.58	278	7198m	0.162	ng/ul	
26) Benzo(a,h,i)perylene	27.38	276	20028m	0.448	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed