

Data Path : Z:\HPCHEM1\BNA E\DATA\BE081517\
 Data File : BE093803.D
 Acq On : 15 Aug 2017 12:19
 Operator : SJ/JU
 Sample : PB101423BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SBLK23

Quant Time: Aug 16 05:44:29 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 16 05:35:21 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.92	152	2647	0.40	ng/ul	0.00
2) Naphthalene-d8	10.71	136	13657	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.52	164	7995	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.26	188	17203	0.40	ng/ul	0.00
16) Chrysene-d12	21.41	240	18500	0.40	ng/ul	0.00
20) Perylene-d12	23.76	264	960625	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.29	152	5500	0.25	ng/ul	0.00
14) Fluoranthene-d10	19.28	212	12841	0.24	ng/ul	0.00
Target Compounds						
					Ovalue	
9) Fluorene	15.51	166	1629	0.049	ng/ul#	22
17) Pyrene	19.66	202	1118	0.021	ng/ul#	71


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE081517\
Data File : BE093803.D
Acq On : 15 Aug 2017 12:19
Operator : SJ/JU
Sample : PB101423BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK23

Quant Time: Aug 16 05:44:29 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 16 05:35:21 2017
Response via : Initial Calibration

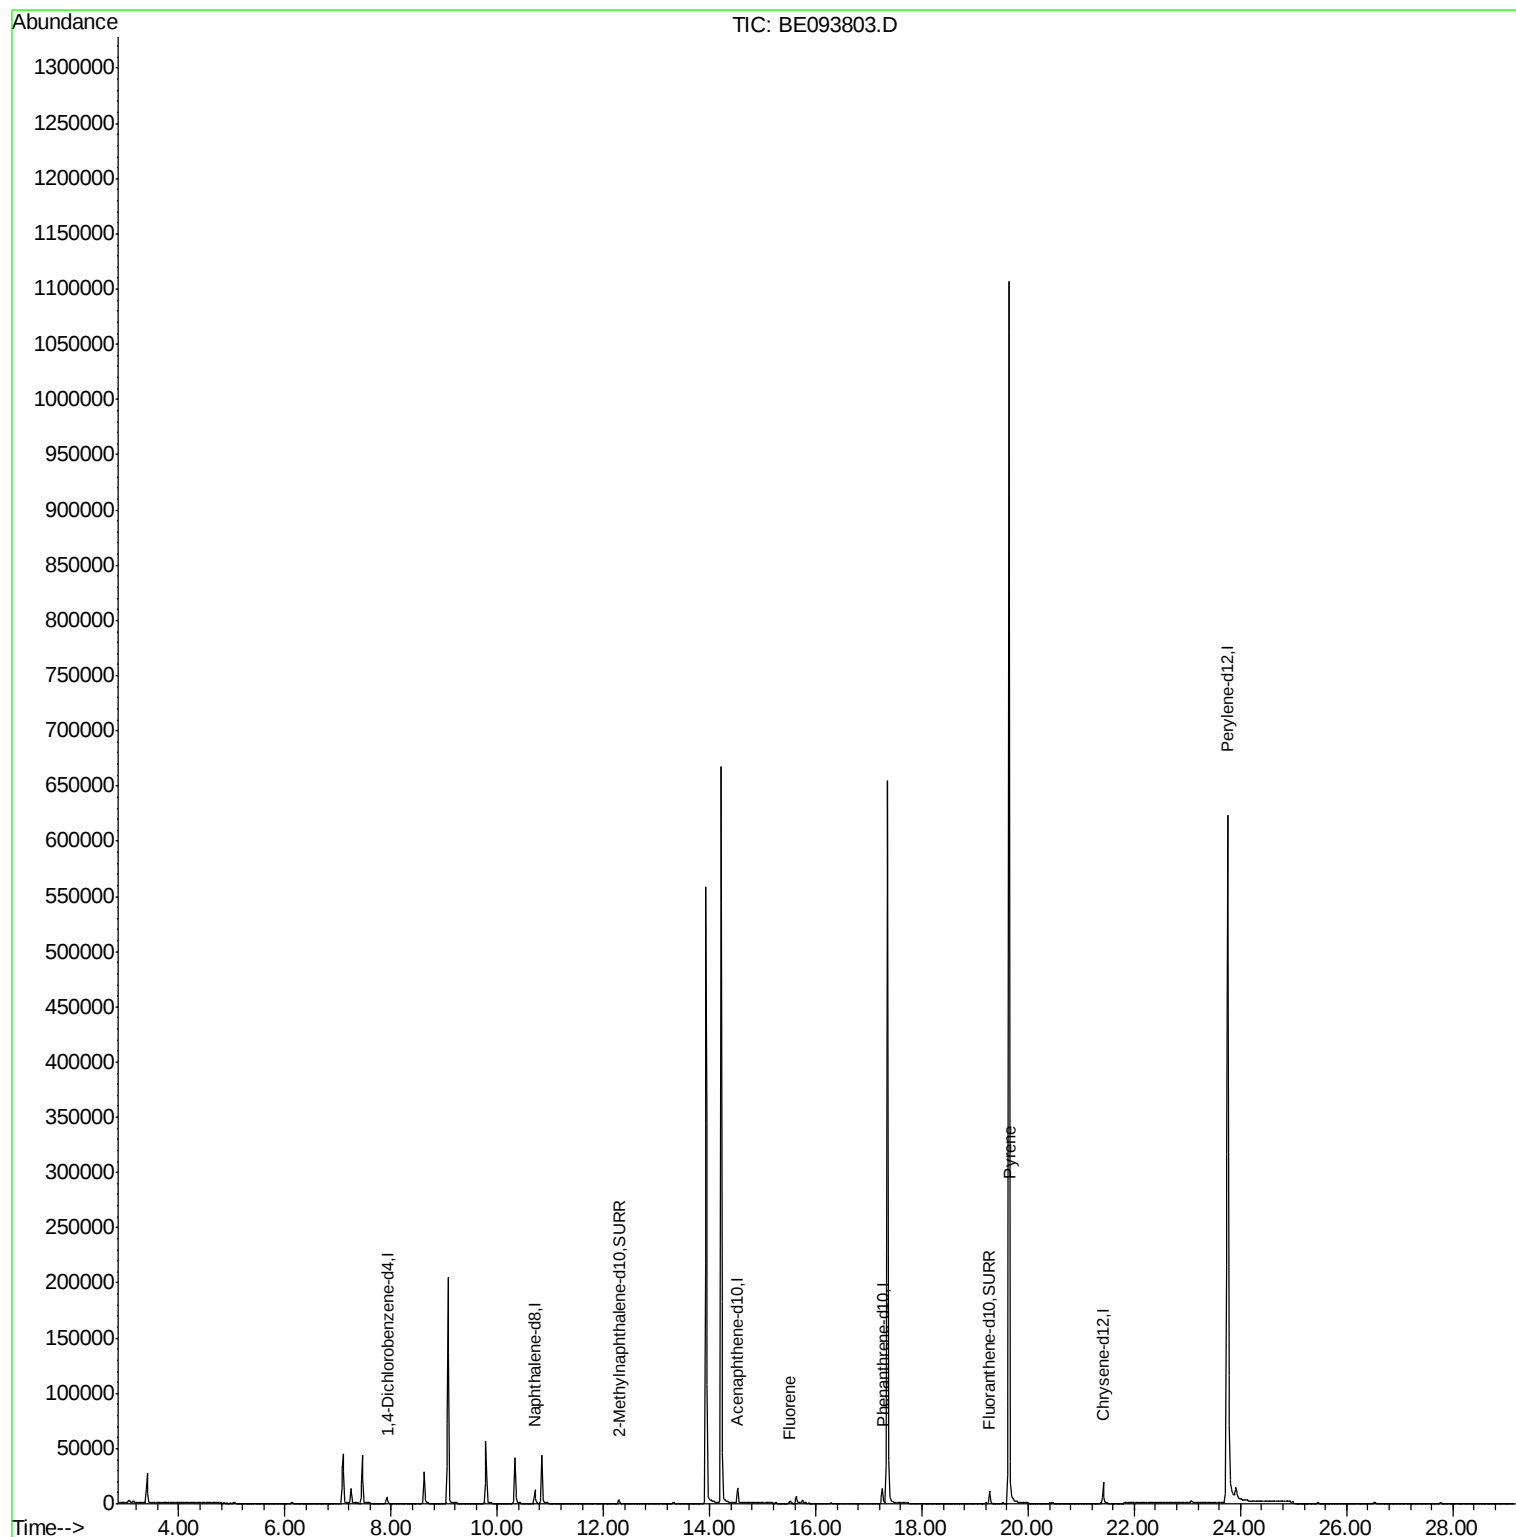

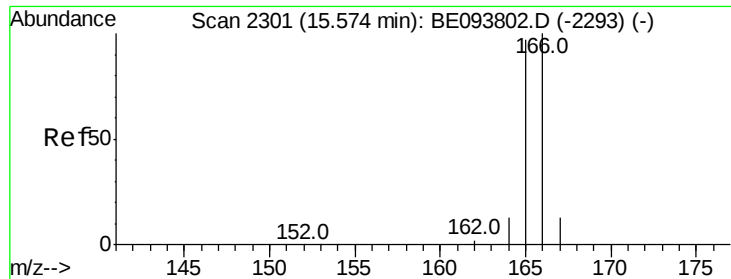

#9

Fluorene

Concen: 0.049 ng/ul

RT: 15.51 min Scan# 2293

Delta R.T. -0.06 min

Lab File: BE093803.D

Acq: 15 Aug 2017 12:19

Instrument :

BNA_E

ClientSampleId :

SBLK23





Tot Ion:166 Resp: 1629

Ion Ratio Lower Upper

166 100

165 8.4 73.4 110.2#

167 32.9 14.6 22.0#

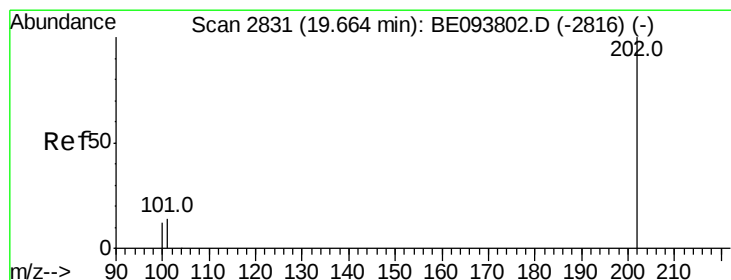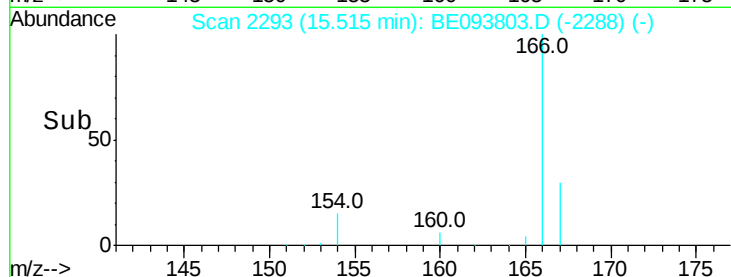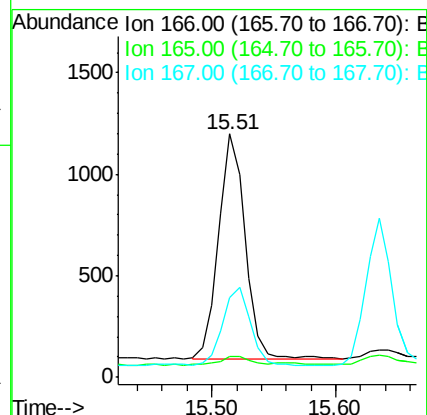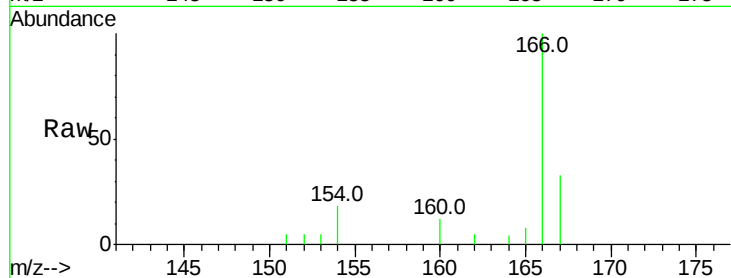

#17

Pyrene

Concen: 0.021 ng/ul

RT: 19.66 min Scan# 2831

Delta R.T. -0.00 min

Lab File: BE093803.D

Acq: 15 Aug 2017 12:19

Tgt Ion:202 Resp: 1118

Ion Ratio Lower Upper

202 100

101 26.5 18.2 27.4

100 43.7 15.6 23.4#

