

Data Path : Z:\HPCHEM1\BNA E\DATA\BE081517\
 Data File : BE093811.D
 Acq On : 15 Aug 2017 17:18
 Operator : SJ/JU
 Sample : I4673-08
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AL1

Quant Time: Aug 16 05:46:29 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 16 05:35:21 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.92	152	2381	0.40	ng/ul	0.00
2) Naphthalene-d8	10.70	136	12683	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.52	164	7832	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.26
16) Chrysene-d12	21.41	240	16929	0.40	ng/ul	0.00
20) Perylene-d12	23.76	264	1192941	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.29	152	6307	0.31	ng/ul	0.00
14) Fluoranthene-d10	19.27	212	16708	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	19.64	202	2710	0.055	ng/ul#	Ovalue 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE081517\
Data File : BE093811.D
Acq On : 15 Aug 2017 17:18
Operator : SJ/JU
Sample : I4673-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AL1

Quant Time: Aug 16 05:46:29 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 16 05:35:21 2017
Response via : Initial Calibration

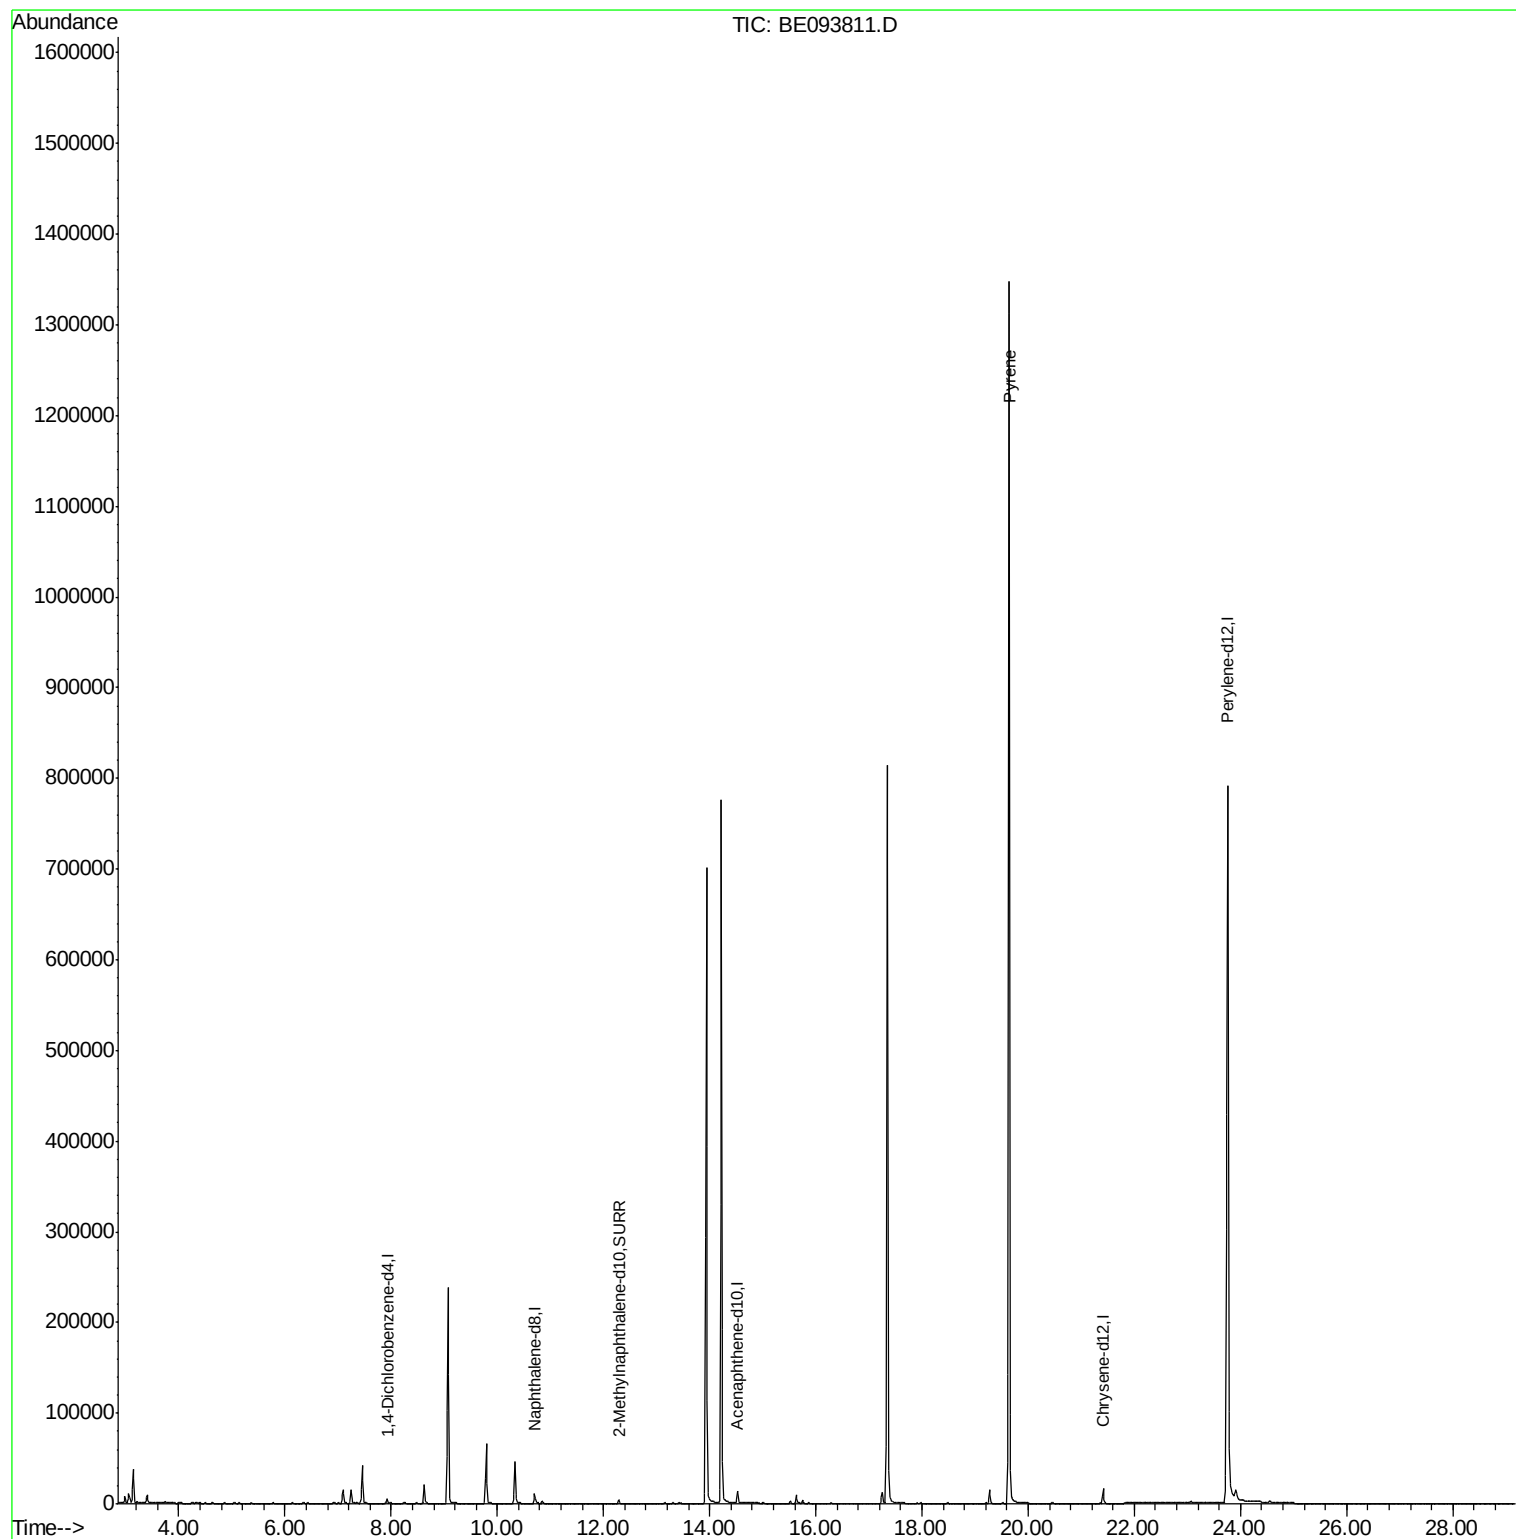

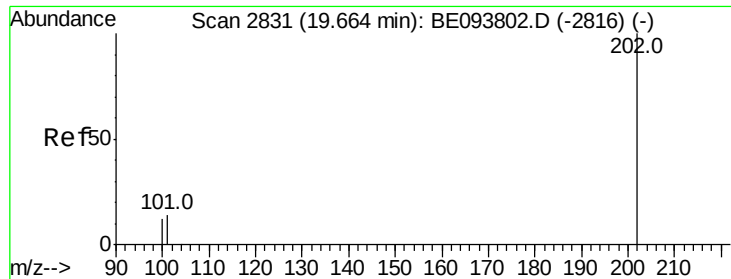

#17
 Pvrene
 Concen: 0.055 ng/ul
 RT: 19.64 min Scan# 2826
 Delta R.T. -0.02 min
 Lab File: BE093811.D
 Acq: 15 Aug 2017 17:18

Instrument :
 BNA_E
 ClientSampleId :
 C0AL1

Tot Ion:202 Resp: 2710
 Ion Ratio Lower Upper
 202 100
 101 167.2 18.2 27.4#
 100 888.4 15.6 23.4#

