

Data Path : Z:\HPCHEM1\BNA E\DATA\BE081517\
 Data File : BE093820.D
 Acq On : 15 Aug 2017 22:52
 Operator : SJ/JU
 Sample : I4672-14
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AJ2

Quant Time: Aug 16 07:37:39 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 16 07:30:49 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.92	152	2604	0.40	ng/ul	0.00
2) Naphthalene-d8	10.70	136	14050	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.52	164	8534	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.26	188	17811	0.40	ng/ul	0.00
16) Chrysene-d12	21.41	240	18454	0.40	ng/ul	0.00
20) Perylene-d12	23.76	264	935254	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.28	152	5425	0.24	ng/ul	0.00
14) Fluoranthene-d10	19.27	212	13377	0.24	ng/ul	0.00
Target Compounds				Ovalue		
3) Naphthalene	10.76	128	5427	0.159	ng/ul#	94
5) 2-Methylnaphthalene	12.36	142	2245	0.090	ng/ul	99
7) Acenaphthylene	14.24	152	1307	0.037	ng/ul#	84
8) Acenaphthene	14.59	153	2129	0.076	ng/ul	99
9) Fluorene	15.57	166	2518	0.071	ng/ul	94
12) Phenanthrene	17.29	178	35066	0.723	ng/ul#	89
13) Anthracene	17.38	178	9489	0.201	ng/ul#	91
15) Fluoranthene	19.30	202	76674	1.264	ng/ul	84
17) Pyrene	19.66	202	71846	1.334	ng/ul#	83
18) Benzo(a)anthracene	21.39	228	38115	0.712	ng/ul#	87
19) Chrysene	21.45	228	36646	0.714	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE081517\
Data File : BE093820.D
Acq On : 15 Aug 2017 22:52
Operator : SJ/JU
Sample : I4672-14
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AJ2

Quant Time: Aug 16 07:37:39 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 16 07:30:49 2017
Response via : Initial Calibration

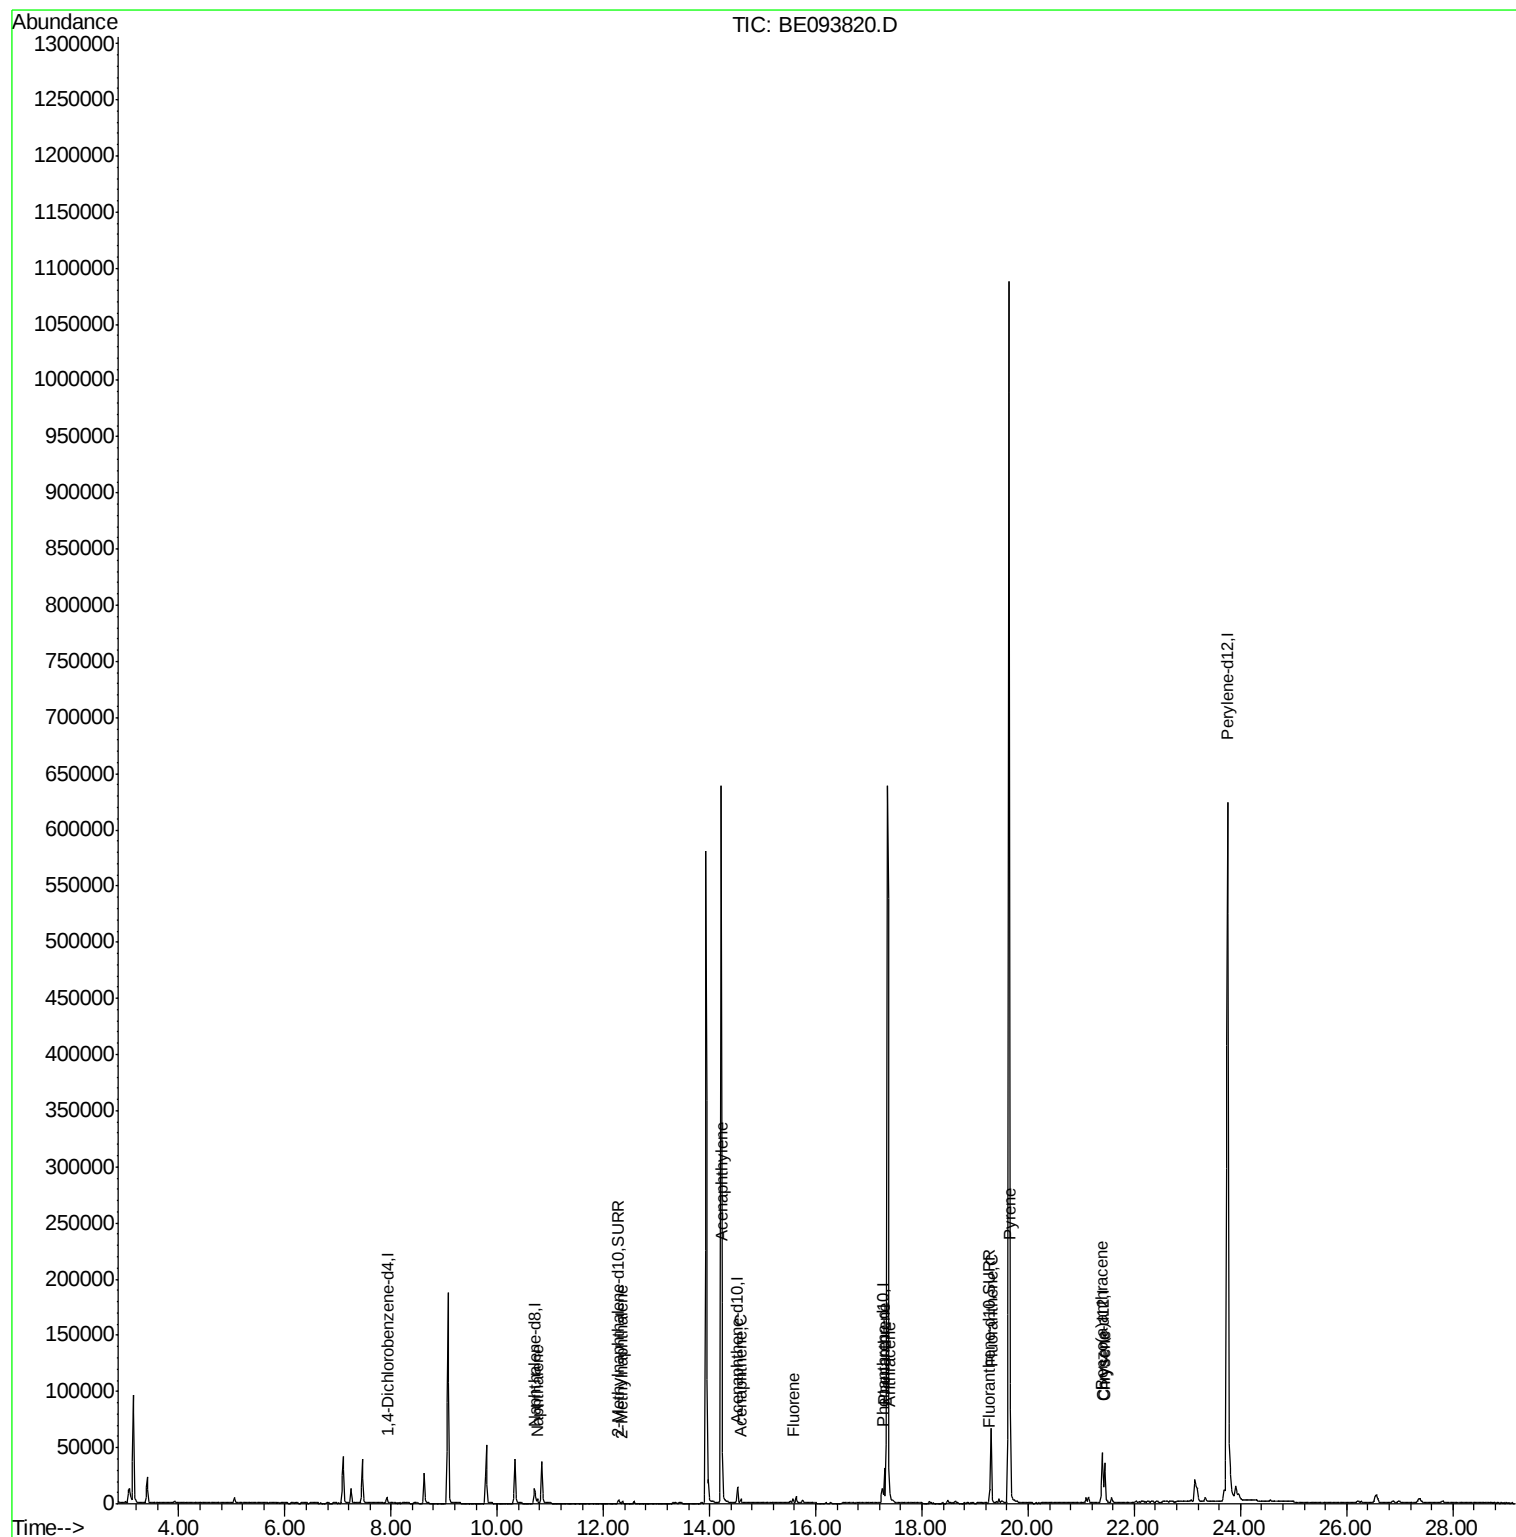

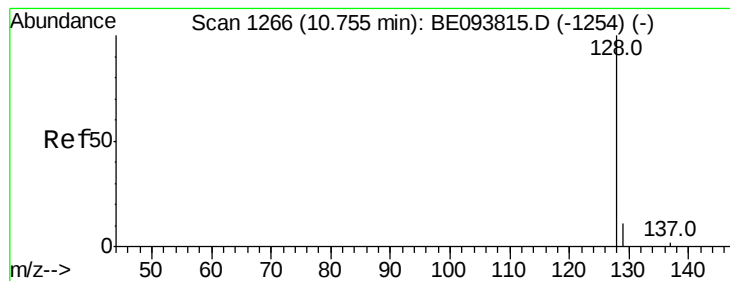

#3

Naphthalene

Concen: 0.159 ng/ul

RT: 10.76 min Scan# 1266

Delta R.T. 0.00 min

Lab File: BE093820.D

Acq: 15 Aug 2017 22:52

Instrument :

BNA_E

ClientSampleId :

C0AJ2


Tot Ion:128 Resp: 5427

Ion Ratio Lower Upper

128 100

129 12.9 11.3 16.9




127 0.0 4.0 6.0#

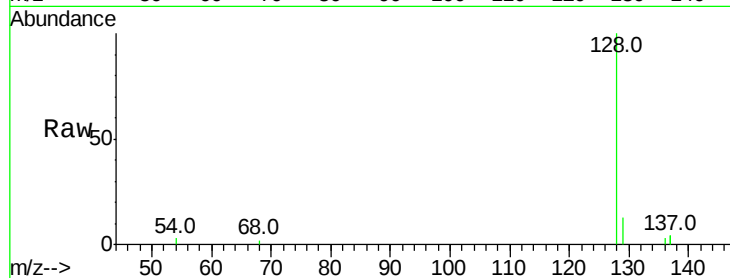

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

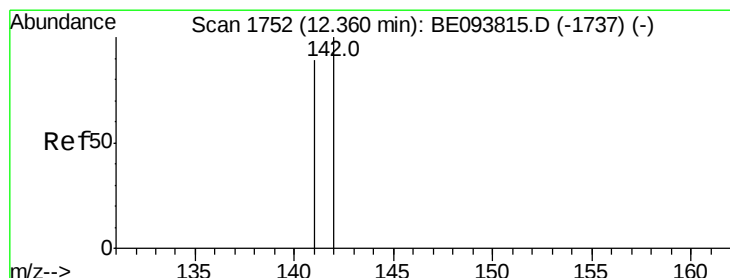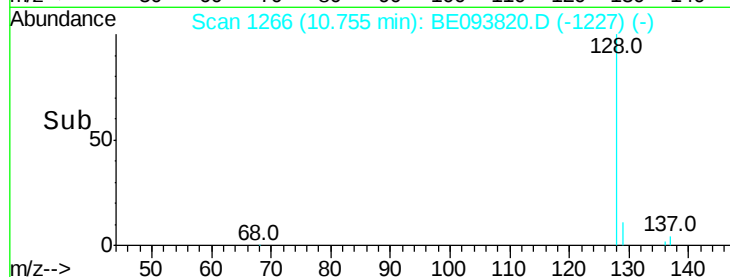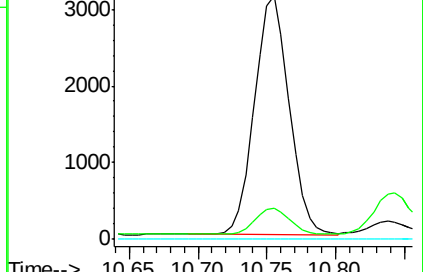

#5

2-Methylnaphthalene

Concen: 0.090 ng/ul

RT: 12.36 min Scan# 1751

Delta R.T. -0.00 min

Lab File: BE093820.D


Acq: 15 Aug 2017 22:52

Tgt Ion:142 Resp: 2245

Ion Ratio Lower Upper



142 100


141 89.4 72.6 108.8

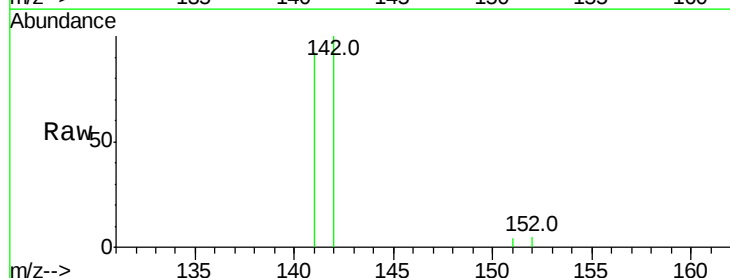

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

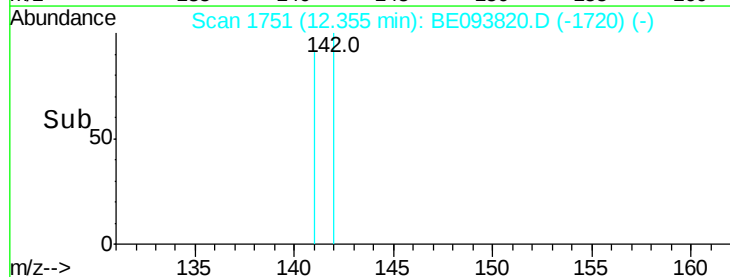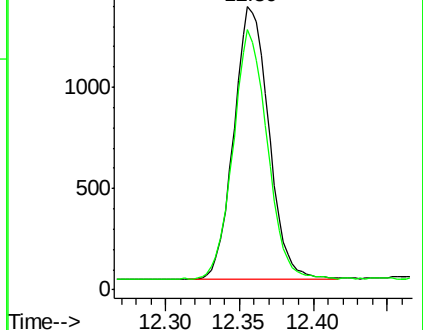

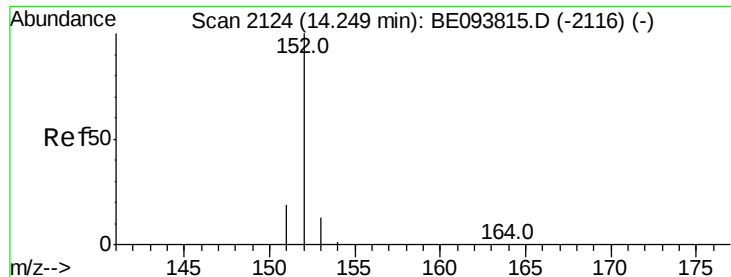

#7

Acenaphthylene

Concen: 0.037 ng/ul

RT: 14.24 min Scan# 2124

Delta R.T. -0.01 min

Lab File: BE093820.D

Acq: 15 Aug 2017 22:52

Instrument :

BNA_E

ClientSampleId :

C0AJ2


Tot Ion:152 Resp: 1307

Ion Ratio Lower Upper

152 100

151 27.4 17.1 25.7#




153 25.0 12.8 19.2#

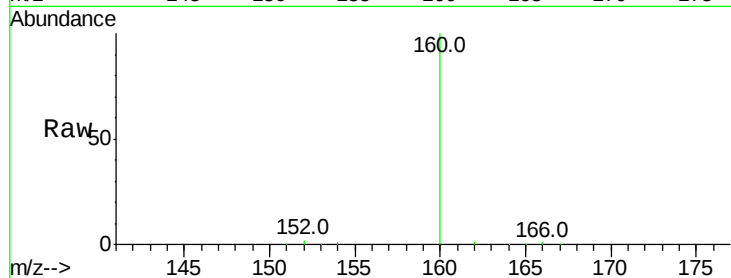

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

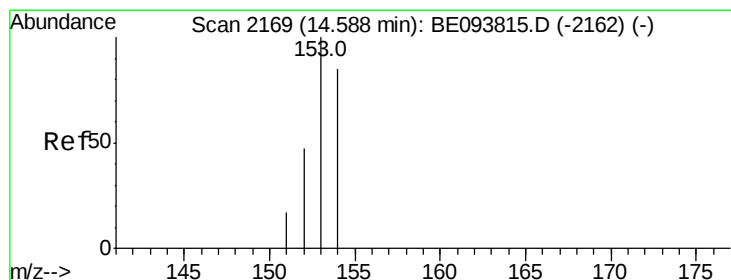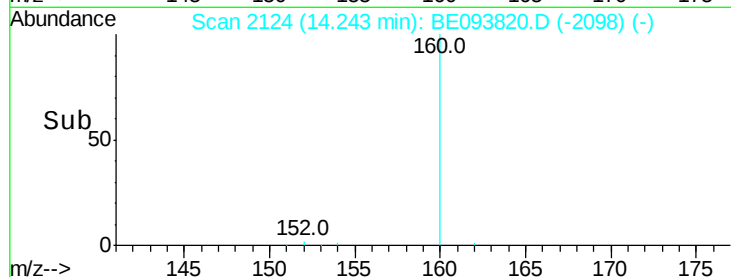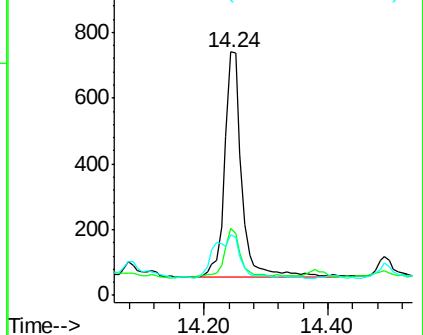

#8

Acenaphthene

Concen: 0.076 ng/ul

RT: 14.59 min Scan# 2170

Delta R.T. 0.00 min

Lab File: BE093820.D

Acq: 15 Aug 2017 22:52


Tgt Ion:153 Resp: 2129

Ion Ratio Lower Upper

153 100

152 48.6 40.3 60.5



154 89.1 71.4 107.2

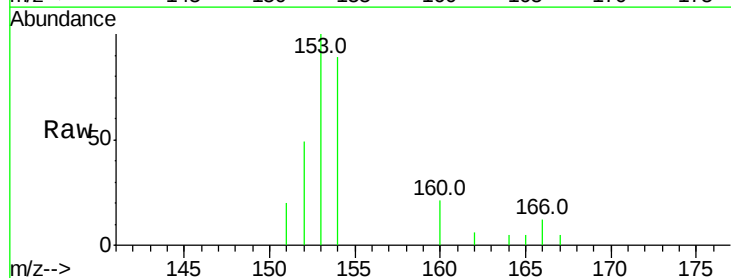


Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

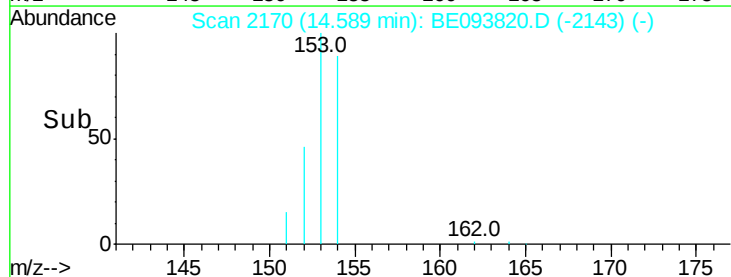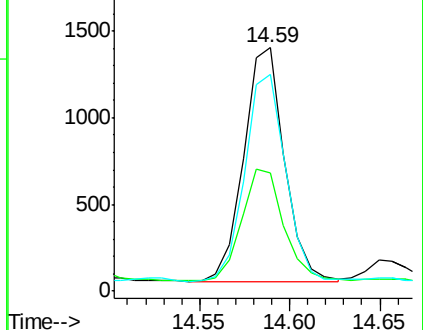

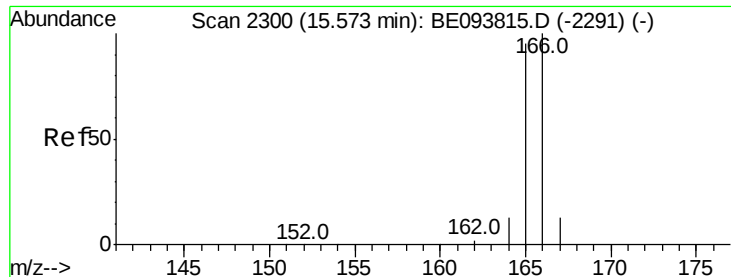

#9

Fluorene

Concen: 0.071 ng/ul

RT: 15.57 min Scan# 2300

Delta R.T. -0.01 min

Lab File: BE093820.D

Acq: 15 Aug 2017 22:52

Instrument :

BNA_E

ClientSampleId :

C0AJ2


Tot Ion:166 Resp: 2518

Ion Ratio Lower Upper




166 100

165 98.7 73.4 110.2

167 18.4 14.6 22.0

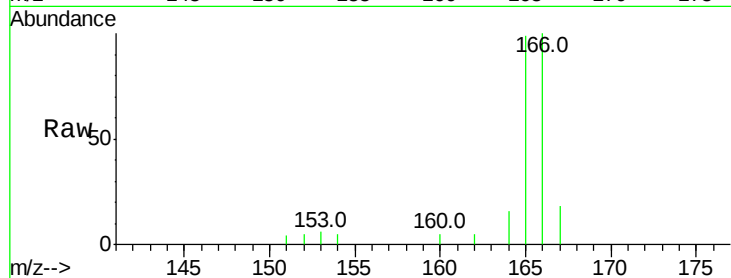

Abundance Ion 166.00 (165.70 to 166.70): E
Ion 165.00 (164.70 to 165.70): E
Ion 167.00 (166.70 to 167.70): E

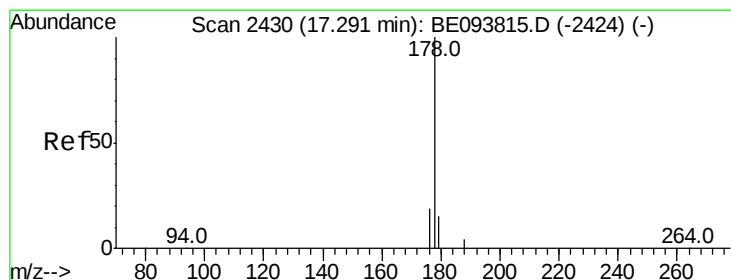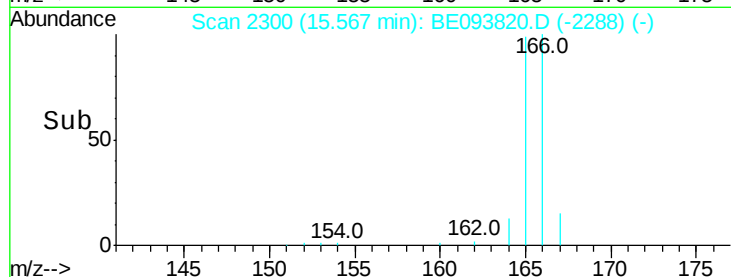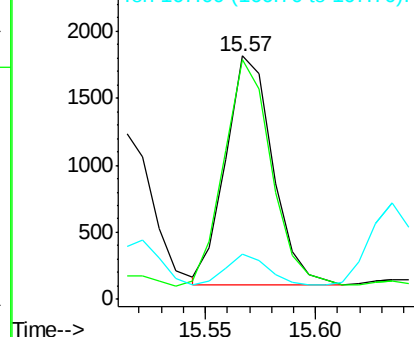

#12

Phenanthrene

Concen: 0.723 ng/ul

RT: 17.29 min Scan# 2431

Delta R.T. 0.00 min

Lab File: BE093820.D

Acq: 15 Aug 2017 22:52


Tgt Ion:178 Resp: 35066

Ion Ratio Lower Upper



178 100


179 15.1 18.4 27.6#

176 18.9 13.6 20.4

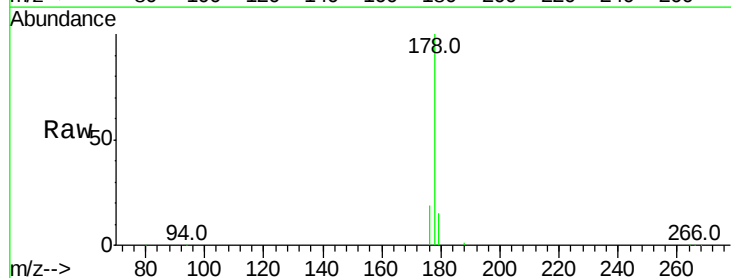

Abundance Ion 178.00 (177.70 to 178.70): E
Ion 179.00 (178.70 to 179.70): E
Ion 176.00 (175.70 to 176.70): E

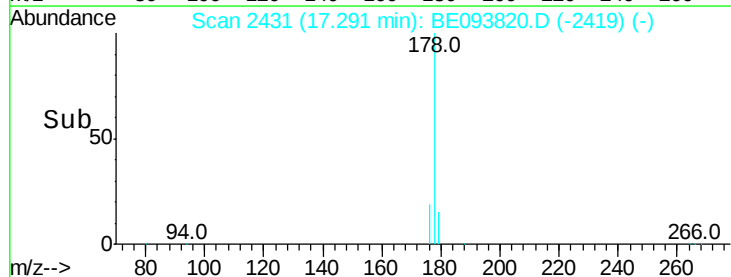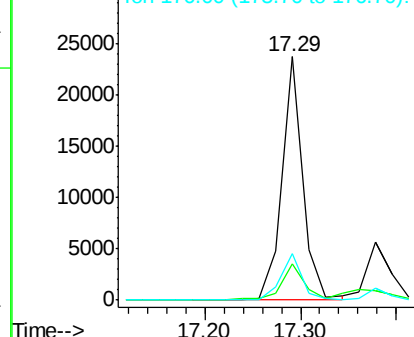

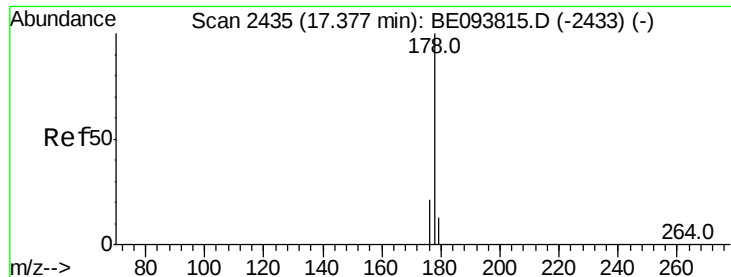

#13

Anthracene

Concen: 0.201 ng/ul

RT: 17.38 min Scan# 2436

Delta R.T. 0.00 min

Lab File: BE093820.D

Acq: 15 Aug 2017 22:52

Instrument :

BNA_E

ClientSampleId :

C0AJ2





Tot Ion:178 Resp: 9489

Ion Ratio Lower Upper

178 100

179 16.6 18.1 27.1#

176 20.6 14.7 22.1

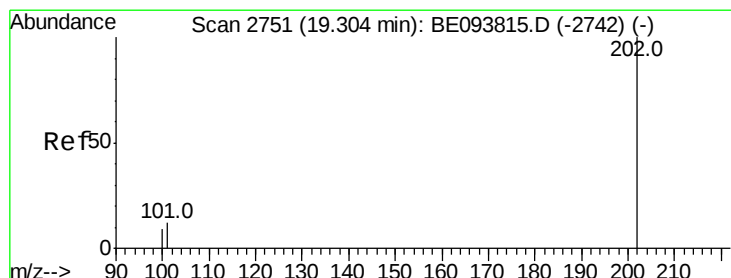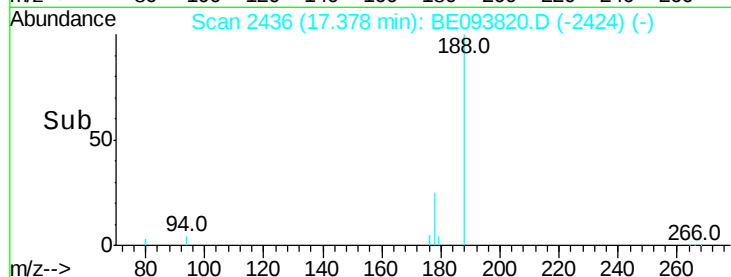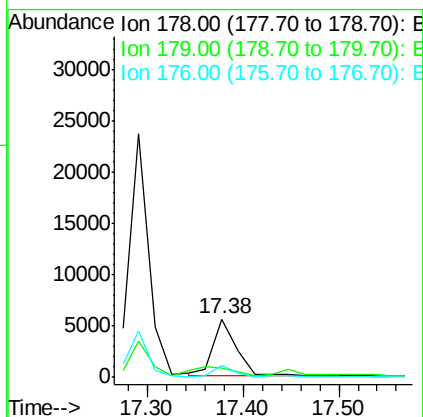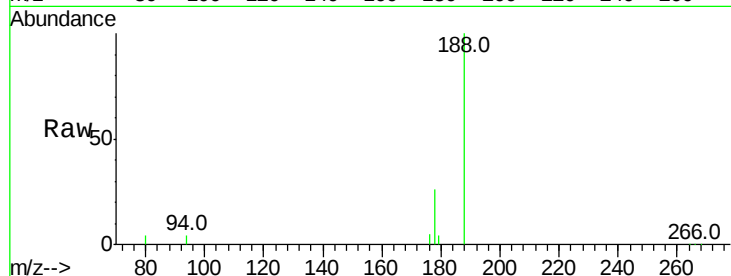

#15

Fluoranthene

Concen: 1.264 ng/ul

RT: 19.30 min Scan# 2752

Delta R.T. 0.00 min

Lab File: BE093820.D

Acq: 15 Aug 2017 22:52




Tgt Ion:202 Resp: 76674


Ion Ratio Lower Upper

202 100

101 11.2 0.0 30.3

100 8.9 0.0 39.5

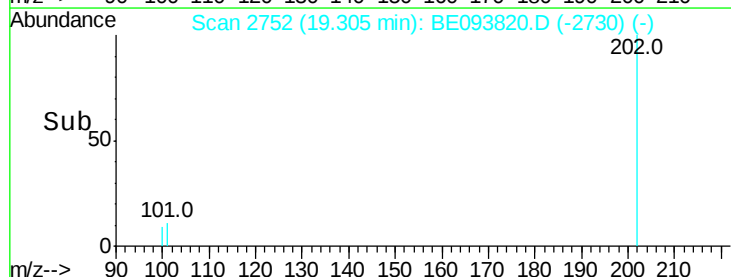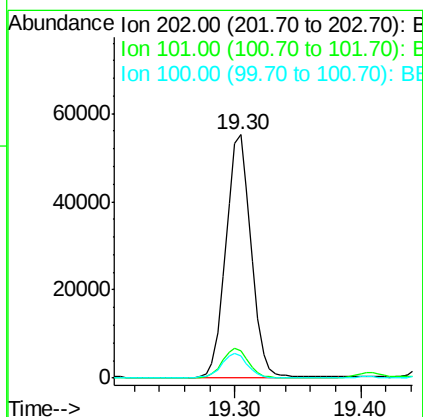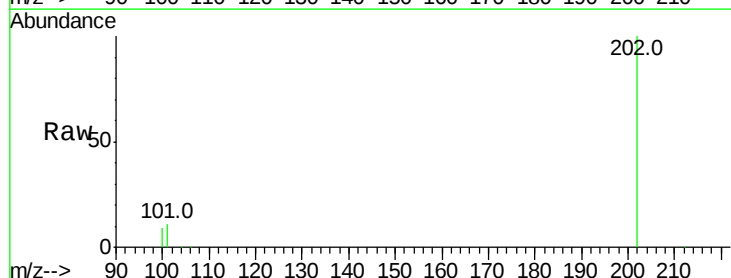

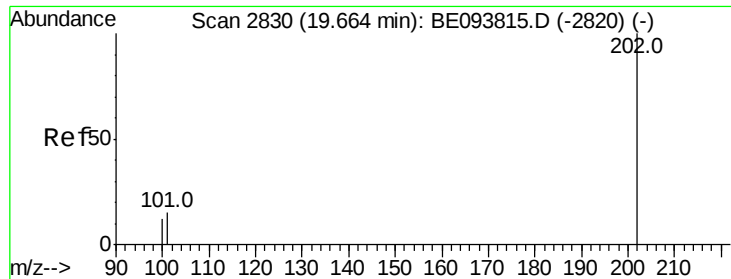

#17

Pvrene

Concen: 1.334 ng/ul

RT: 19.66 min Scan# 2831

Delta R.T. 0.00 min

Lab File: BE093820.D

Acq: 15 Aug 2017 22:52

Instrument :

BNA_E

ClientSampleId :

C0AJ2


Tot Ion:202 Resp: 71846

Ion Ratio Lower Upper

202 100

101 13.9 18.2 27.4#




100 12.1 15.6 23.4#

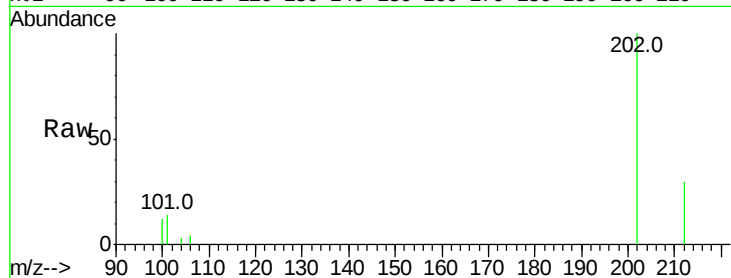

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): E

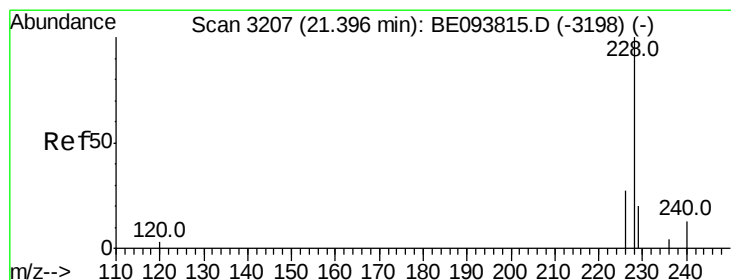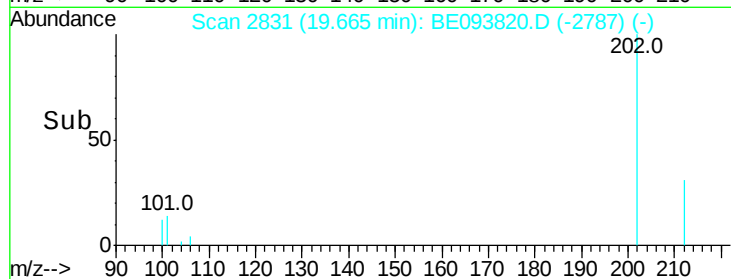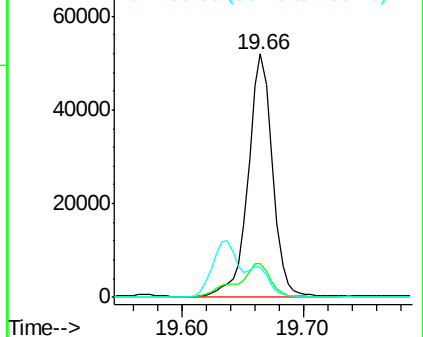

#18

Benzo(a)anthracene

Concen: 0.712 ng/ul

RT: 21.39 min Scan# 3207

Delta R.T. -0.00 min

Lab File: BE093820.D

Acq: 15 Aug 2017 22:52


Tgt Ion:228 Resp: 38115

Ion Ratio Lower Upper

228 100

229 21.7 22.8 34.2#



226 28.0 17.0 25.6#

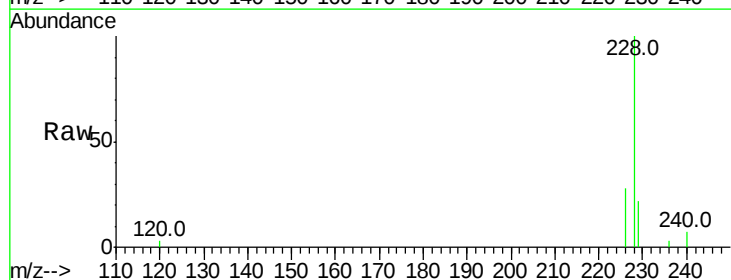


Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

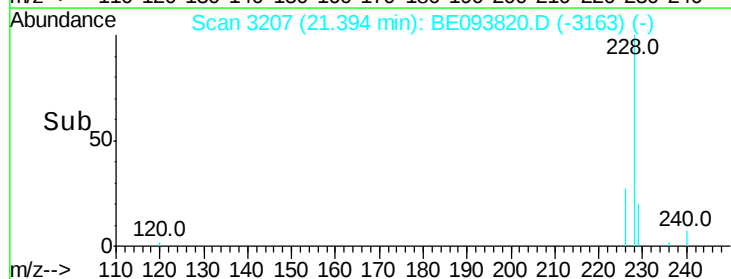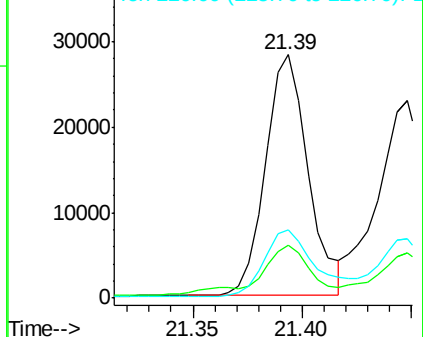

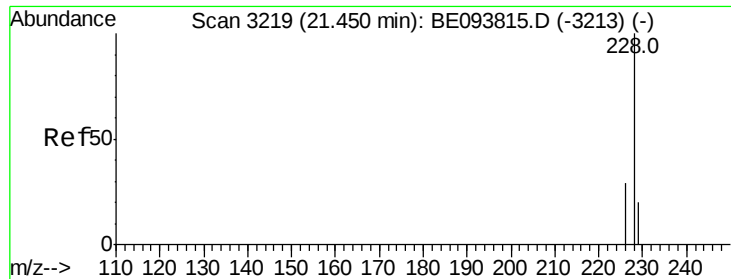

#19

Chrysene

Concen: 0.714 ng/ul

RT: 21.45 min Scan# 3219

Delta R.T. -0.00 min

Lab File: BE093820.D

Acq: 15 Aug 2017 22:52

Instrument :

BNA_E

ClientSampleId :

C0AJ2

Tot Ion:228 Resp: 36646

Ion Ratio Lower Upper

228 100

226 30.0 23.4 35.0

229 22.8 17.7 26.5

