

Data Path : Z:\HPCHEM1\BNA E\DATA\BE081517\
 Data File : BE093830.D
 Acq On : 16 Aug 2017 5:05
 Operator : SJ/JU
 Sample : I4529-11DL 5X
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AA5DL

Quant Time: Aug 16 07:39:14 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 16 07:30:49 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.92	152	2363	0.40	ng/ul	0.00
2) Naphthalene-d8	10.70	136	12562	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.52	164	8197	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.26	188	15988	0.40	ng/ul	0.00
16) Chrysene-d12	21.41	240	16977	0.40	ng/ul	0.00
20) Perylene-d12	23.91	264	17238	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.28	152	1825	0.09	ng/ul	0.00
14) Fluoranthene-d10	19.27	212	5255	0.10	ng/ul	0.00
Target Compounds				Ovalue		
3) Naphthalene	10.75	128	25019	0.819	ng/ul#	93
5) 2-Methylnaphthalene	12.35	142	31561	1.416	ng/ul	100
7) Acenaphthylene	14.24	152	5244	0.153	ng/ul#	65
8) Acenaphthene	14.58	153	7585	0.281	ng/ul	95
9) Fluorene	15.57	166	39407	1.156	ng/ul	92
12) Phenanthrene	17.29	178	93915	2.157	ng/ul#	92
13) Anthracene	17.38	178	23218	0.547	ng/ul#	91
15) Fluoranthene	19.30	202	49573	0.910	ng/ul	83
17) Pyrene	19.66	202	58805	1.187	ng/ul#	83
18) Benzo(a)anthracene	21.39	228	18097	0.368	ng/ul#	81
19) Chrysene	21.45	228	18740	0.397	ng/ul#	82
21) Benzo(b)fluoranthene	23.14	252	19930	0.374	ng/ul	94
22) Benzo(k)fluoranthene	23.14	252	19930	0.379	ng/ul#	92
23) Benzo(a)pyrene	23.80	252	12482	0.246	ng/ul	96
24) Indeno(1,2,3-cd)pyrene	26.55	276	5571	0.099	ng/ul#	83
25) Dibenzo(a,h)anthracene	26.56	278	1420	0.030	ng/ul#	18
26) Benzo(a,h,i)perylene	27.37	276	4302	0.091	ng/ul#	82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE081517\
Data File : BE093830.D
Acq On : 16 Aug 2017 5:05
Operator : SJ/JU
Sample : I4529-11DL 5X
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AA5DL

Quant Time: Aug 16 07:39:14 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 16 07:30:49 2017
Response via : Initial Calibration

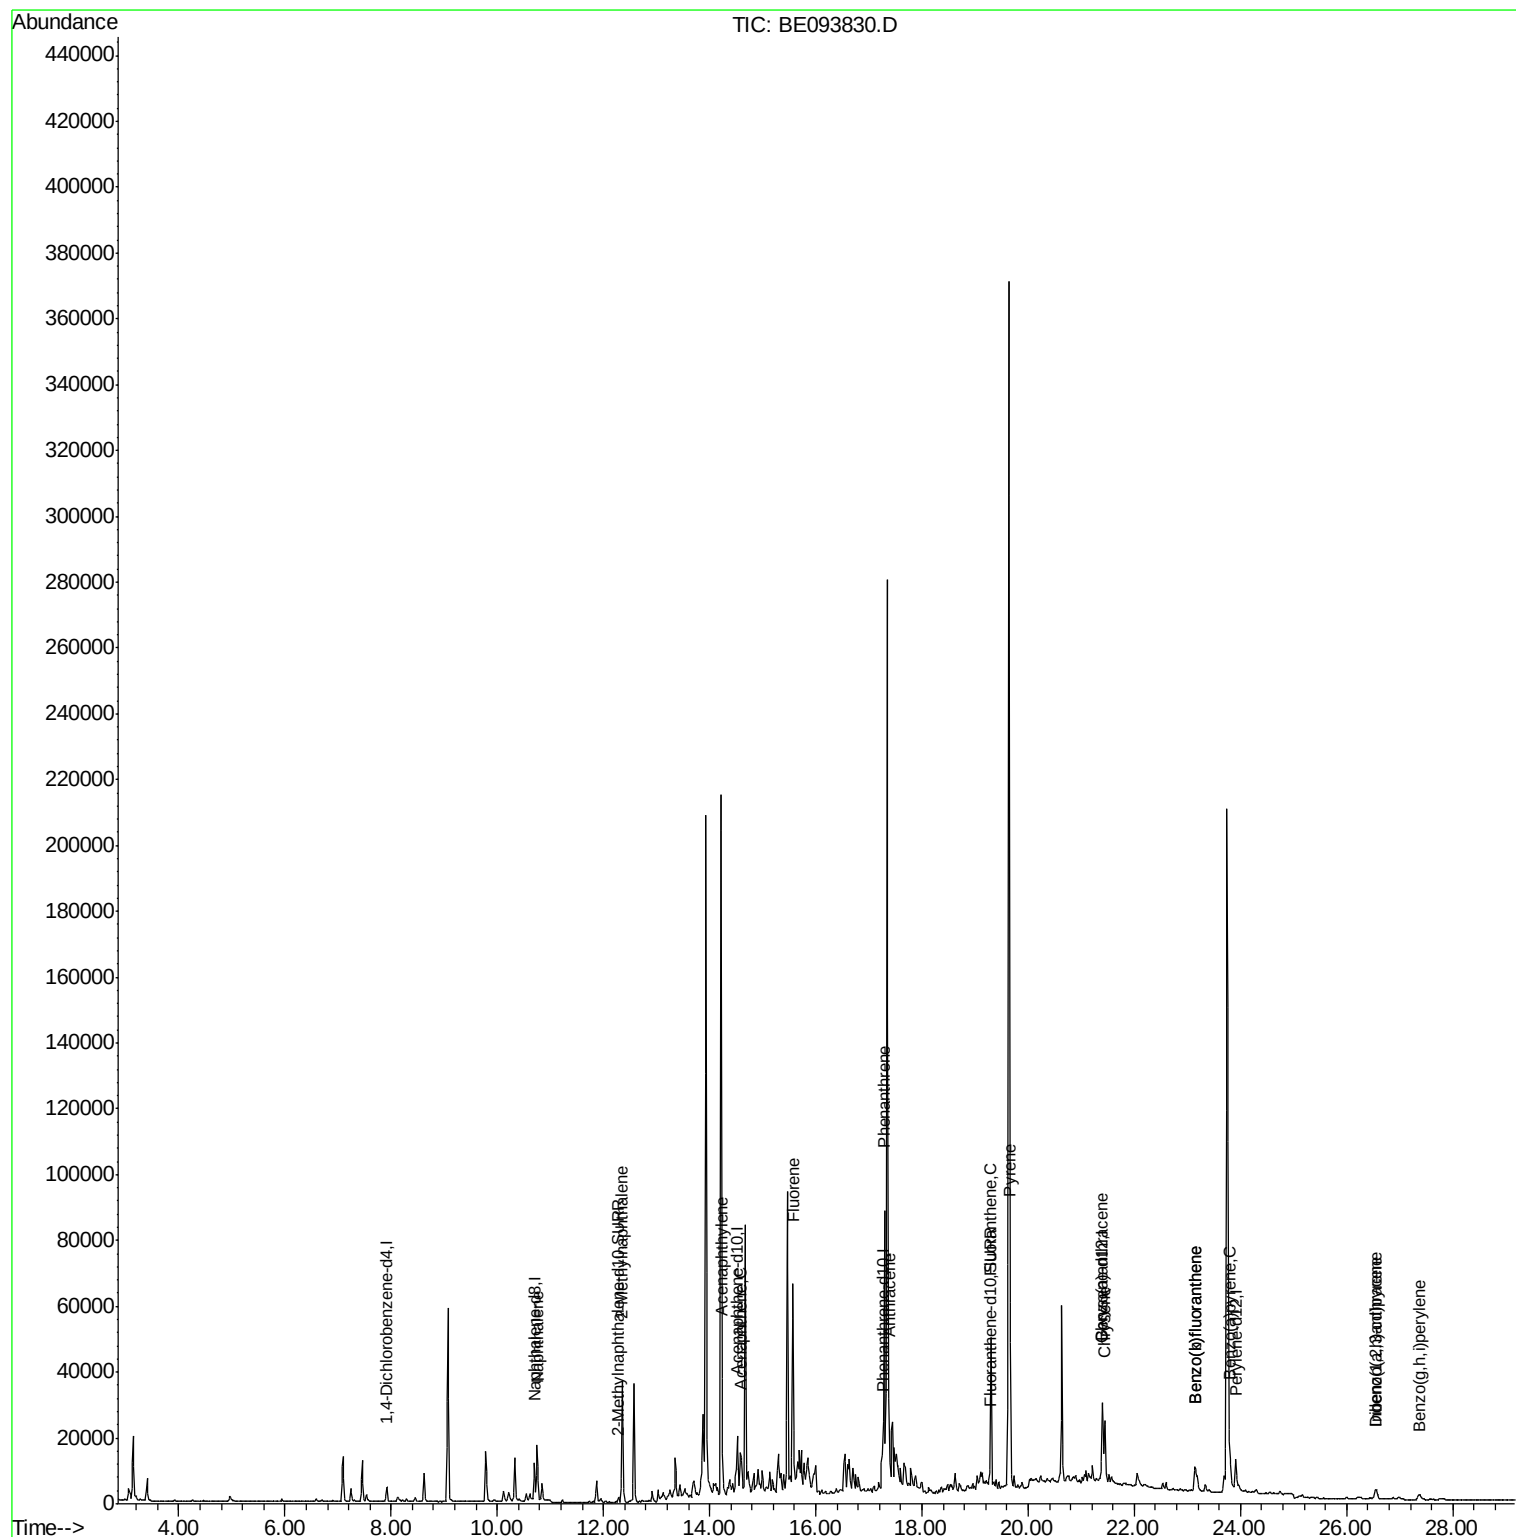



#3

Naphthalene

Concen: 0.819 ng/ul

RT: 10.75 min Scan# 1266

Delta R.T. -0.00 min

Lab File: BE093830.D

Acq: 16 Aug 2017 5:05

Instrument :

BNA_E

ClientSampleId :

C0AA5DL


Tot Ion:128 Resp: 25019

Ion Ratio Lower Upper

128 100

129 12.6 11.3 16.9




127 0.0 4.0 6.0#

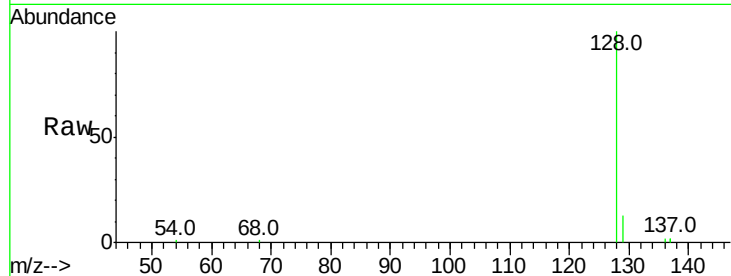

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

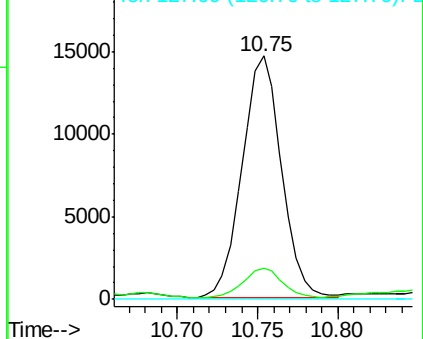

#5

2-Methylnaphthalene

Concen: 1.416 ng/ul

RT: 12.35 min Scan# 1751

Delta R.T. -0.01 min

Lab File: BE093830.D


Acq: 16 Aug 2017 5:05

Tgt Ion:142 Resp: 31561

Ion Ratio Lower Upper



142 100


141 90.4 72.6 108.8



Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

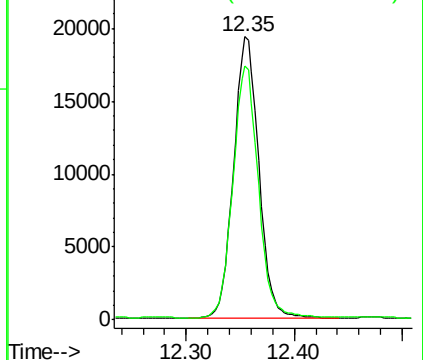



#7

Acenaphthylene

Concen: 0.153 ng/ul

RT: 14.24 min Scan# 2125

Delta R.T. -0.01 min

Lab File: BE093830.D

Acq: 16 Aug 2017 5:05

Instrument :

BNA_E

ClientSampleId :

C0AA5DL





Tot Ion:152 Resp: 5244

Ion Ratio Lower Upper

152 100

151 27.7 17.1 25.7#

153 42.6 12.8 19.2#

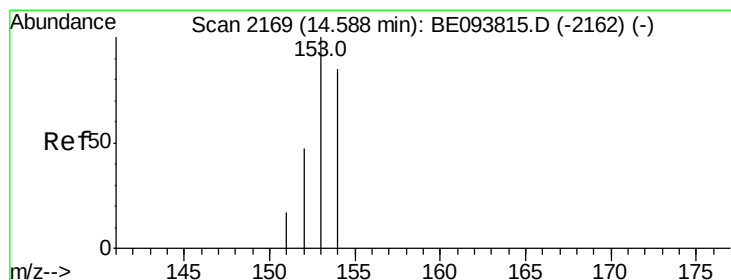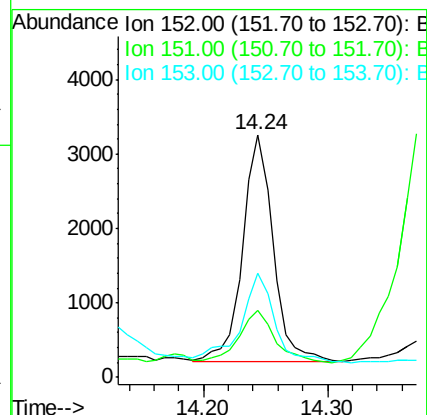

#8

Acenaphthene

Concen: 0.281 ng/ul

RT: 14.58 min Scan# 2170

Delta R.T. -0.01 min

Lab File: BE093830.D

Acq: 16 Aug 2017 5:05




Tgt Ion:153 Resp: 7585


Ion Ratio Lower Upper

153 100

152 52.5 40.3 60.5

154 84.2 71.4 107.2

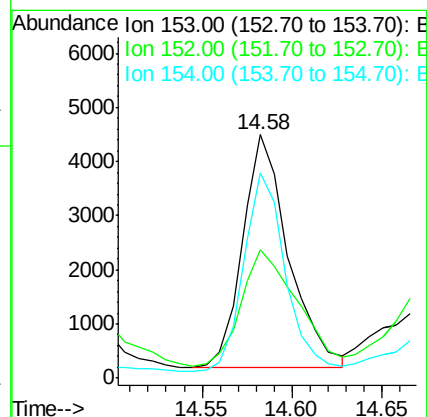



#9

Fluorene

Concen: 1.156 ng/ul

RT: 15.57 min Scan# 2301

Delta R.T. -0.01 min

Lab File: BE093830.D

Acq: 16 Aug 2017 5:05

Instrument :

BNA_E

ClientSampleId :

C0AA5DL





Tot Ion:166 Resp: 39407

Ion Ratio Lower Upper

166 100

165 100.2 73.4 110.2

167 17.0 14.6 22.0

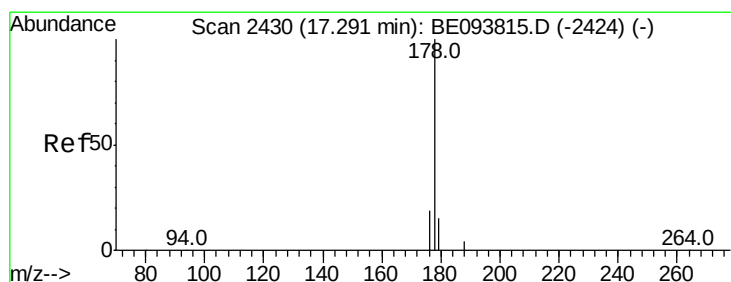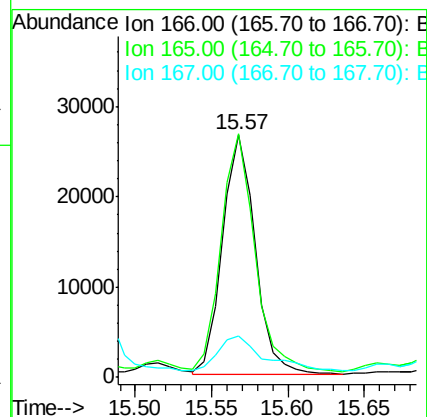

#12

Phenanthrene

Concen: 2.157 ng/ul

RT: 17.29 min Scan# 2432

Delta R.T. 0.00 min

Lab File: BE093830.D

Acq: 16 Aug 2017 5:05




Tgt Ion:178 Resp: 93915


Ion Ratio Lower Upper

178 100

179 17.8 18.4 27.6#

176 19.2 13.6 20.4

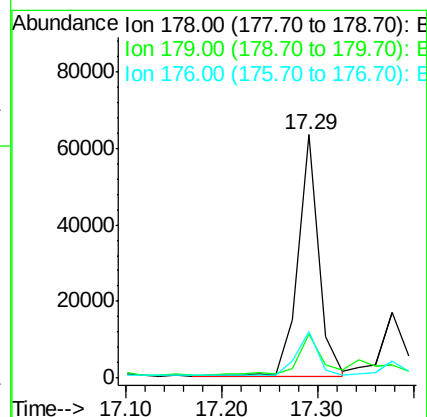



#13

Anthracene

Concen: 0.547 ng/ul

RT: 17.38 min Scan# 2437

Delta R.T. 0.00 min

Lab File: BE093830.D

Acq: 16 Aug 2017 5:05

Instrument :

BNA_E

ClientSampleId :

C0AA5DL


Tot Ion:178 Resp: 23218

Ion Ratio Lower Upper

178 100

179 21.1 18.1 27.1




176 25.5 14.7 22.1#

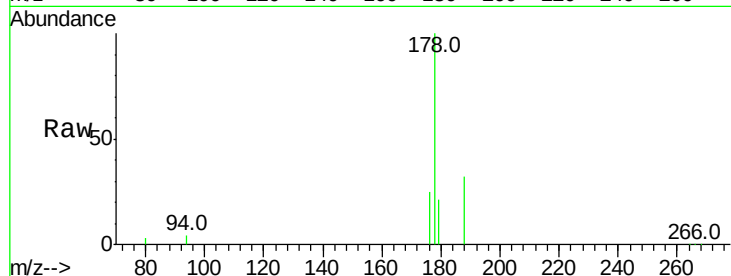

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

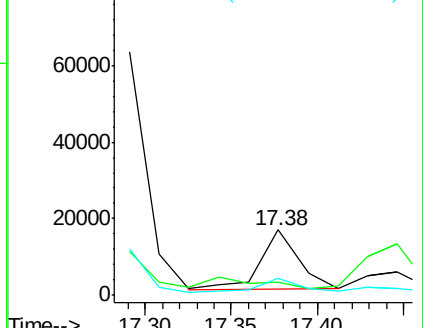

#15

Fluoranthene

Concen: 0.910 ng/ul

RT: 19.30 min Scan# 2753

Delta R.T. -0.00 min

Lab File: BE093830.D

Acq: 16 Aug 2017 5:05


Tgt Ion:202 Resp: 49573

Ion Ratio Lower Upper

202 100

101 12.7 0.0 30.3



100 9.3 0.0 39.5




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): E

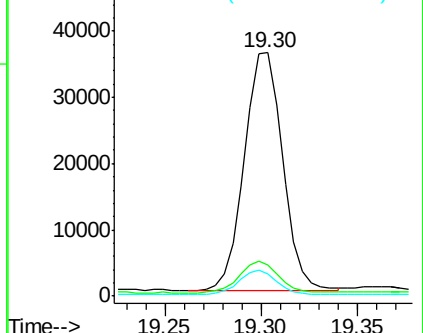



#17

Pvrene

Concen: 1.187 ng/ul

RT: 19.66 min Scan# 2832

Delta R.T. -0.00 min

Lab File: BE093830.D

Acq: 16 Aug 2017 5:05

Instrument :

BNA_E

ClientSampleId :

C0AA5DL


Tot Ion:202 Resp: 58805

Ion Ratio Lower Upper

202 100

101 14.4 18.2 27.4#




100 11.7 15.6 23.4#

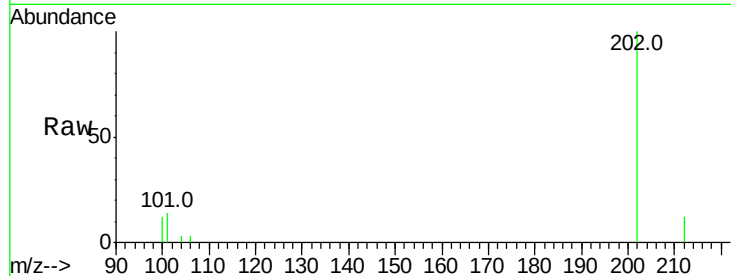

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): E

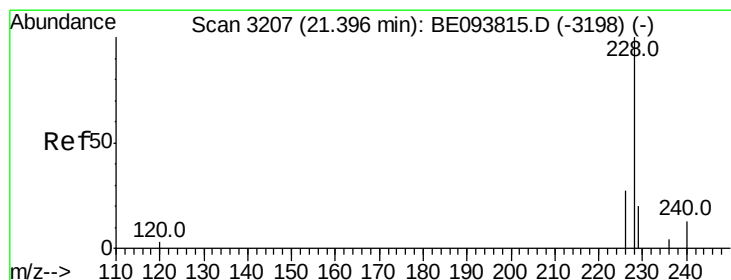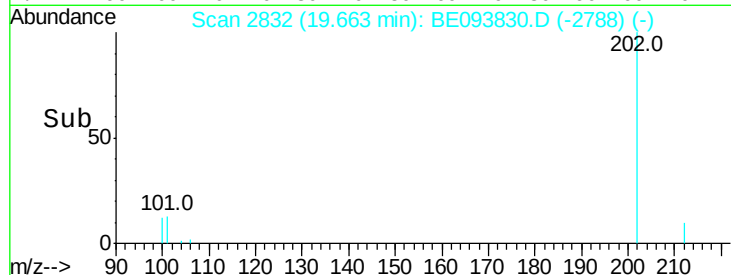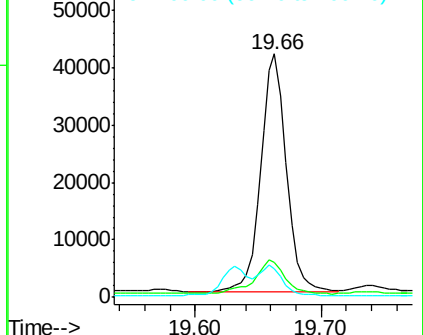

#18

Benzo(a)anthracene

Concen: 0.368 ng/ul

RT: 21.39 min Scan# 3208

Delta R.T. -0.01 min

Lab File: BE093830.D

Acq: 16 Aug 2017 5:05


Tgt Ion:228 Resp: 18097

Ion Ratio Lower Upper

228 100

229 35.1 22.8 34.2#



226 34.5 17.0 25.6#




Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

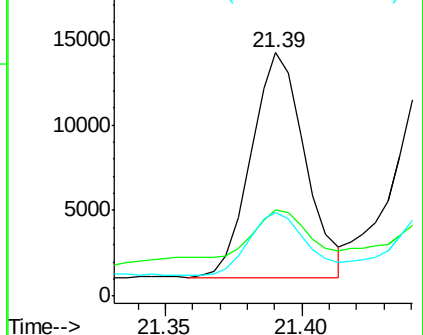



#19

Chrysene

Concen: 0.397 ng/ul

RT: 21.45 min Scan# 3220

Delta R.T. -0.01 min

Lab File: BE093830.D

Acq: 16 Aug 2017 5:05

Instrument :

BNA_E

ClientSampleId :

C0AA5DL


Tot Ion:228 Resp: 18740

Ion Ratio Lower Upper

228 100

226 36.5 23.4 35.0#




229 33.9 17.7 26.5#



Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

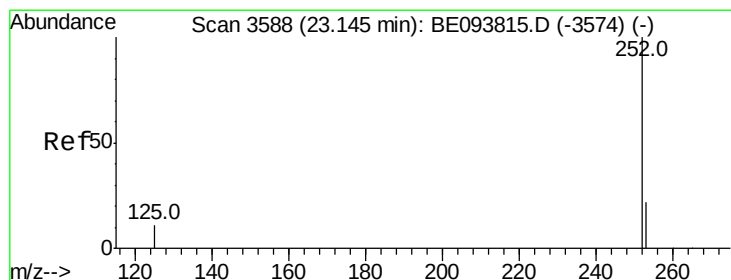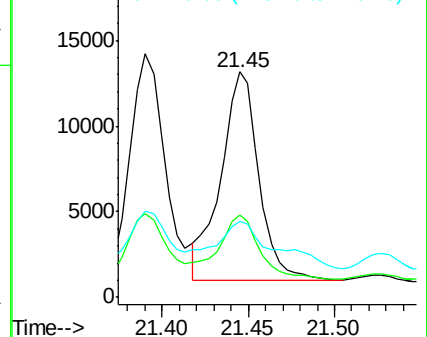

#21

Benzo(b)fluoranthene

Concen: 0.374 ng/ul

RT: 23.14 min Scan# 3590

Delta R.T. -0.00 min

Lab File: BE093830.D

Acq: 16 Aug 2017 5:05


Tgt Ion:252 Resp: 19930

Ion Ratio Lower Upper

252 100

253 33.4 0.0 64.2



125 23.0 0.0 35.0

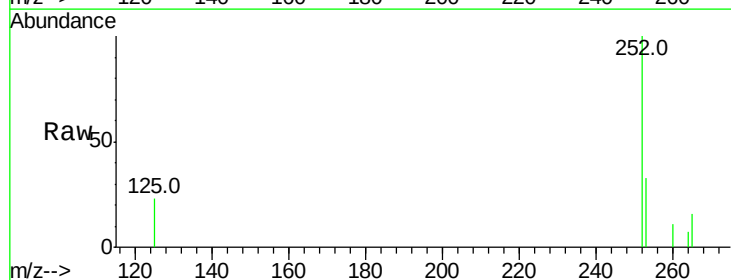


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

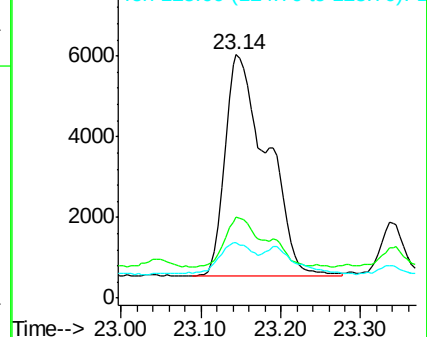



#22

Benzo(k)fluoranthene

Concen: 0.379 ng/ul

RT: 23.14 min Scan# 3590

Delta R.T. -0.05 min

Lab File: BE093830.D

Acq: 16 Aug 2017 5:05

Instrument :

BNA_E

ClientSampleId :

C0AA5DL





Tot Ion:252 Resp: 19930

Ion Ratio Lower Upper

252 100

253 33.4 24.5 36.7

125 23.0 13.7 20.5#

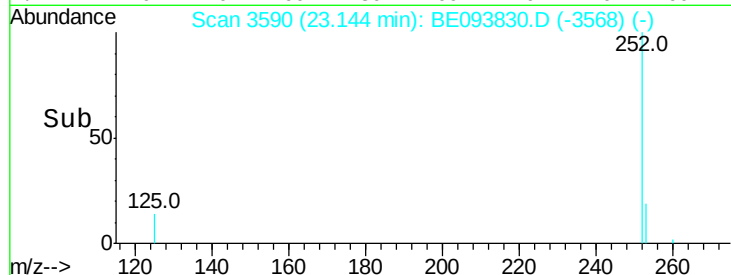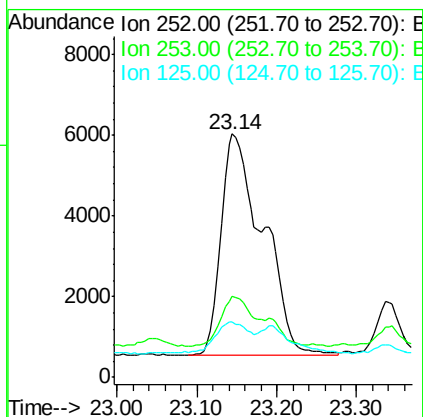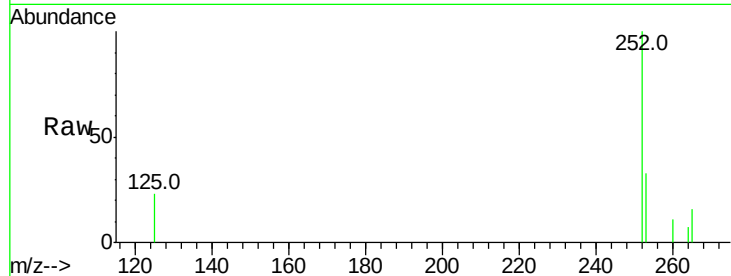

#23

Benzo(a)pyrene

Concen: 0.246 ng/ul

RT: 23.80 min Scan# 3734

Delta R.T. -0.00 min

Lab File: BE093830.D

Acq: 16 Aug 2017 5:05




Tgt Ion:252 Resp: 12482


Ion Ratio Lower Upper

252 100

253 32.1 28.5 42.7

125 23.0 18.1 27.1

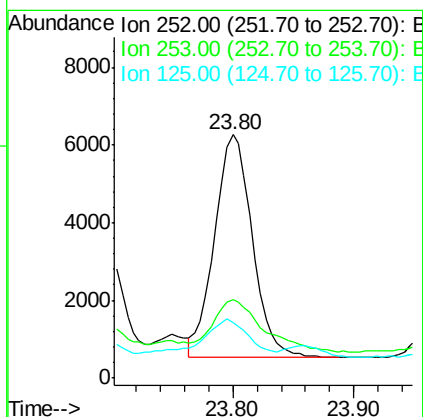







#24

Indeno(1,2,3-cd)pyrene
Concen: 0.099 ng/ul
RT: 26.55 min Scan# 4334
Delta R.T. -0.02 min
Lab File: BE093830.D
Acq: 16 Aug 2017 5:05

Instrument :
BNA_E
ClientSampleId :
C0AA5DL




Tot Ion:276 Resp: 5571
Ion Ratio Lower Upper
276 100
138 27.1 28.0 42.0#
227 0.0 8.0 12.0#

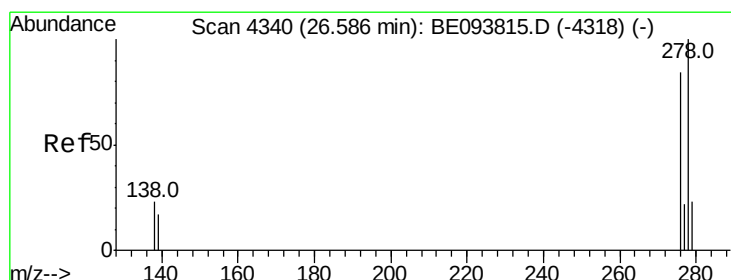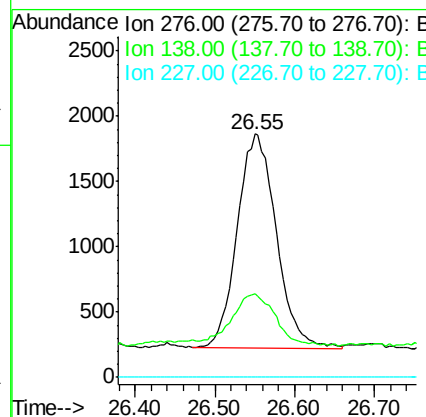


#25

Dibenzo(a,h)anthracene
Concen: 0.030 ng/ul
RT: 26.56 min Scan# 4337
Delta R.T. -0.02 min
Lab File: BE093830.D
Acq: 16 Aug 2017 5:05

Tgt Ion:278 Resp: 1420
Ion Ratio Lower Upper
278 100
139 74.9 17.4 26.0#
279 66.8 25.9 38.9#

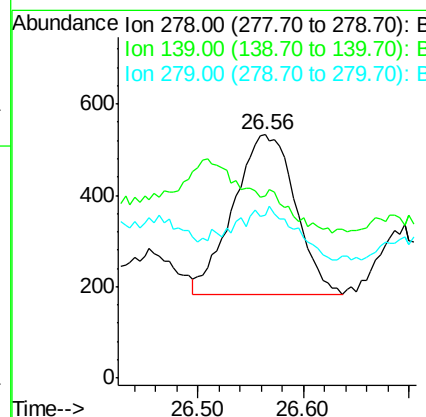

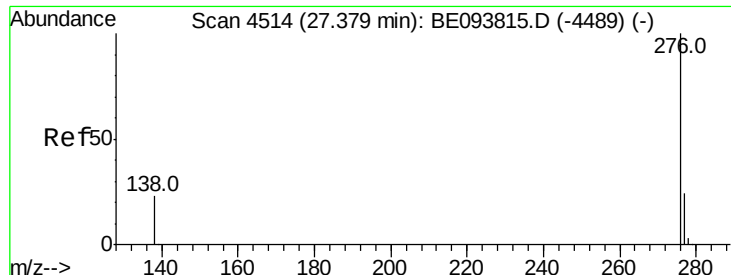

#26

Benzo(a,h,i)perylene

Concen: 0.091 ng/ul

RT: 27.37 min Scan# 4513

Delta R.T. -0.01 min

Lab File: BE093830.D

Acq: 16 Aug 2017 5:05

Instrument :

BNA_E

ClientSampleId :

C0AA5DL


Tot Ion:276 Resp: 4302

Ion Ratio Lower Upper

276 100

138 36.4 21.8 32.8#

277 34.5 20.5 30.7#

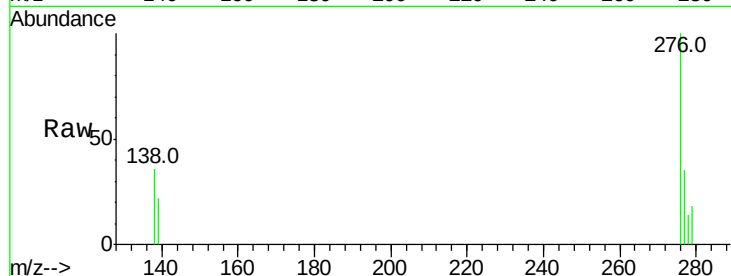

Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

