

Quantitation Report (QT Reviewed)


Data Path : Z:\HPCHEM1\BNA E\DATA\BE081517\
 Data File : BE093803.D
 Acq On : 15 Aug 2017 12:19
 Operator : SJ/JU
 Sample : FB101423BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 SBLK23

Manual Integrations
 APPROVED

Sohil
 8/16/2017 6:42:37 PM

Quant Time: Aug 16 06:45:34 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 16 05:35:21 2017
 Response via : Initial Calibration

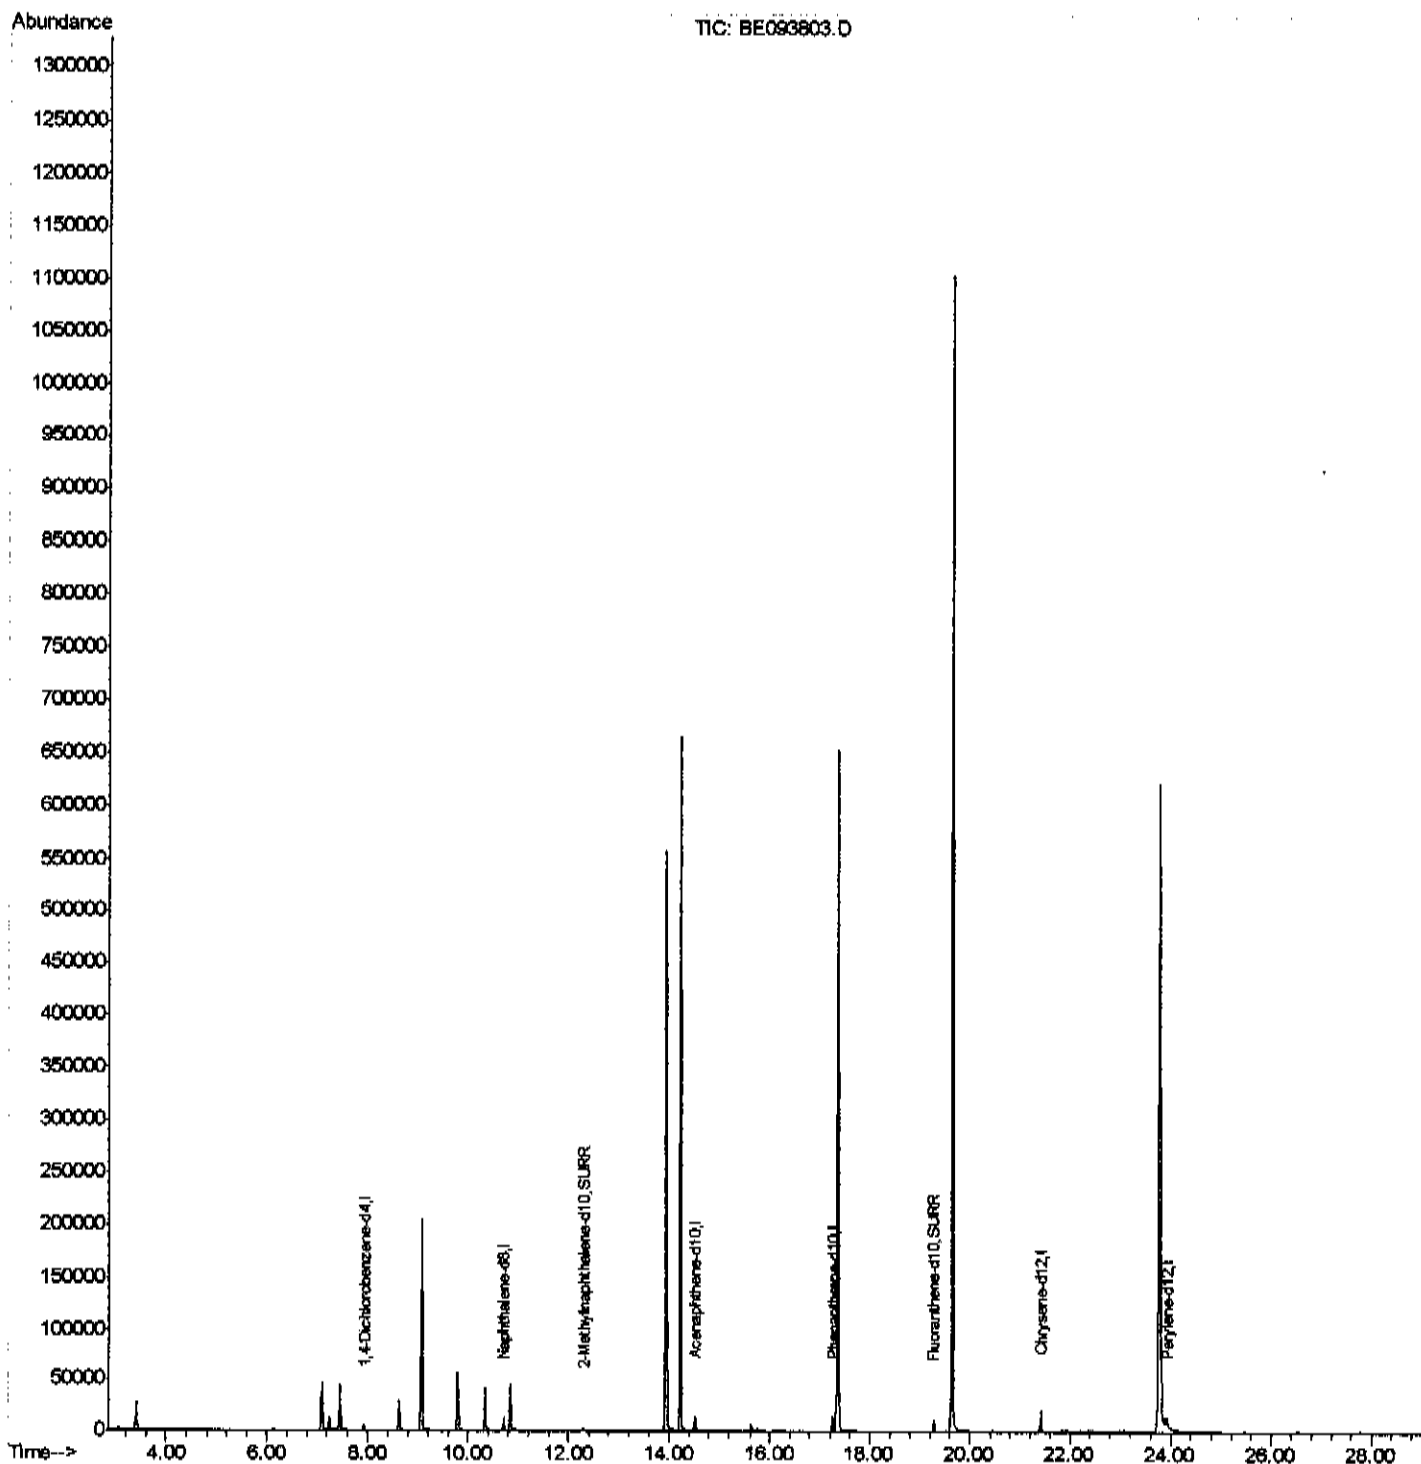

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA E\DATA\BE081517\
 Data File : BE093803.D
 Acq On : 15 Aug 2017 12:19
 Operator : SJ/JU
 Sample : PB101423BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 SBLK23

Manual Integrations
 APPROVED

Sohil
 8/16/2017 6:42:37 PM

Quant Time: Aug 16 05:44:29 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 16 05:35:21 2017
 Response via : Initial Calibration

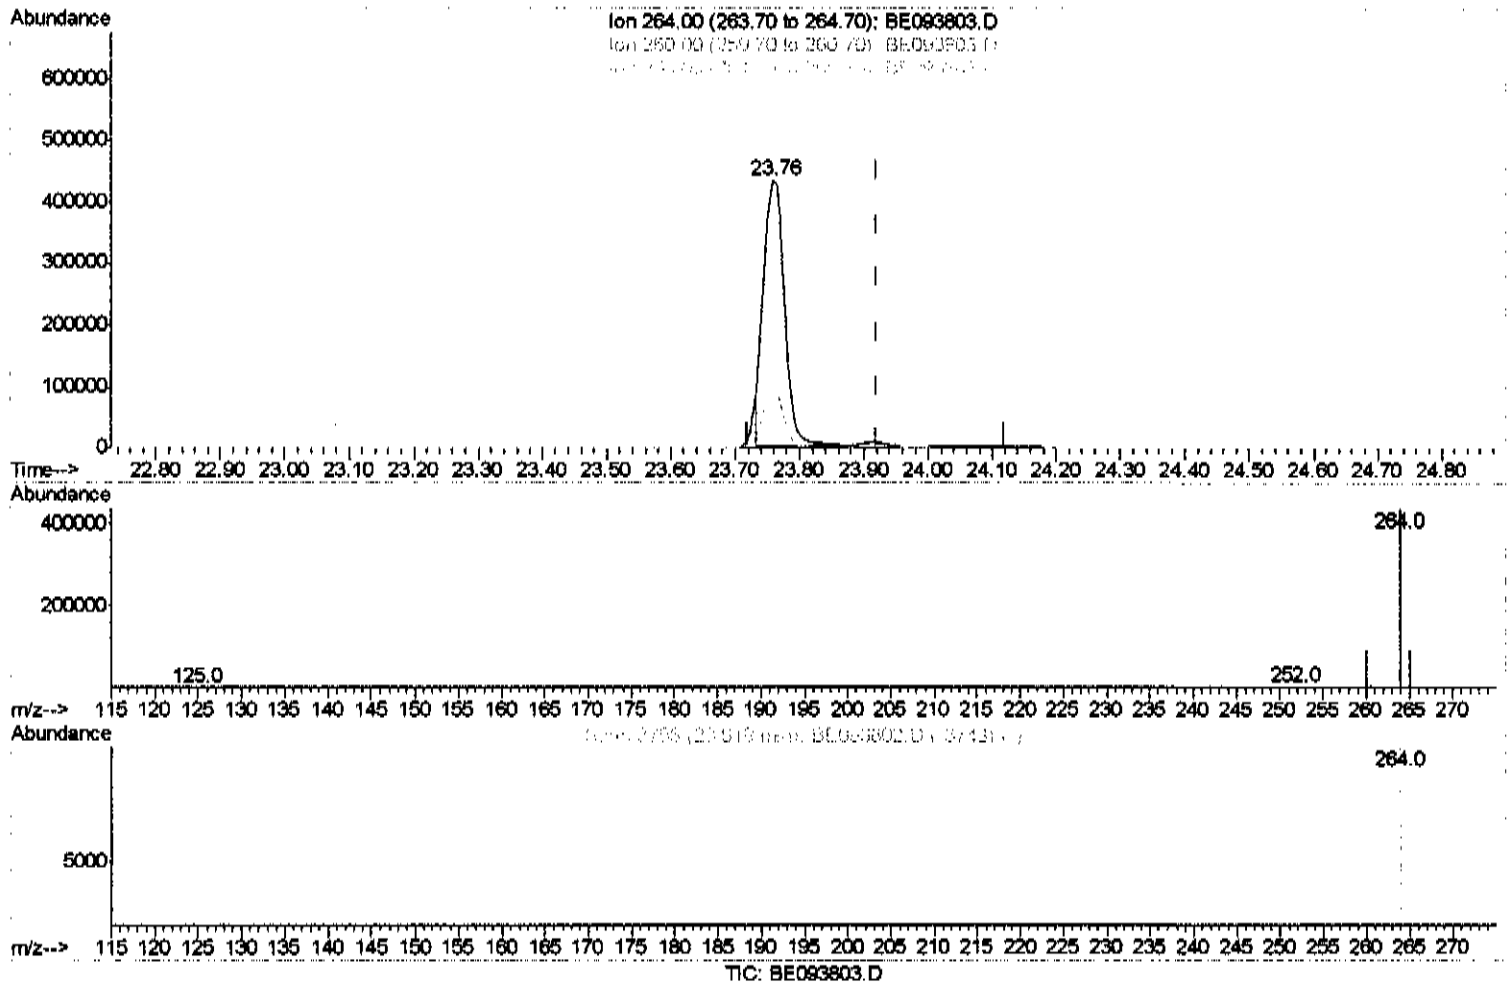

(20) Perylene-d12 (I)

23.759min (-0.160) 0.40ng/ul

response 980625

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.09%
265.00	103.50	21.50%
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE081517\
 Data File : BE093803.D
 Acq On : 15 Aug 2017 12:19
 Operator : SJ/JU
 Sample : PB101423BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 SBLK23

Manual Integrations
 APPROVED

Sohil
 8/16/2017 6:42:37 PM

Quant Time: Aug 16 05:44:29 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 16 05:35:21 2017
 Response via : Initial Calibration

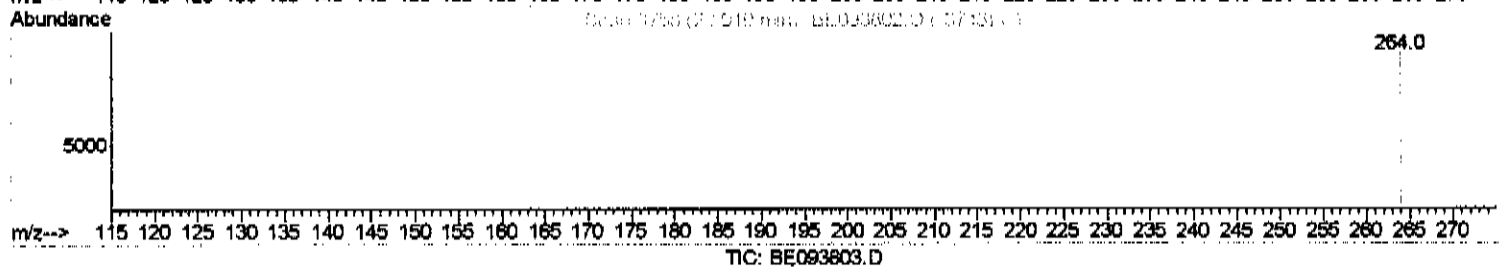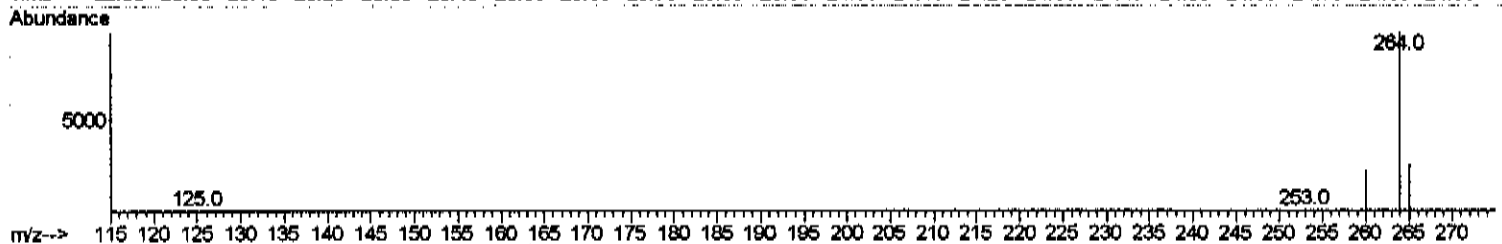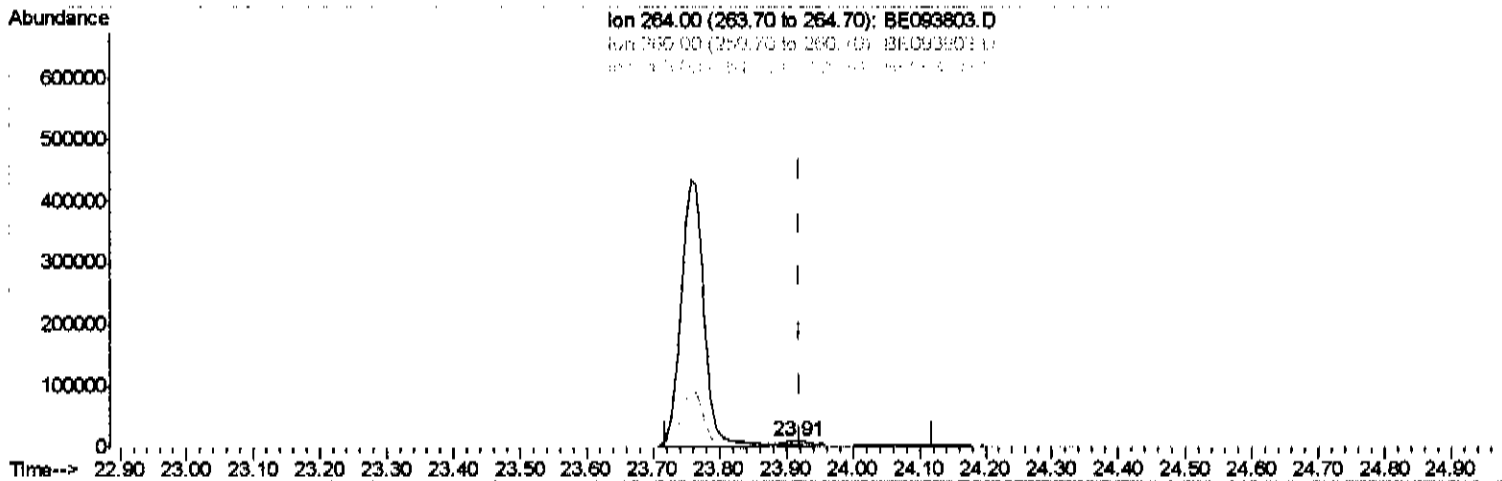

(20) Perylene-d12 (I)

23.914min (-0.005) 0.40ng/ul m

response 12930

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	24.23
265.00	103.50	27.36#
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Instrument :
BNA_E
ClientSampleId :
SBLK23

Manual Integrations
APPROVED

Sohil
8/16/2017 6:42:37 PM

Data Path : Z:\HPCHEM1\BNA E\DATA\BE081517\
Data File : BE093803.D
Acq On : 15 Aug 2017 12:19
Operator : SJ/JU
Sample : PB101423BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Aug 16 06:45:34 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 16 05:35:21 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.92	152	2647	0.40	ng/ul	0.00
2) Naphthalene-d8	10.71	136	13657	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.52	164	7995	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.26	188	17203	0.40	ng/ul	0.00
16) Chrysene-d12	21.41	240	18500	0.40	ng/ul	0.00
20) Perylene-d12	23.91	264	12930m	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.29	152	5500	0.25	ng/ul	0.00
14) Fluoranthene-d10	19.28	212	12841	0.24	ng/ul	0.00

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Handwritten signature: 8/17/17