

Quantitation Report (QT Reviewed)


Data Path : Z:\HPCHEM1\BNA E\DATA\BE081517\
 Data File : BE093813.D
 Acq On : 15 Aug 2017 18:32
 Operator : SJ/JU
 Sample : I4673-13
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 C0AK4

Manual Integrations
 APPROVED

Sohil
 8/16/2017 6:42:07 PM

Quant Time: Aug 16 07:26:14 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 16 05:35:21 2017
 Response via : Initial Calibration

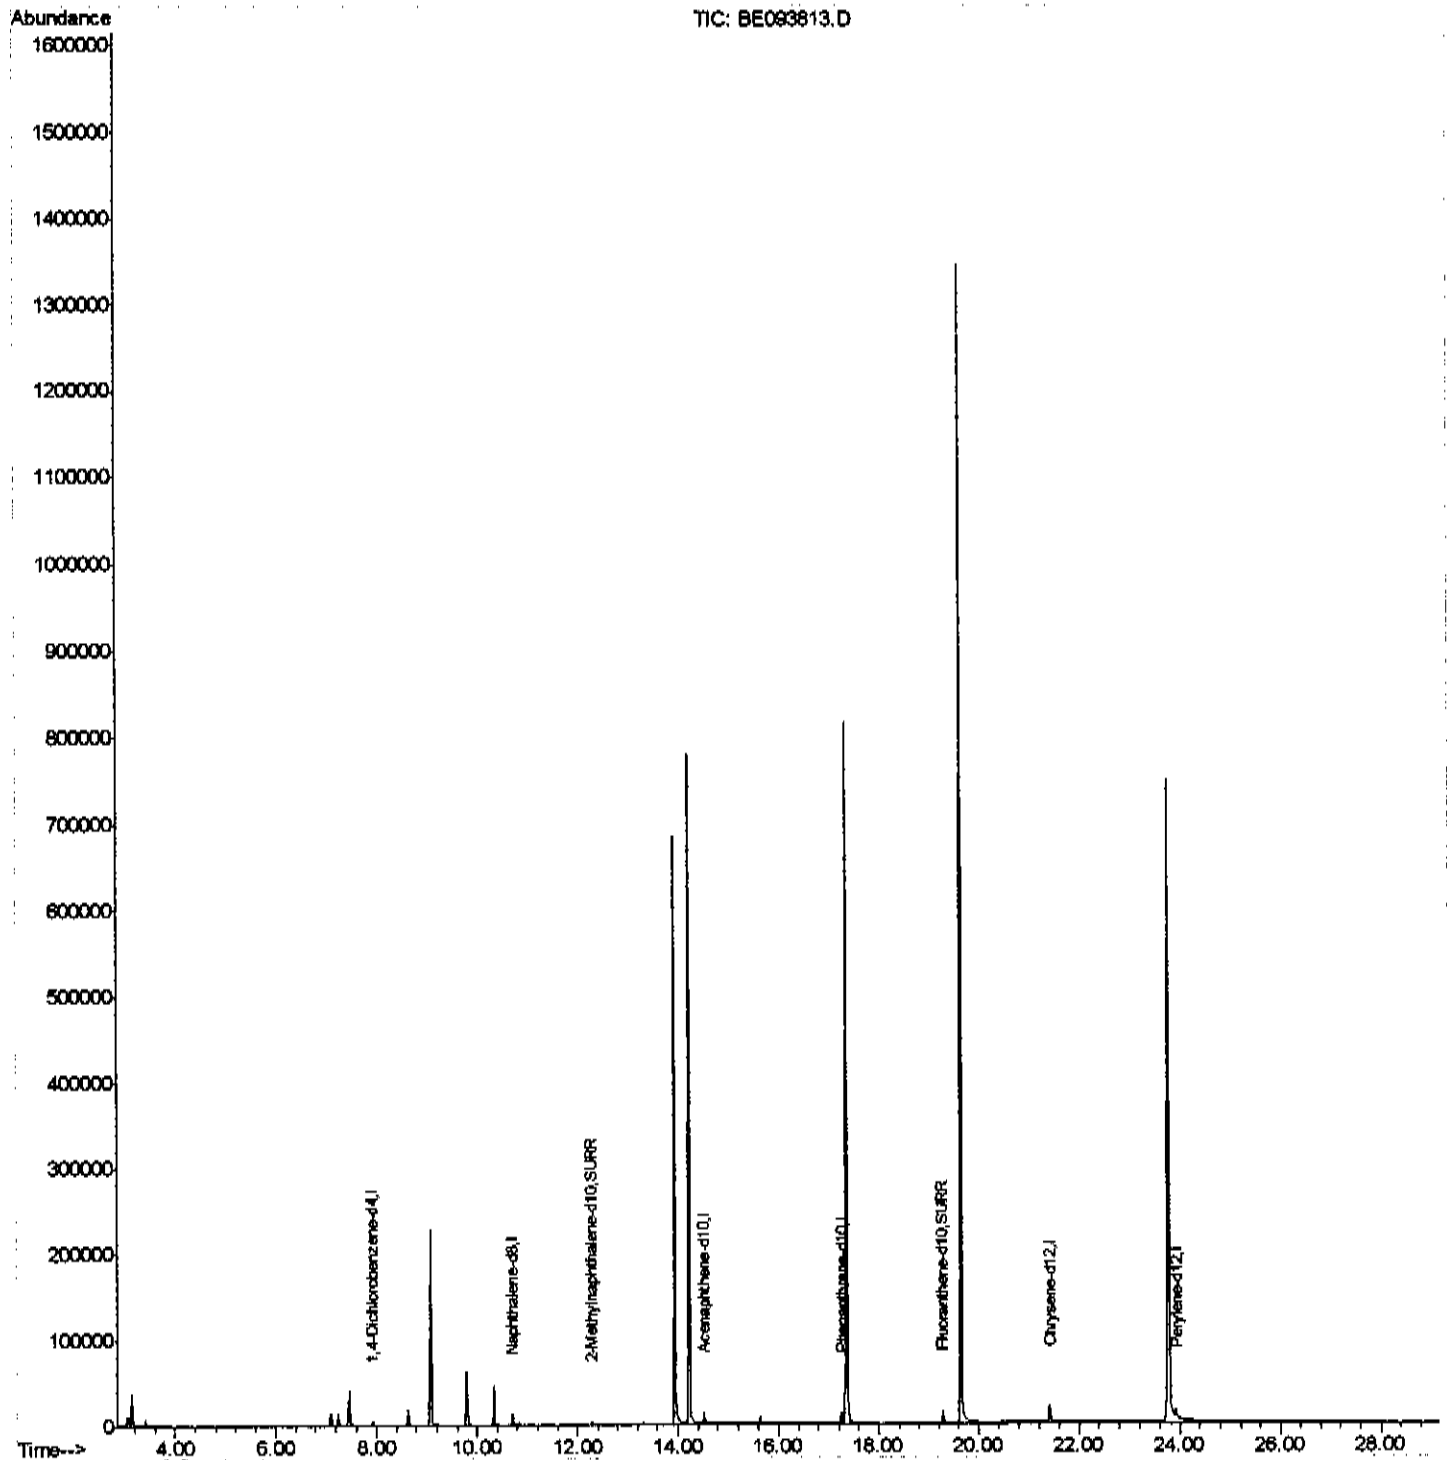

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA E\DATA\BE081517\
 Data File : BE093813.D
 Acq On : 15 Aug 2017 18:32
 Operator : SJ/JU
 Sample : I4673-13
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 C0AK4

Manual Integrations
 APPROVED

Sohil
 8/16/2017 6:42:07 PM

Quant Time: Aug 16 05:46:39 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 16 05:35:21 2017
 Response via : Initial Calibration

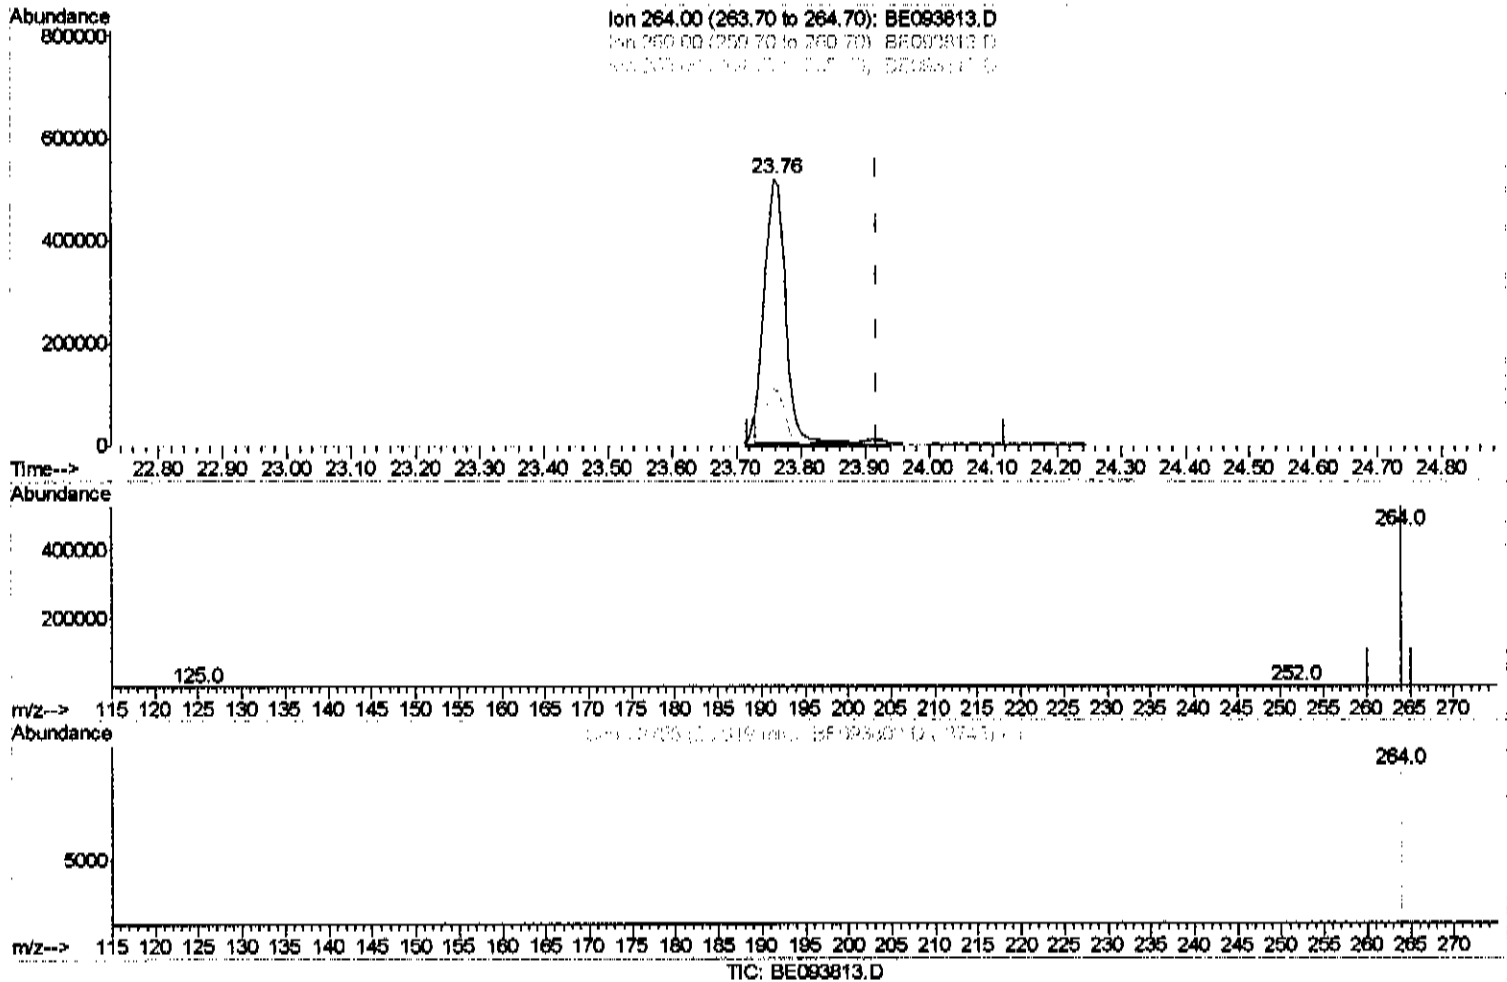

(20) Perylene-d12 (I)

23.760min (-0.160) 0.40ng/ul

response 1140673

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.26#
265.00	103.50	21.74#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA E\DATA\BE081517\
 Data File : BE093813.D
 Acq On : 15 Aug 2017 18:32
 Operator : SJ/JU
 Sample : I4673-13
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AK4

Manual Integrations
 APPROVED

Sohil
 8/16/2017 6:42:07 PM

Quant Time: Aug 16 05:46:39 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 16 05:35:21 2017
 Response via : Initial Calibration

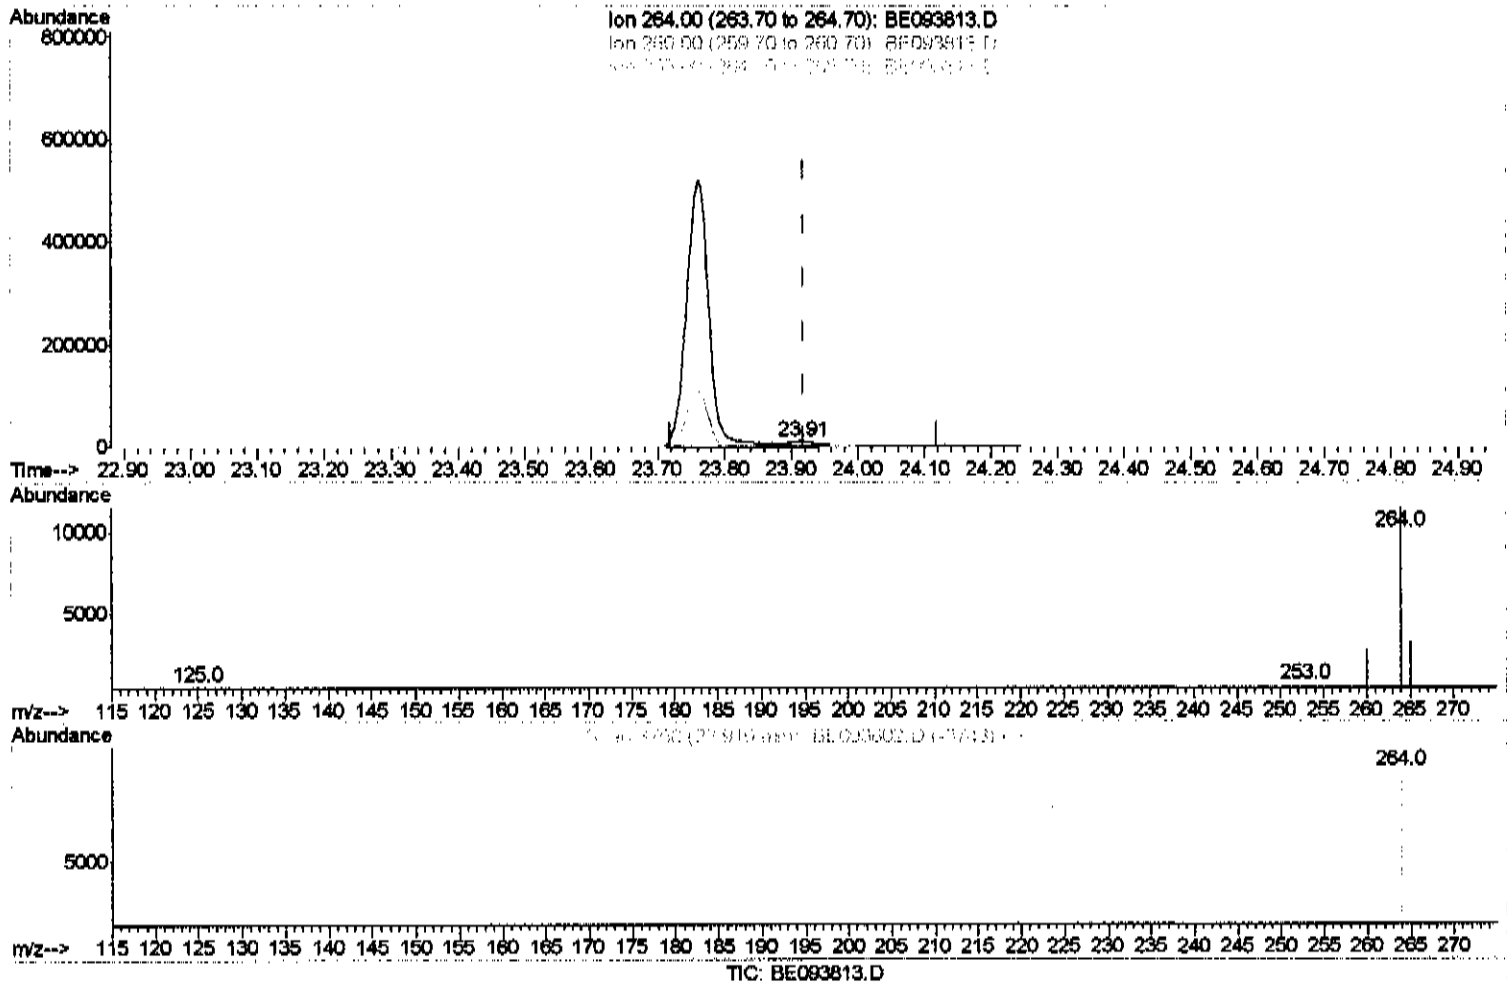

(20) Perylene-d12 (I)

23.914min (-0.005) 0.40ng/ul m

response 23565

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	23.59#
265.00	103.50	27.27#
0.00	0.00	0.00

SJ
 8/17/17

Quantitation Report (QT Reviewed)

Instrument :
BNA_E
ClientSampled :
C0AK4

Manual Integrations
APPROVED

Sohil
8/16/2017 6:42:07 PM

Data Path : Z:\HPCHEM1\BNA E\DATA\BE081517\
Data File : BE093813.D
Acq On : 15 Aug 2017 18:32
Operator : SJ/JU
Sample : I4673-13
Misc :
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Aug 16 07:26:14 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE072417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
OLast Update : Wed Aug 16 05:35:21 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.92	152	2699	0.40	ng/ul	0.00
2) Naphthalene-d8	10.70	136	14207	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.52	164	8244	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.26	188	18422	0.40	ng/ul	0.00
16) Chrysene-d12	21.41	240	19159	0.40	ng/ul	0.00
20) Perylene-d12	23.91	264	23565m	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.29	152	6441	0.28	ng/ul	0.00
14) Fluoranthene-d10	19.27	212	17173	0.30	ng/ul	0.00

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

JUL 8/17/17