


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE081715\
 Data File : BE090531.D
 Acq On : 17 Aug 2015 13:00
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE081415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 14 16:52:42 2015

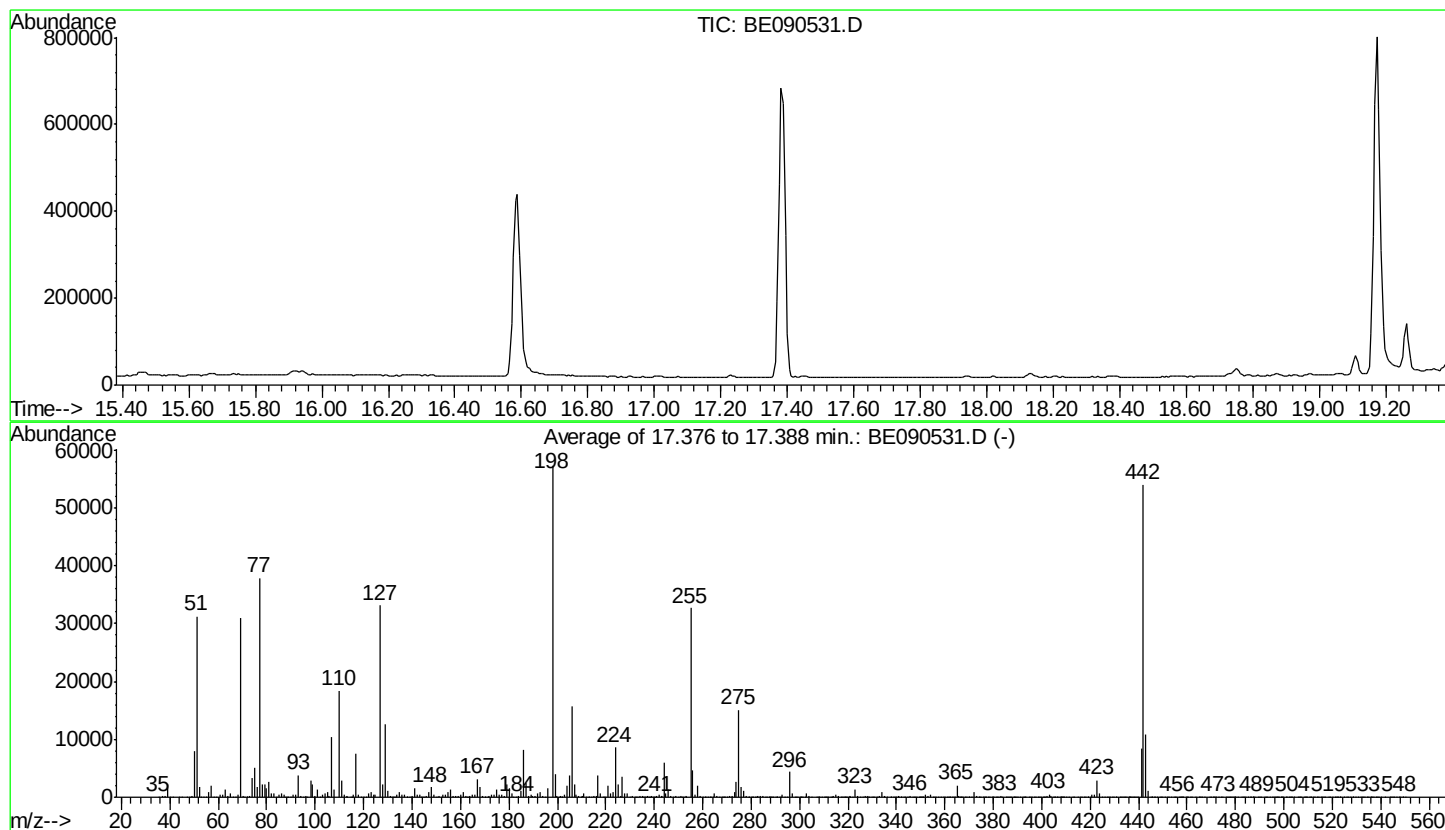

AutoFind: Scans 2517, 2518, 2519; Background Corrected with Scan 2509

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.5	31226	PASS
68	69	0.00	2	1.1	344	PASS
69	198	0.00	100	53.9	30864	PASS
70	69	0.00	2	0.4	124	PASS
127	198	10	80	57.8	33112	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	57268	PASS
199	198	5	9	6.9	3929	PASS
275	198	10	60	26.3	15067	PASS
365	198	1	100	3.5	2014	PASS
441	442	0.01	24	15.6	8428	PASS
442	198	50	100	94.3	54024	PASS
443	442	15	24	20.1	10851	PASS