


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE081715\
Data File : BE090547.D
Acq On : 17 Aug 2015 23:45
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE081415.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Aug 14 16:52:42 2015

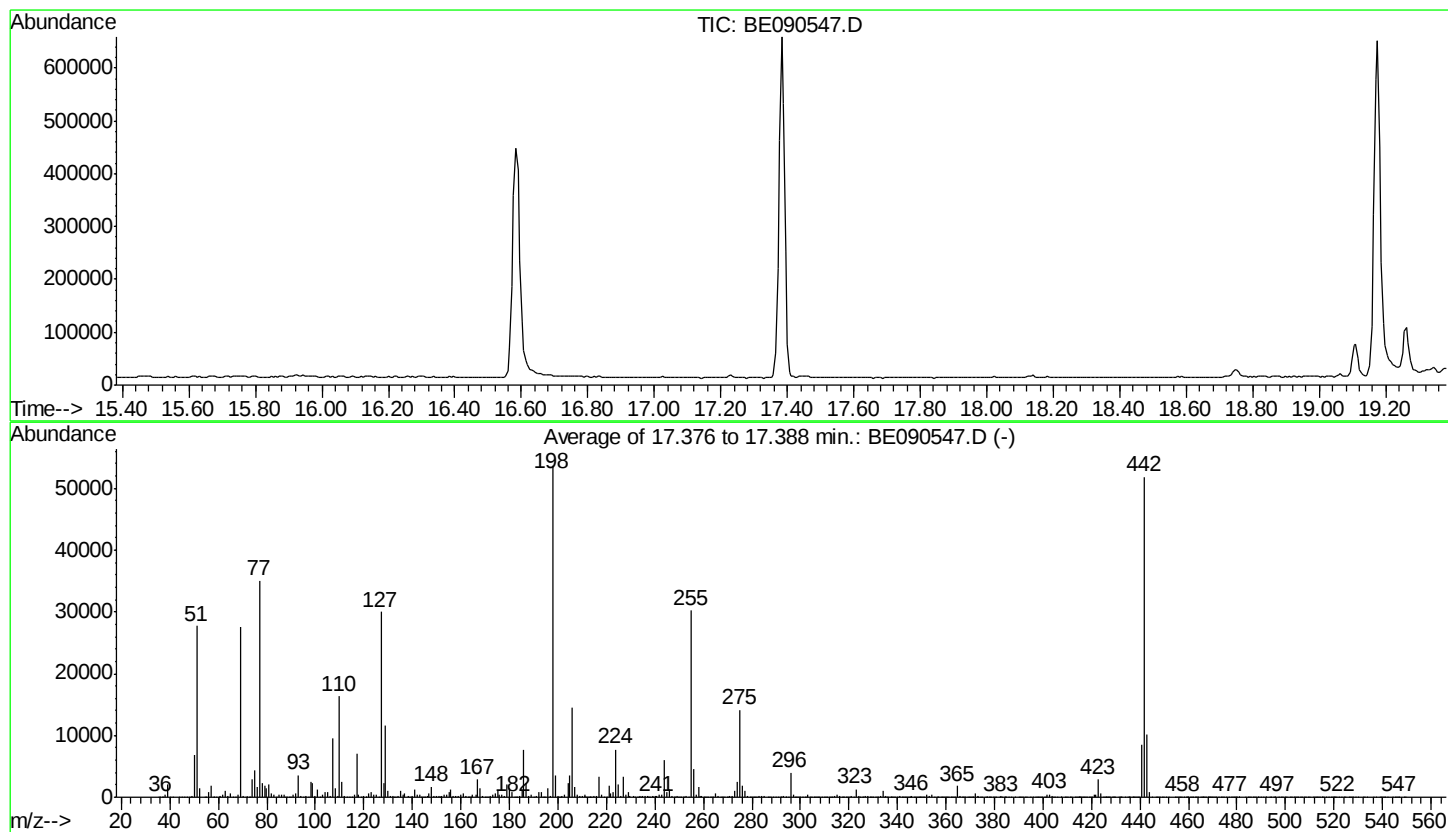

AutoFind: Scans 2517, 2518, 2519; Background Corrected with Scan 2509

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.7	27742	PASS
68	69	0.00	2	1.7	477	PASS
69	198	0.00	100	51.3	27535	PASS
70	69	0.00	2	0.9	257	PASS
127	198	10	80	56.0	30040	PASS
197	198	0.00	2	0.3	138	PASS
198	198	100	100	100.0	53680	PASS
199	198	5	9	6.5	3485	PASS
275	198	10	60	26.3	14094	PASS
365	198	1	100	3.4	1826	PASS
441	442	0.01	24	16.5	8568	PASS
442	198	50	100	96.6	51874	PASS
443	442	15	24	19.4	10078	PASS